

Data Path : Z:\HPCHEM1\BNA F\DATA\BF042817\
 Data File : BF094695.D
 Acq On : 28 Apr 2017 20:31
 Operator : SJ/MA
 Sample : I2895-13
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Apr 28 23:06:55 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF041717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 17 14:59:23 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	5.77	152	112304	20.00	ng	0.00
21) Naphthalene-d8	7.26	136	426903	20.00	ng	0.00
38) Acenaphthene-d10	9.40	164	172410	20.00	ng	0.00
63) Phenanthrene-d10	11.22	188	267071	20.00	ng	0.00
75) Chrysene-d12	14.47	240	225223	20.00	ng	0.00
86) Perylene-d12	16.10	264	171670	20.00	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	4.33	112	824419	121.79	ng	0.03
7) Phenol-d6	5.40	99	989721	124.02	ng	0.00
23) Nitrobenzene-d5	6.42	82	576205	83.34	ng	0.00
41) 2,4,6-Tribromophenol	10.37	330	149073	110.54	ng	0.00
44) 2-Fluorobiphenyl	8.58	172	799922	68.26	ng	0.00
78) Terphenyl-d14	13.19	244	469129	55.68	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	6.42	70	75662	14.31	ng	# 75
49) Dimethylphthalate	9.08	163	94209	7.33	ng	99
56) 2,4-Dinitrotoluene	9.40	165	22155	6.26	ng	# 31


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF042817\
Data File : BF094695.D
Acq On : 28 Apr 2017 20:31
Operator : SJ/MA
Sample : I2895-13
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Apr 28 23:06:55 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF041717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 17 14:59:23 2017
Response via : Initial Calibration

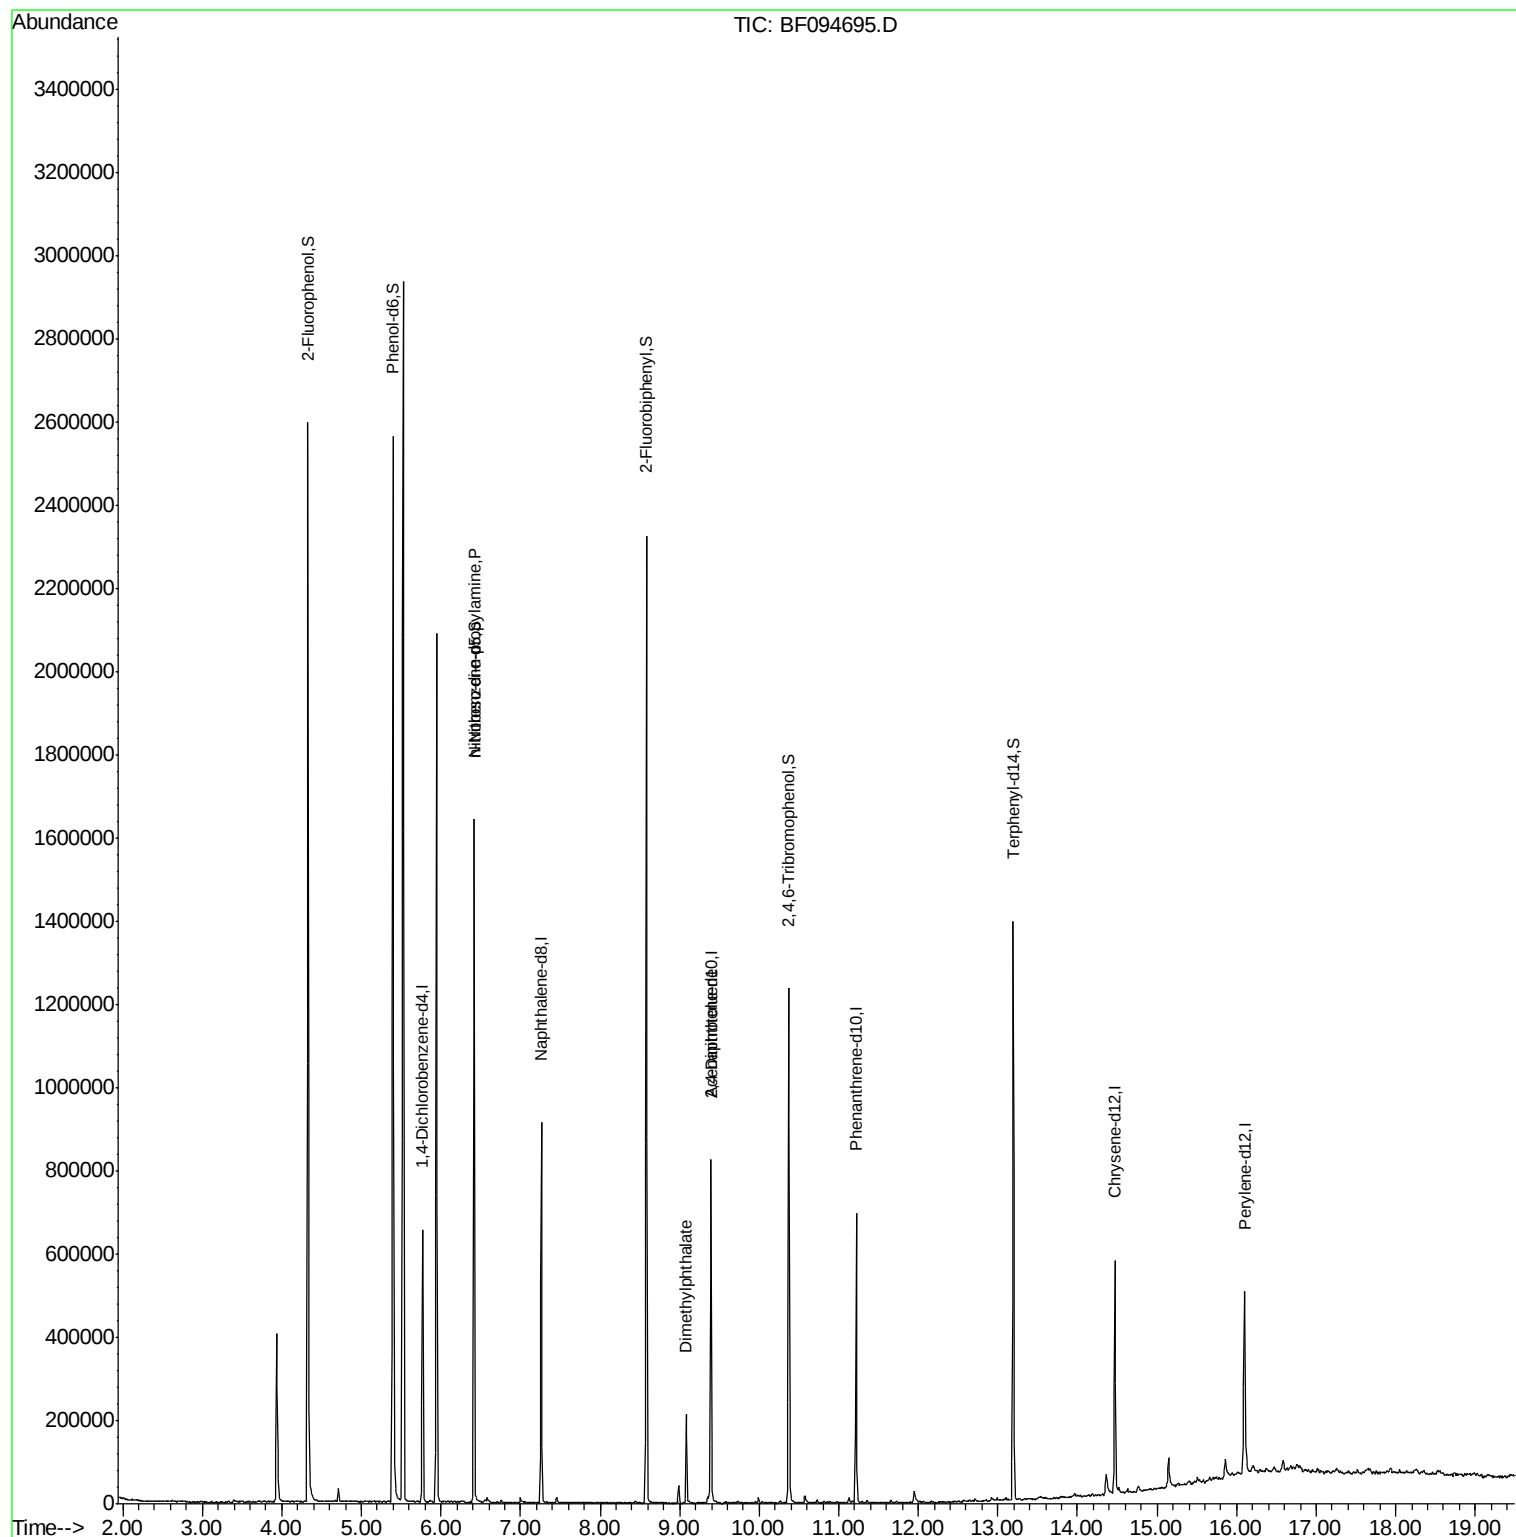

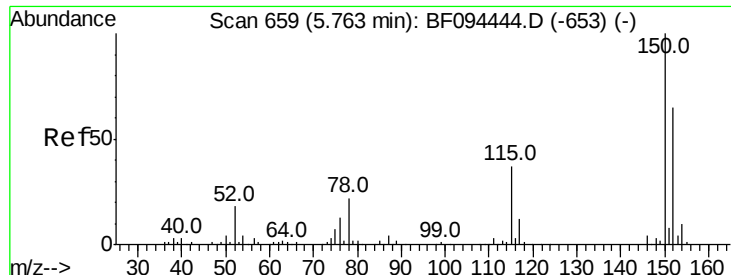


#1



1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 5.77 min Scan# 652
Delta R.T. 0.01 min
Lab File: BF094695.D
Acq: 28 Apr 2017 20:31

Instrument :
BNA_F
ClientSampleId :

Tot Ion:152 Resp: 112304
Ion Ratio Lower Upper
152 100
150 152.2 126.2 189.2
115 56.5 52.2 78.2

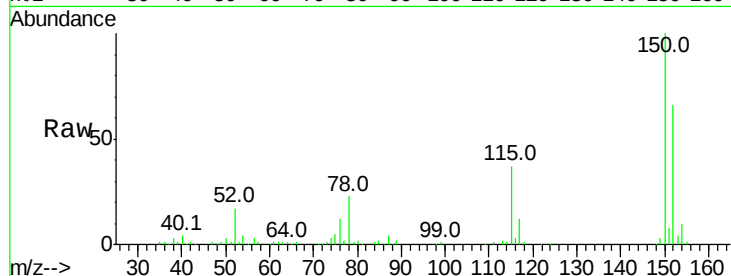


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

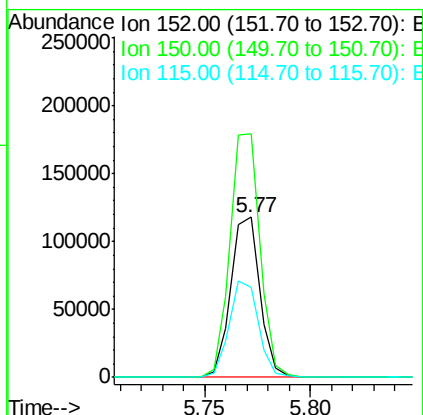



#5




2-Fluorophenol
Concen: 121.79 ng
RT: 4.33 min Scan# 407
Delta R.T. 0.03 min
Lab File: BF094695.D
Acq: 28 Apr 2017 20:31

Tgt Ion:112 Resp: 824419
Ion Ratio Lower Upper
112 100
64 54.2 46.0 69.0
63 27.6 23.4 35.0



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

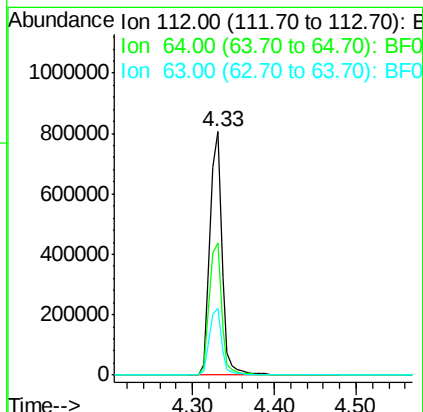

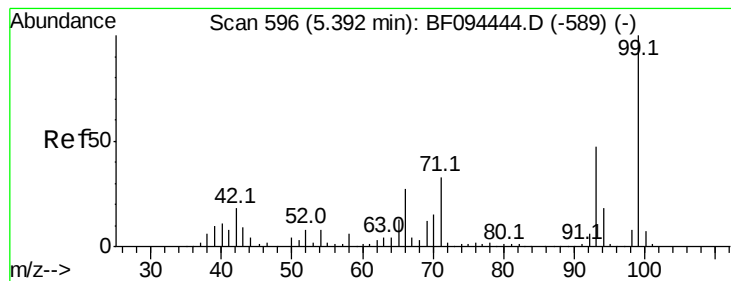

#7

Phenol-d6

Concen: 124.02 ng

RT: 5.40 min Scan# 589

Delta R.T. 0.01 min

Lab File: BF094695.D

Acq: 28 Apr 2017 20:31

Instrument :

BNA_F

ClientSampleId :





Tot Ion: 99 Resp: 989721

Ion Ratio Lower Upper

99 100

42 17.2 13.5 20.3

71 33.2 24.5 36.7

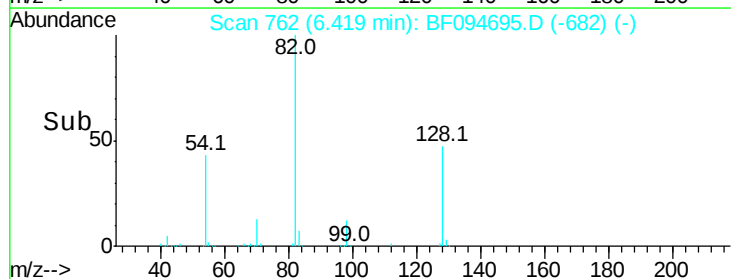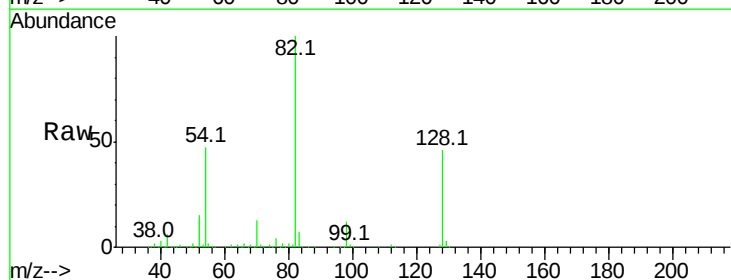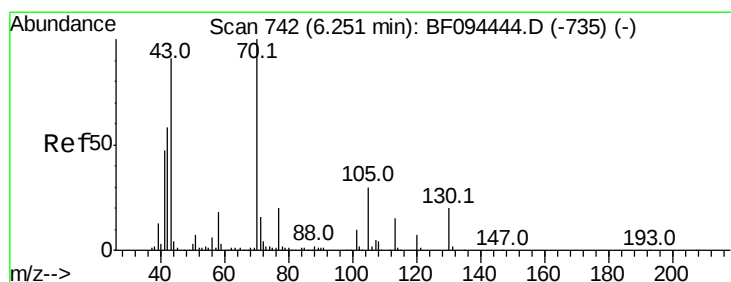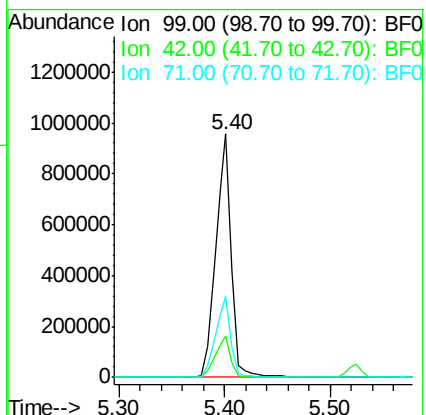

#19

n-Nitroso-di-n-propylamine

Concen: 14.31 ng

RT: 6.42 min Scan# 762

Delta R.T. 0.17 min

Lab File: BF094695.D

Acq: 28 Apr 2017 20:31

Tgt Ion: 70 Resp: 75662


Ion Ratio Lower Upper


70 100

42 44.2 47.2 70.8#

101 0.0 7.2 10.8#

130 2.1 15.9 23.9#

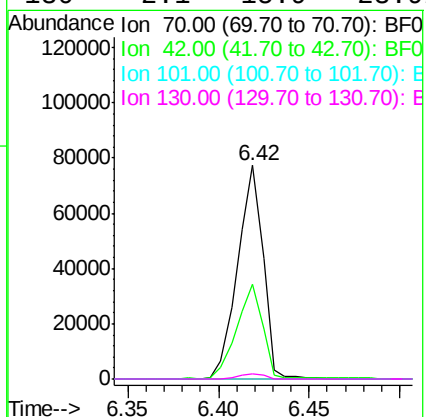







#21
Naphthalene-d8
Concen: 20.00 ng
RT: 7.26 min Scan# 905
Delta R.T. -0.00 min
Lab File: BF094695.D
Acq: 28 Apr 2017 20:31

Instrument :
BNA_F
ClientSampleId :

Tot Ion:136	Resp:	426903
Ion	Ratio	Lower Upper
136	100	
137	10.7	8.5 12.7
54	6.8	4.9 7.3
68	5.5	4.1 6.1

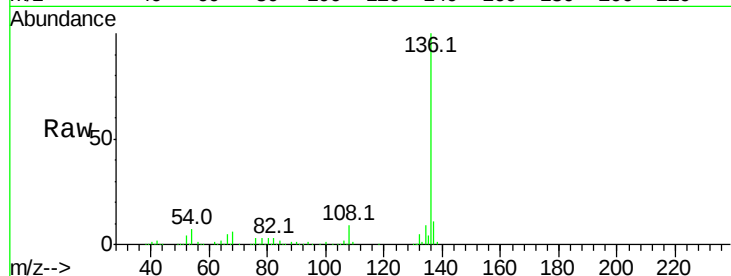


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF0
Ion 68.00 (67.70 to 68.70): BF0

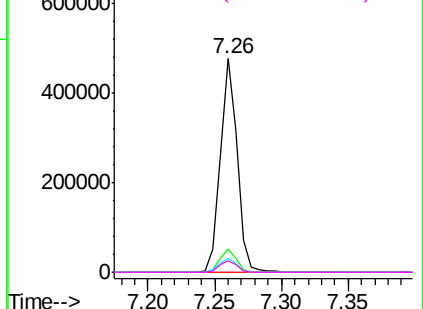



#23
Nitrobenzene-d5
Concen: 83.34 ng
RT: 6.42 min Scan# 762
Delta R.T. 0.00 min
Lab File: BF094695.D
Acq: 28 Apr 2017 20:31

Tgt Ion: 82	Resp:	576205
Ion	Ratio	Lower Upper
82	100	
128	46.5	34.0 51.0
54	47.3	42.2 63.2

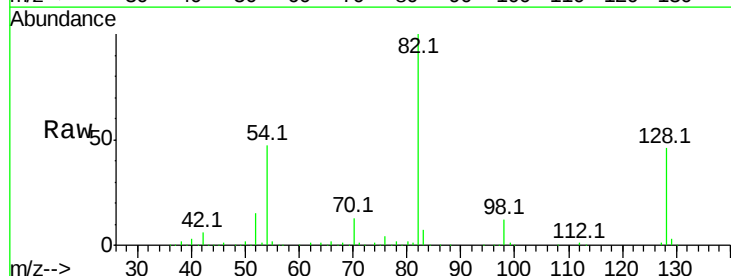

Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF0

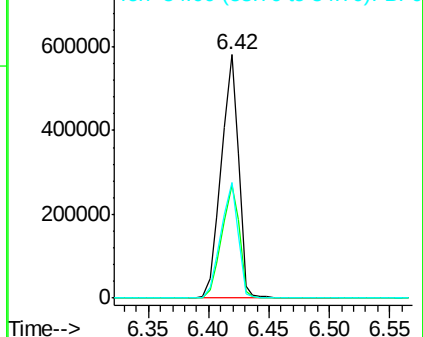



#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.40 min Scan# 1268

Delta R.T. -0.00 min

Lab File: BF094695.D

Acq: 28 Apr 2017 20:31

Instrument :

BNA_F

ClientSampled :


Tot Ion:164 Resp: 172410

Ion Ratio Lower Upper

164 100

162 105.3 82.6 123.8




160 45.6 36.2 54.2



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

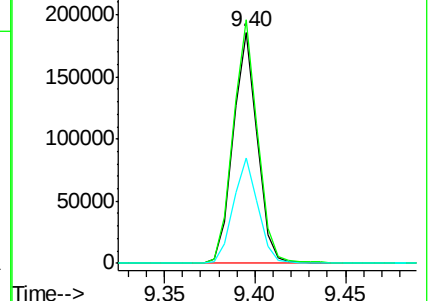

#41

2,4,6-Tribromophenol

Concen: 110.54 ng

RT: 10.37 min Scan# 1434

Delta R.T. -0.00 min

Lab File: BF094695.D

Acq: 28 Apr 2017 20:31


Tgt Ion:330 Resp: 149073

Ion Ratio Lower Upper

330 100

332 93.8 76.6 115.0



141 38.8 31.4 47.2




Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

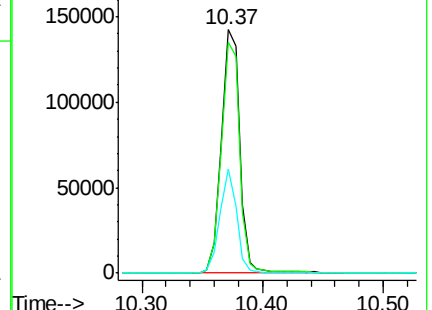


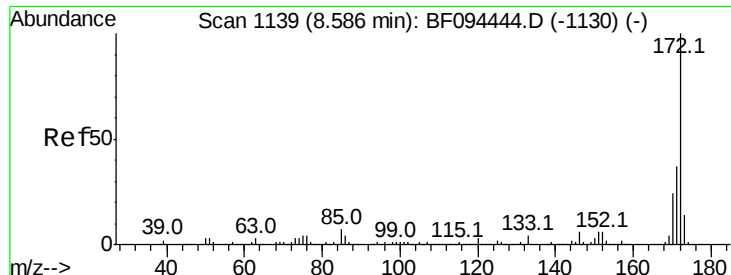




#44
2-Fluorobiphenyl
Concen: 68.26 ng
RT: 8.58 min Scan# 1130
Delta R.T. -0.00 min
Lab File: BF094695.D
Acq: 28 Apr 2017 20:31

Instrument :
BNA_F
ClientSampleId :

Tot Ion:172 Resp: 799922
Ion Ratio Lower Upper
172 100
171 35.9 29.6 44.4
170 23.6 19.8 29.8

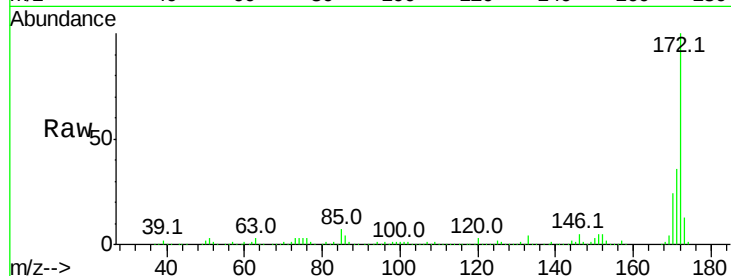


Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

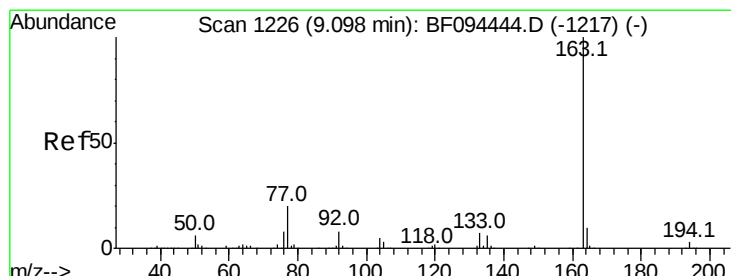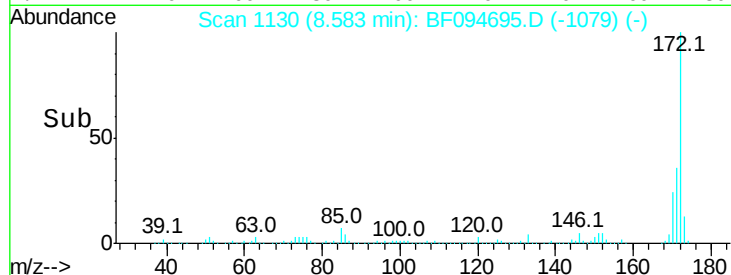
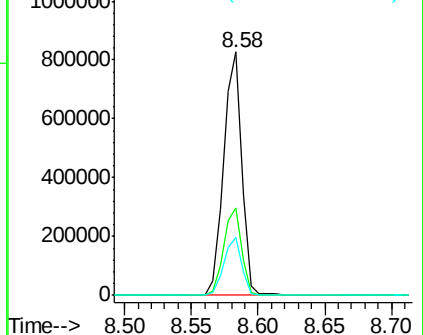


#49
Dimethylphthalate
Concen: 7.33 ng
RT: 9.08 min Scan# 1215
Delta R.T. -0.01 min
Lab File: BF094695.D
Acq: 28 Apr 2017 20:31

Tgt Ion:163 Resp: 94209
Ion Ratio Lower Upper
163 100
194 3.8 2.6 4.0
164 10.4 8.4 12.6

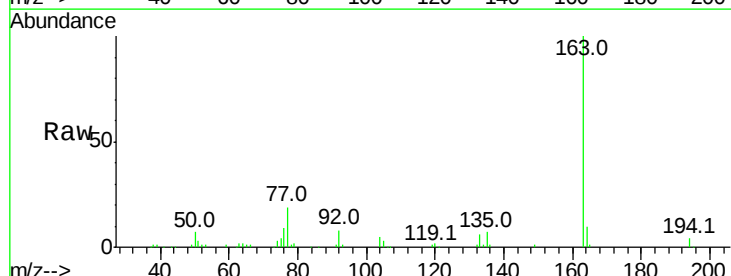

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

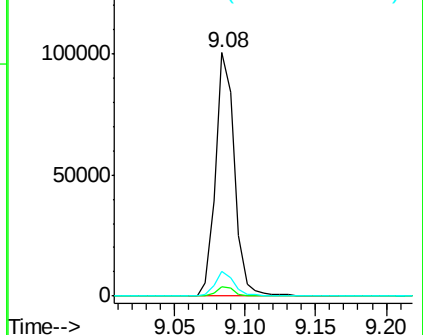



#56

2,4-Dinitrotoluene

Concen: 6.26 ng

RT: 9.40 min Scan# 1268

Delta R.T. -0.26 min

Lab File: BF094695.D

Acq: 28 Apr 2017 20:31

Instrument :

BNA_F

ClientSampleId :

Tot Ion:165 Resp: 22155


Ion Ratio Lower Upper

165 100

63 0.0 25.4 38.0#

89 0.0 46.4 69.6#

182 0.0 1.8 2.6#






Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF0

Ion 89.00 (88.70 to 89.70): BF0

Ion 182.00 (181.70 to 182.70): E

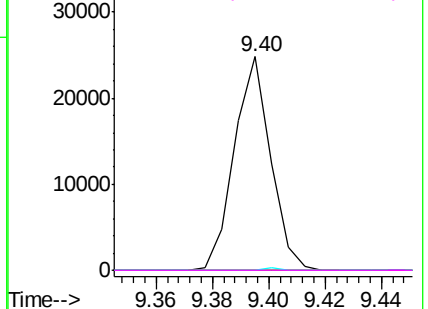

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.22 min Scan# 1578

Delta R.T. -0.00 min

Lab File: BF094695.D

Acq: 28 Apr 2017 20:31


Tgt Ion:188 Resp: 267071

Ion Ratio Lower Upper

188 100

94 9.9 9.4 14.2



80 10.9 10.2 15.2




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

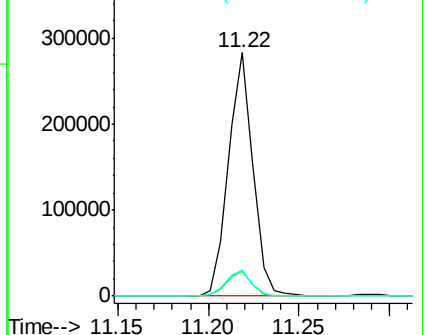



#75

Chrysene-d12

Concen: 20.00 ng

RT: 14.47 min Scan# 2131

Delta R.T. 0.00 min

Lab File: BF094695.D

Acq: 28 Apr 2017 20:31

Instrument :

BNA_F

ClientSampled :


Tot Ion:240 Resp: 225223

Ion Ratio Lower Upper

240 100

120 13.3 5.8 8.8#




236 24.5 20.5 30.7



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

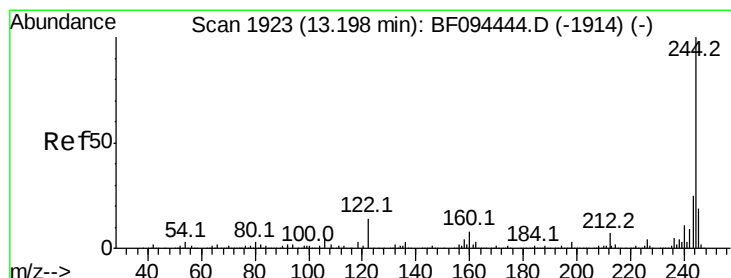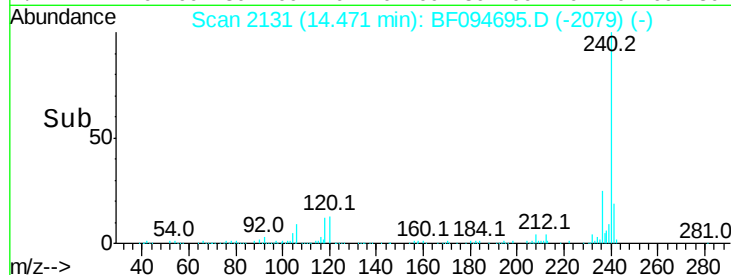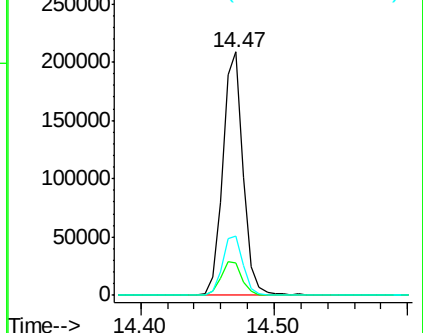

#78

Terphenyl-d14

Concen: 55.68 ng

RT: 13.19 min Scan# 1914

Delta R.T. -0.00 min

Lab File: BF094695.D

Acq: 28 Apr 2017 20:31


Tgt Ion:244 Resp: 469129

Ion Ratio Lower Upper

244 100

212 6.7 6.0 9.0



122 14.2 10.3 15.5




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

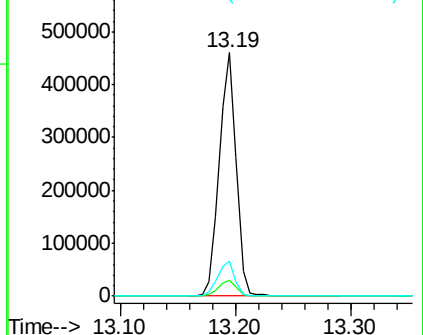


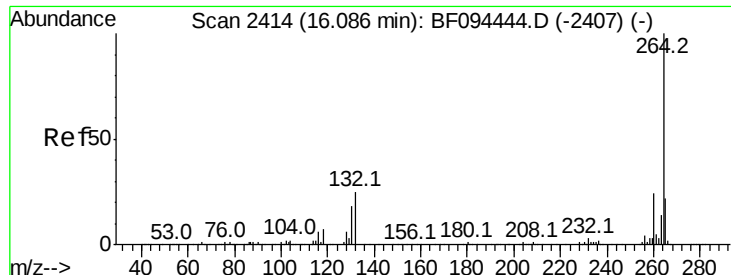

#86
 Pervlene-d12
 Concen: 20.00 ng
 RT: 16.10 min Scan# 2408
 Delta R.T. 0.01 min
 Lab File: BF094695.D
 Acq: 28 Apr 2017 20:31

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	22.9	19.5	29.3
265	21.5	17.2	25.8

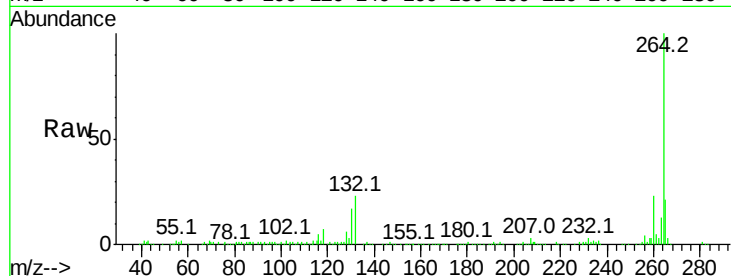

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

