

Data Path : Z:\HPCHEM1\BNA F\DATA\BF042817\
 Data File : BF094694.D
 Acq On : 28 Apr 2017 20:04
 Operator : SJ/MA
 Sample : I2895-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-02-COMP(0-3.0)

Quant Time: Apr 29 01:40:27 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF041717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 17 14:59:23 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	5.77	152	113195	20.00	ng	0.00
21) Naphthalene-d8	7.26	136	429709	20.00	ng	0.00
38) Acenaphthene-d10	9.40	164	182691	20.00	ng	0.00
63) Phenanthrene-d10	11.22	188	278391	20.00	ng	0.00
75) Chrysene-d12	14.47	240	227220	20.00	ng	0.00
86) Perylene-d12	16.10	264	170423	20.00	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	4.33	112	984839	144.34	ng	0.03
7) Phenol-d6	5.41	99	1194223	148.47	ng	0.01
23) Nitrobenzene-d5	6.42	82	698732	100.41	ng	0.00
41) 2,4,6-Tribromophenol	10.38	330	199265	139.45	ng	0.00
44) 2-Fluorobiphenyl	8.58	172	1149099	92.54	ng	0.00
78) Terphenyl-d14	13.19	244	741082	87.18	ng	0.00
Target Compounds						
49) Dimethylphthalate	9.08	163	111435	8.18	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF042817\
Data File : BF094694.D
Acq On : 28 Apr 2017 20:04
Operator : SJ/MA
Sample : I2895-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-02-COMP(0-3.0)

Quant Time: Apr 29 01:40:27 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF041717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 17 14:59:23 2017
Response via : Initial Calibration

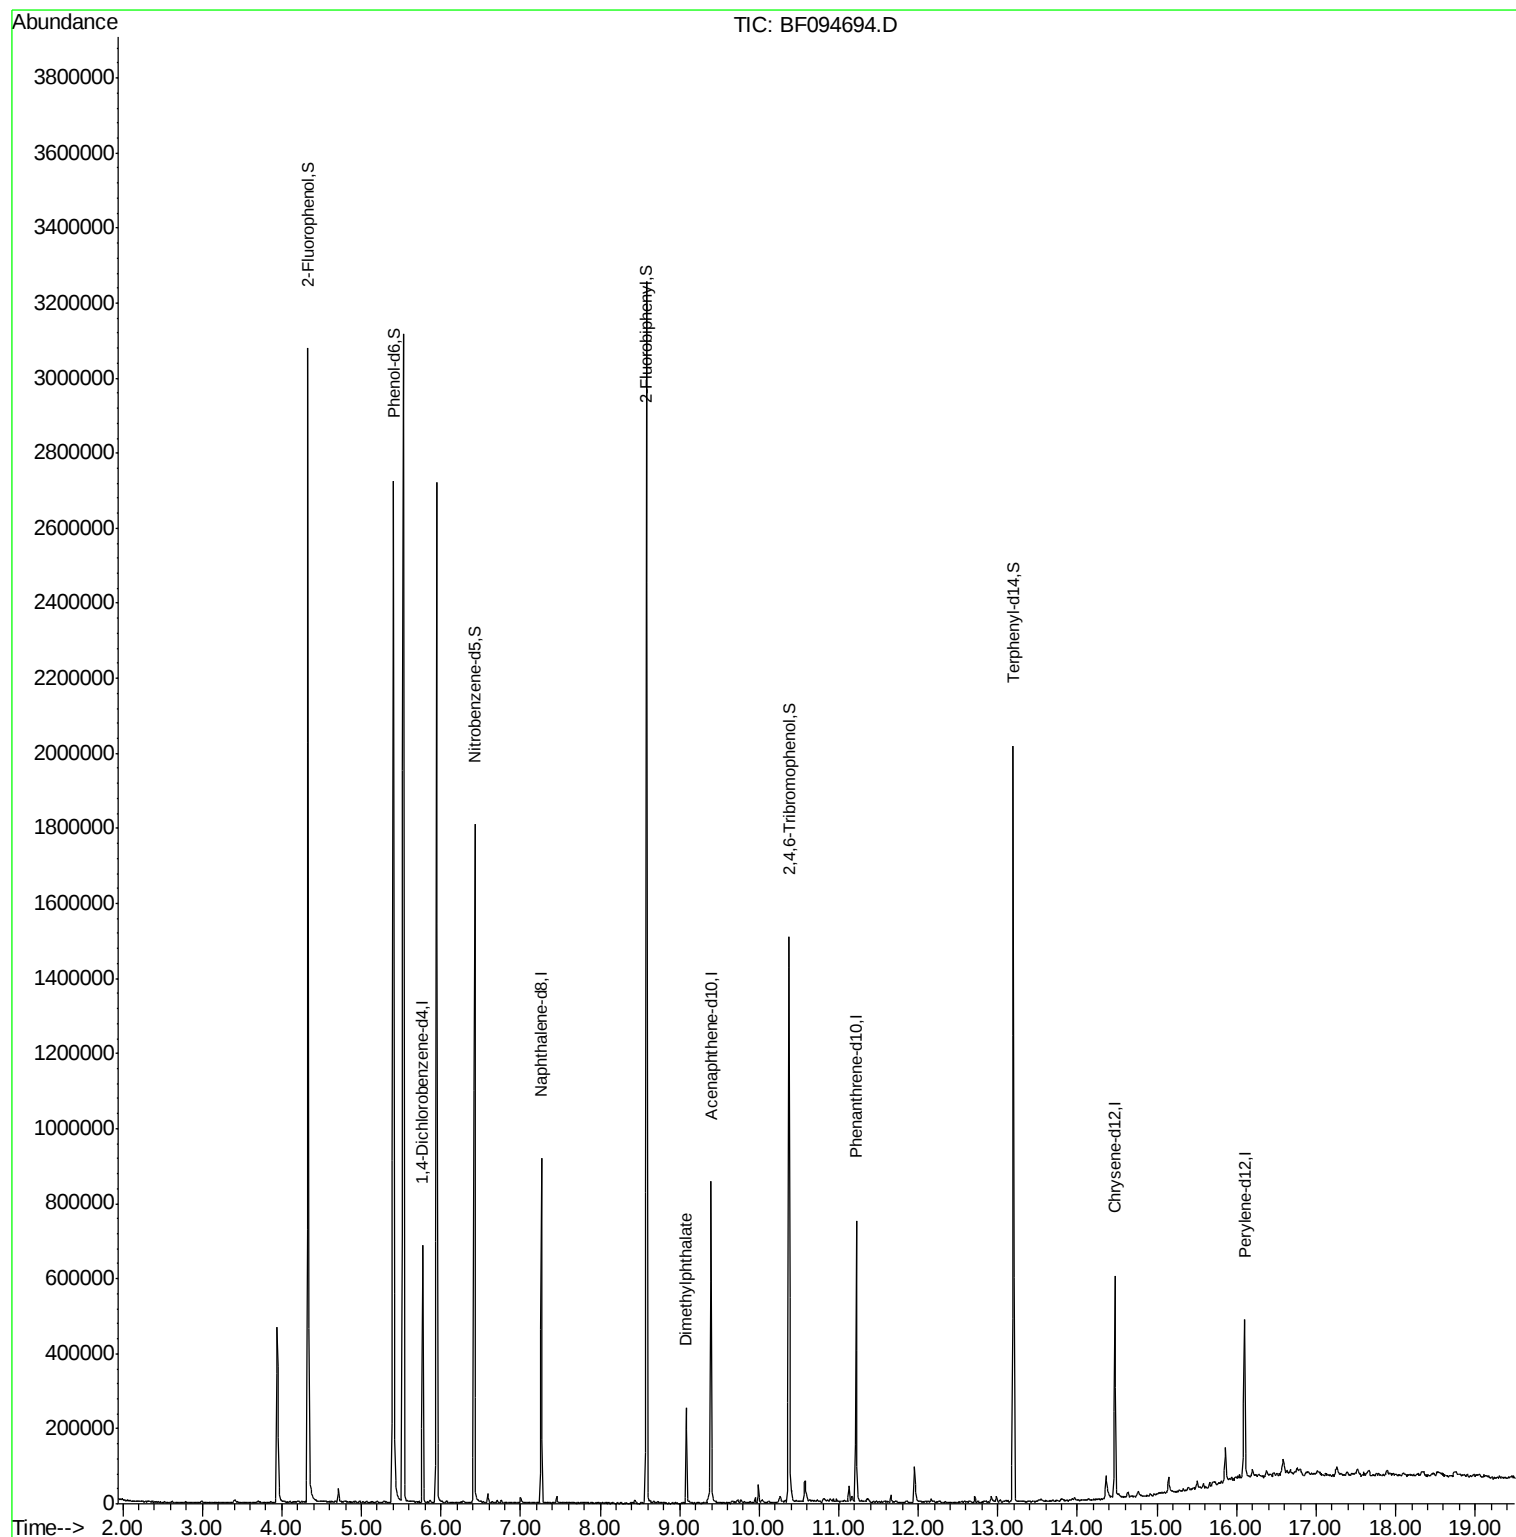

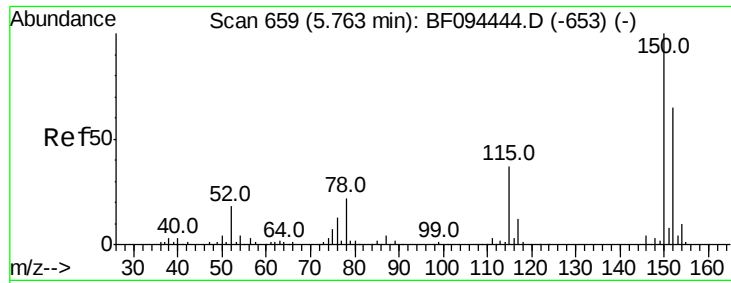


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 5.77 min Scan# 652
Delta R.T. 0.01 min
Lab File: BF094694.D
Acq: 28 Apr 2017 20:04

Instrument :
BNA_F
ClientSampleId :
SB-02-COMP(0-3.0)

Tot Ion:152 Resp: 113195
Ion Ratio Lower Upper
152 100
150 156.1 126.2 189.2
115 61.4 52.2 78.2

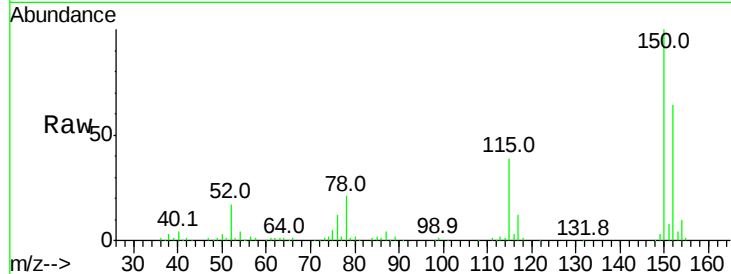


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

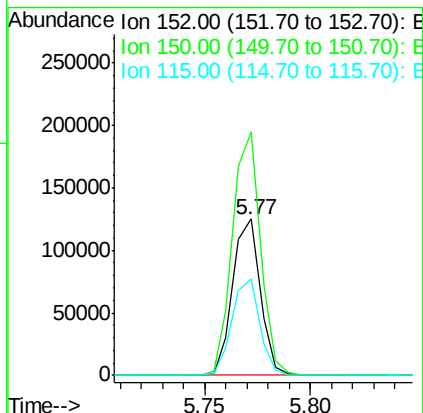



#5


2-Fluorophenol
Concen: 144.34 ng
RT: 4.33 min Scan# 407
Delta R.T. 0.03 min
Lab File: BF094694.D
Acq: 28 Apr 2017 20:04

Tgt Ion:112 Resp: 984839
Ion Ratio Lower Upper
112 100
64 57.3 46.0 69.0
63 28.1 23.4 35.0



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

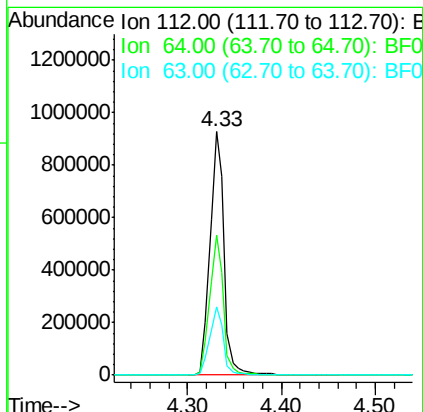

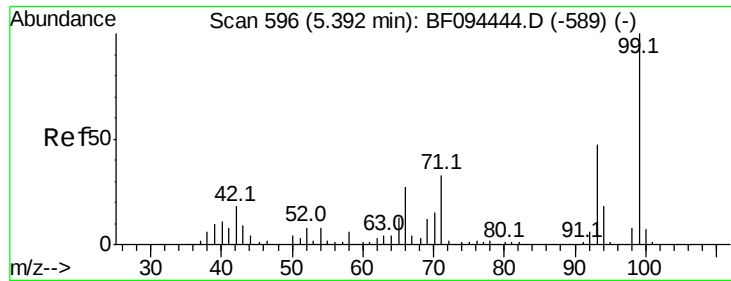

#7

Phenol-d6

Concen: 148.47 ng

RT: 5.41 min Scan# 590

Delta R.T. 0.01 min

Lab File: BF094694.D

Acq: 28 Apr 2017 20:04

Instrument :

BNA_F

ClientSampleId :

SB-02-COMP(0-3.0)


Tot Ion: 99 Resp: 1194223

Ion Ratio Lower Upper

99 100

42 16.7 13.5 20.3




71 32.8 24.5 36.7



Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

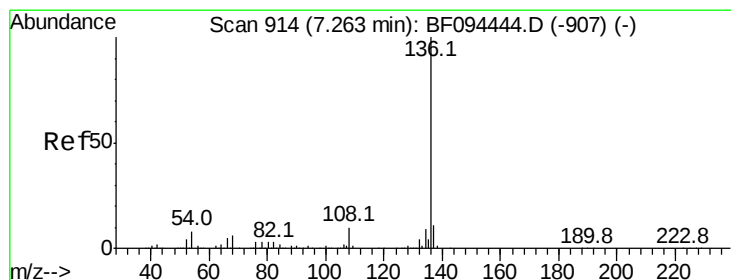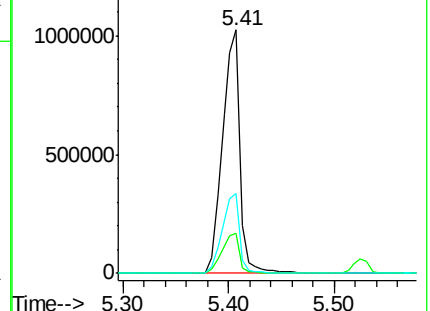

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.26 min Scan# 905

Delta R.T. -0.00 min

Lab File: BF094694.D

Acq: 28 Apr 2017 20:04

Tgt Ion: 136 Resp: 429709


Ion Ratio Lower Upper

136 100

137 10.9 8.5 12.7

54 7.2 4.9 7.3

68 5.3 4.1 6.1






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0



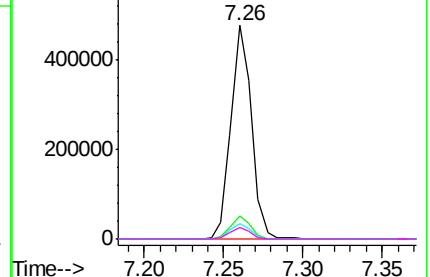



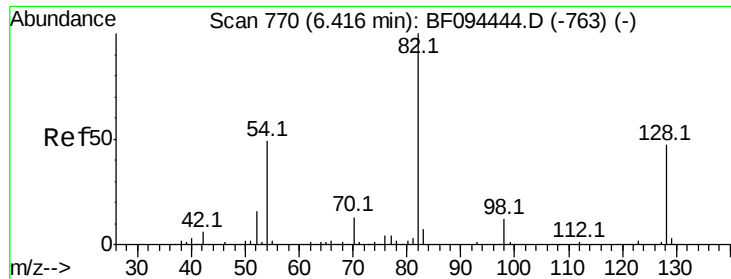

#23
 Nitrobenzene-d5
 Concen: 100.41 ng
 RT: 6.42 min Scan# 763
 Delta R.T. 0.01 min
 Lab File: BF094694.D
 Acq: 28 Apr 2017 20:04




Instrument :
 BNA_F
 ClientSampleId :
 SB-02-COMP(0-3.0)


Tot Ion: 82 Resp: 698732
 Ion Ratio Lower Upper
 82 100
 128 48.4 34.0 51.0
 54 46.6 42.2 63.2

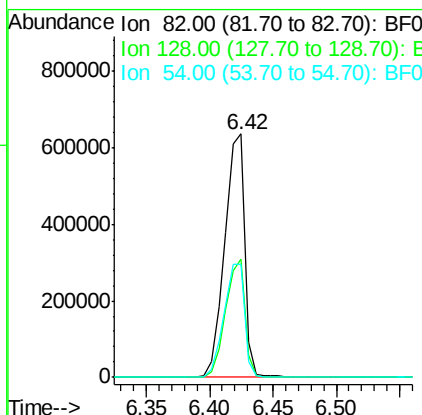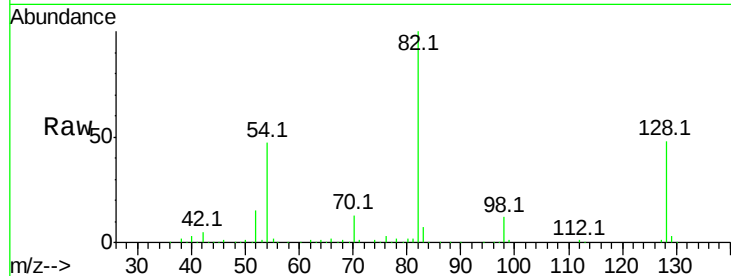

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.40 min Scan# 1268
 Delta R.T. -0.00 min
 Lab File: BF094694.D
 Acq: 28 Apr 2017 20:04

Tgt Ion:164 Resp: 182691
 Ion Ratio Lower Upper
 164 100
 162 100.0 82.6 123.8
 160 44.4 36.2 54.2

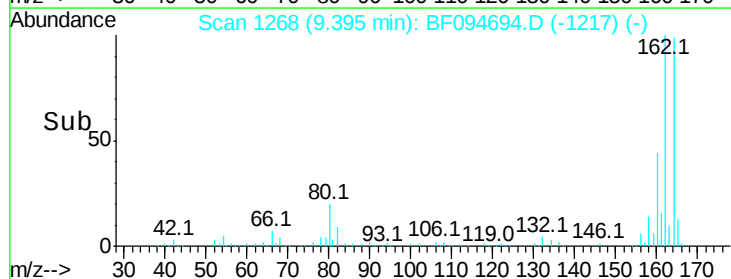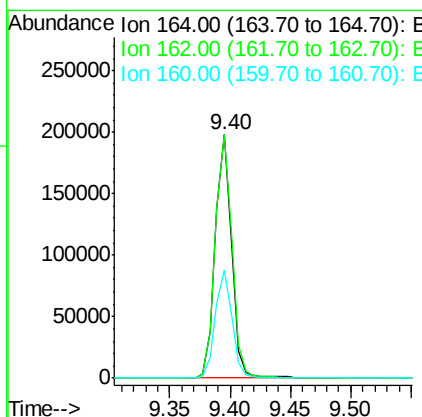


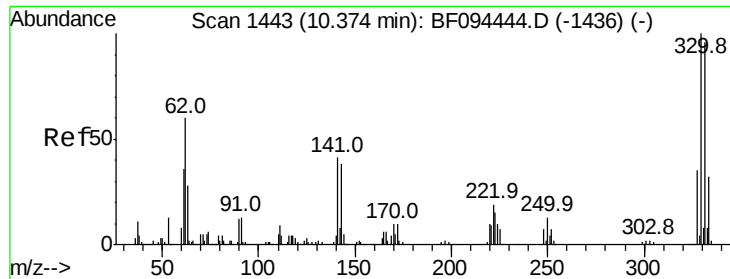




#41
 2,4,6-Tribromophenol
 Concen: 139.45 ng
 RT: 10.38 min Scan# 1435
 Delta R.T. 0.00 min
 Lab File: BF094694.D
 Acq: 28 Apr 2017 20:04

Instrument :
 BNA_F
 ClientSampleId :
 SB-02-COMP(0-3.0)

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.8	76.6	115.0
141	39.6	31.4	47.2

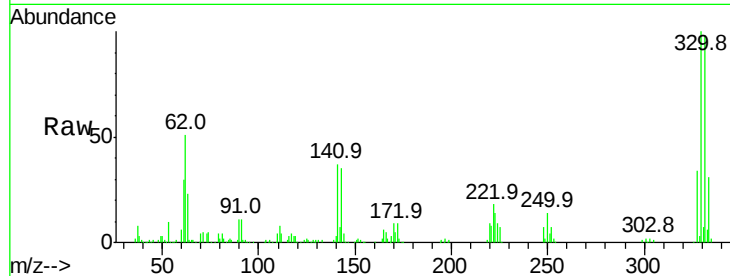


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

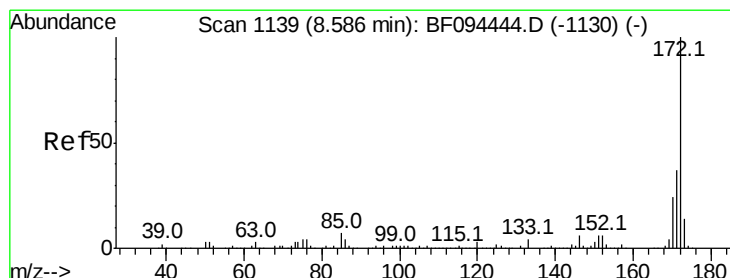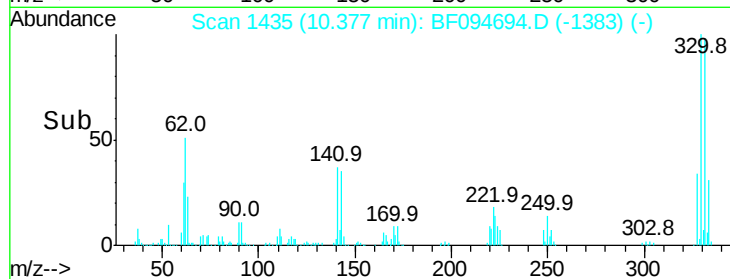
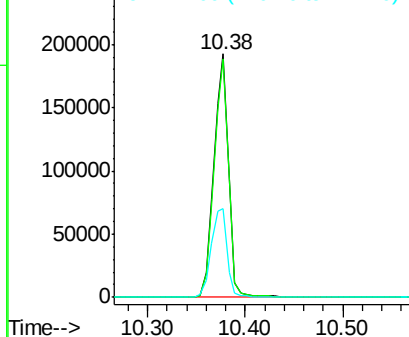



#44
 2-Fluorobiphenyl
 Concen: 92.54 ng
 RT: 8.58 min Scan# 1130
 Delta R.T. -0.00 min
 Lab File: BF094694.D
 Acq: 28 Apr 2017 20:04

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.1	29.6	44.4
170	23.8	19.8	29.8

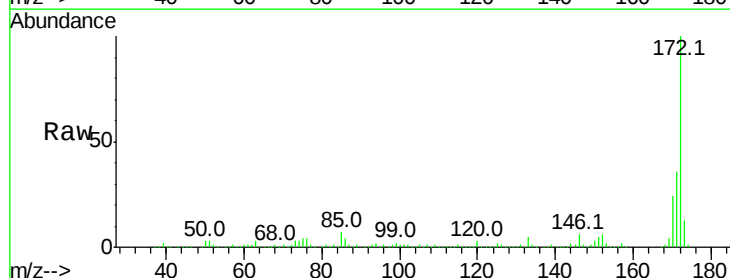

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

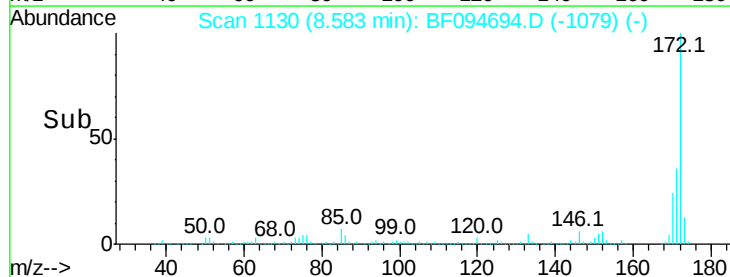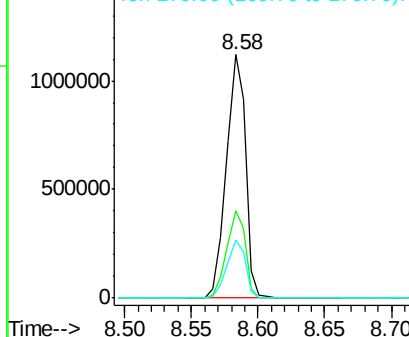



#49

Dimethylphthalate

Concen: 8.18 ng

RT: 9.08 min Scan# 1215

Delta R.T. -0.01 min

Lab File: BF094694.D

Acq: 28 Apr 2017 20:04

Instrument :

BNA_F

ClientSampleId :

SB-02-COMP(0-3.0)


Tot Ion:163 Resp: 111435

Ion Ratio Lower Upper

163 100

194 3.7 2.6 4.0




164 10.2 8.4 12.6



Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

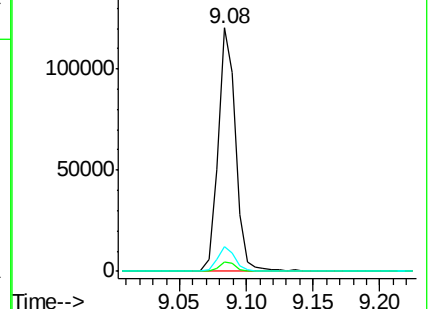

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.22 min Scan# 1578

Delta R.T. -0.00 min

Lab File: BF094694.D

Acq: 28 Apr 2017 20:04


Tgt Ion:188 Resp: 278391

Ion Ratio Lower Upper

188 100

94 10.0 9.4 14.2



80 10.6 10.2 15.2




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

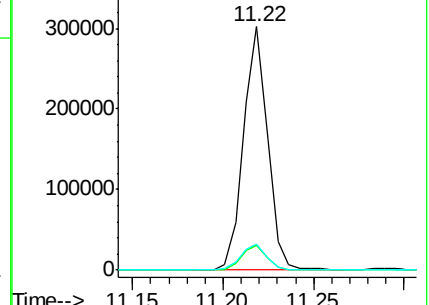



#75

Chrysene-d12

Concen: 20.00 ng

RT: 14.47 min Scan# 2131

Delta R.T. 0.00 min

Lab File: BF094694.D

Acq: 28 Apr 2017 20:04

Instrument :

BNA_F

ClientSampleId :

SB-02-COMP(0-3.0)


Tot Ion:240 Resp: 227220

Ion Ratio Lower Upper

240 100

120 12.8 5.8 8.8#




236 24.6 20.5 30.7

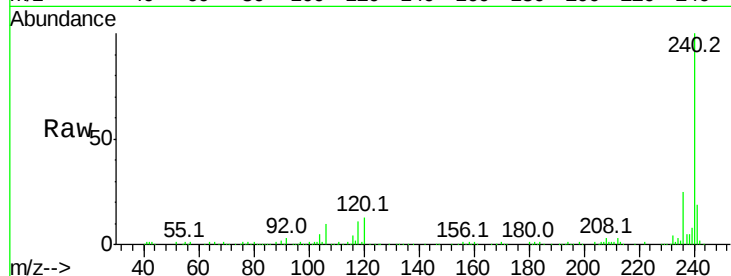

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

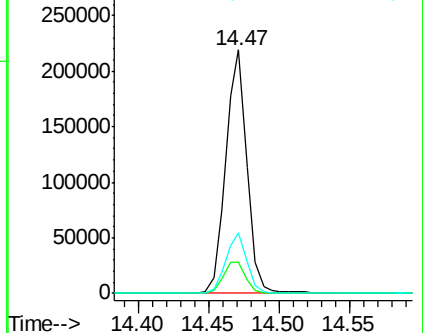

#78

Terphenyl-d14

Concen: 87.18 ng

RT: 13.19 min Scan# 1914

Delta R.T. -0.00 min

Lab File: BF094694.D

Acq: 28 Apr 2017 20:04


Tgt Ion:244 Resp: 741082

Ion Ratio Lower Upper

244 100

212 6.7 6.0 9.0



122 14.7 10.3 15.5




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

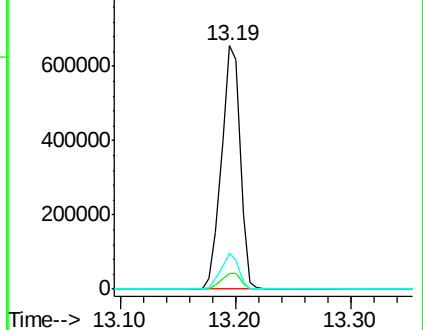


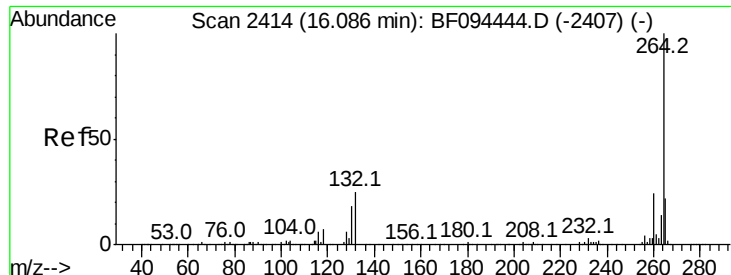

#86
 Pervlene-d12
 Concen: 20.00 ng
 RT: 16.10 min Scan# 2408
 Delta R.T. 0.01 min
 Lab File: BF094694.D
 Acq: 28 Apr 2017 20:04

Instrument :
 BNA_F
 ClientSampleId :
 SB-02-COMP(0-3.0)

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.5	19.5	29.3
265	22.1	17.2	25.8

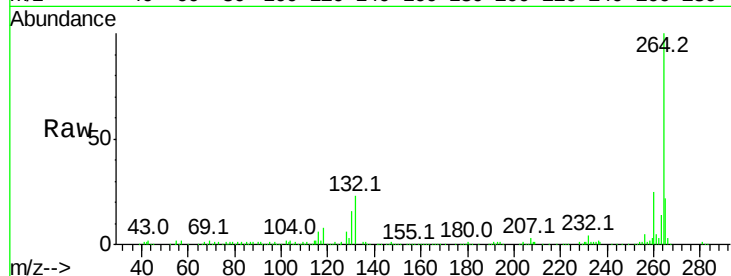

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

