


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF042817\
 Data File : BF094680.D
 Acq On : 28 Apr 2017 13:31
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF041717.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 17 14:59:23 2017

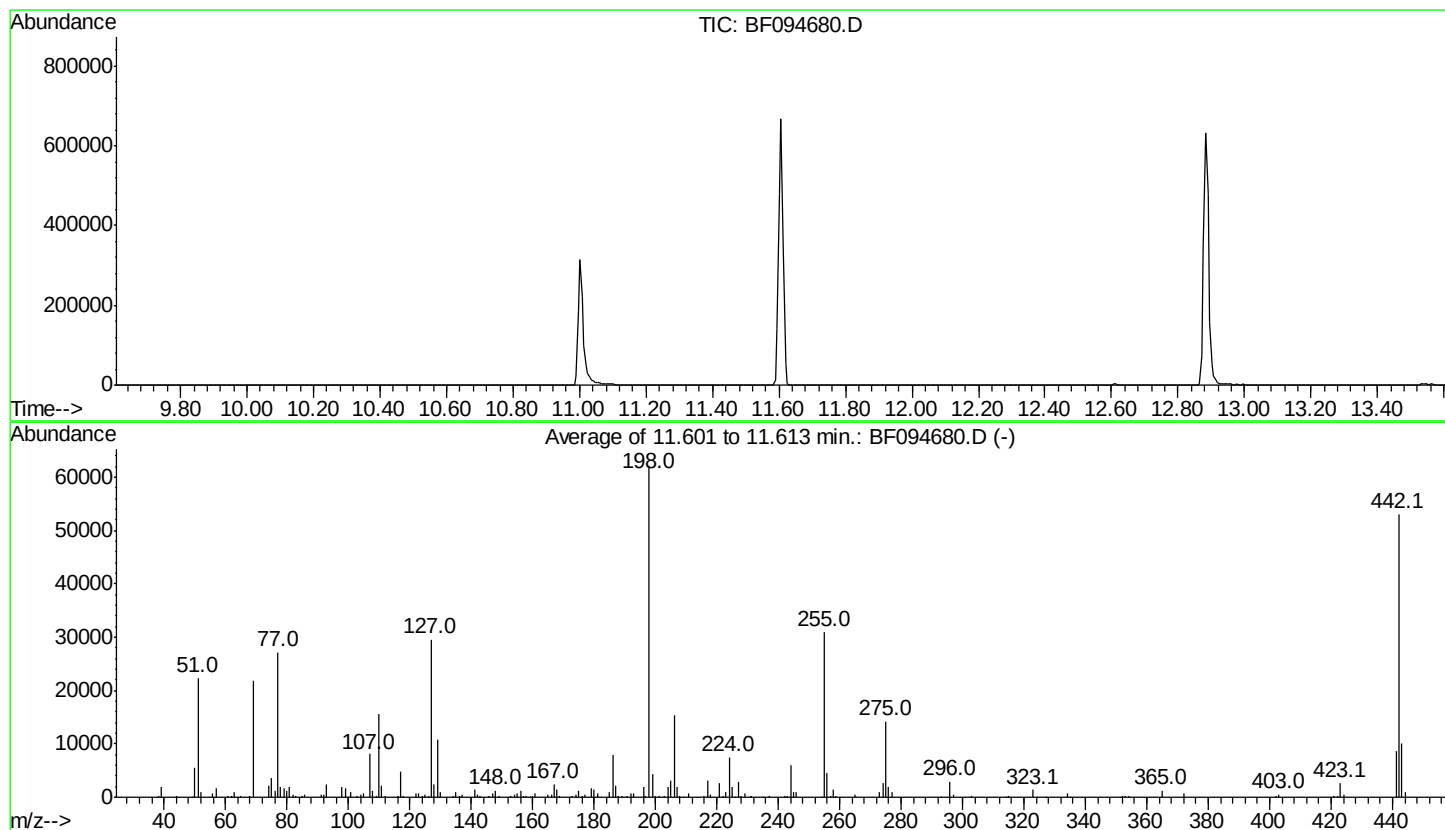

AutoFind: Scans 1643, 1644, 1645; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.0	22387	PASS
68	69	0.00	2	1.7	362	PASS
69	198	0.00	100	35.2	21894	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.7	29618	PASS
197	198	0.00	2	0.3	204	PASS
198	198	100	100	100.0	62133	PASS
199	198	5	9	7.0	4379	PASS
275	198	10	60	22.8	14187	PASS
365	198	1	100	2.1	1318	PASS
441	442	0.01	24	16.4	8722	PASS
442	198	50	100	85.4	53069	PASS
443	442	15	24	19.1	10117	PASS