
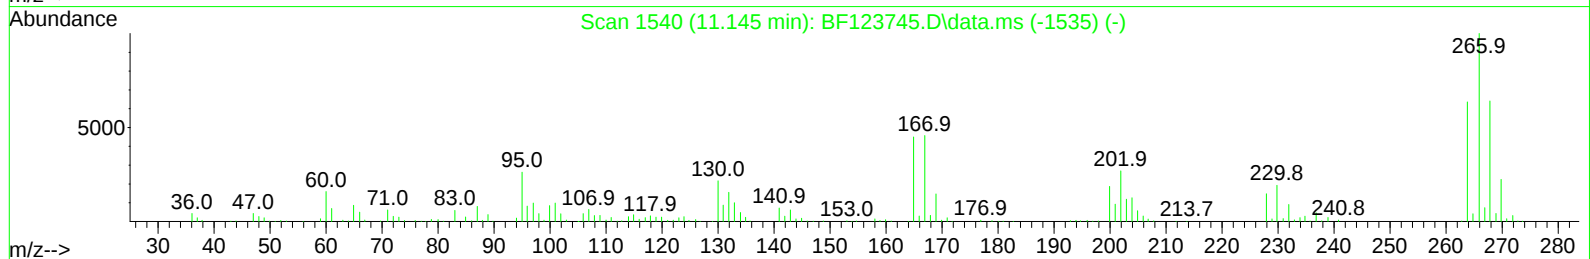
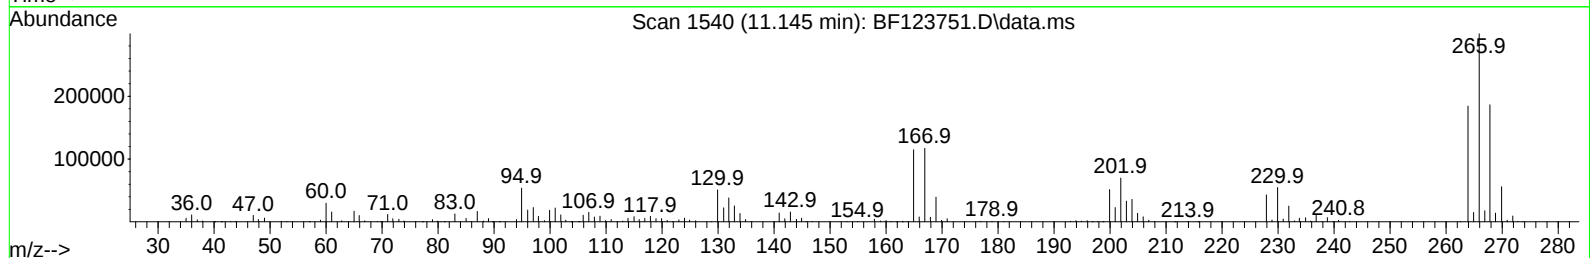


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042821\
Data File : BF123751.D
Acq On : 28 Apr 2021 8:48
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 28 11:13:27 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 27 16:30:39 2021
Response via : Initial Calibration

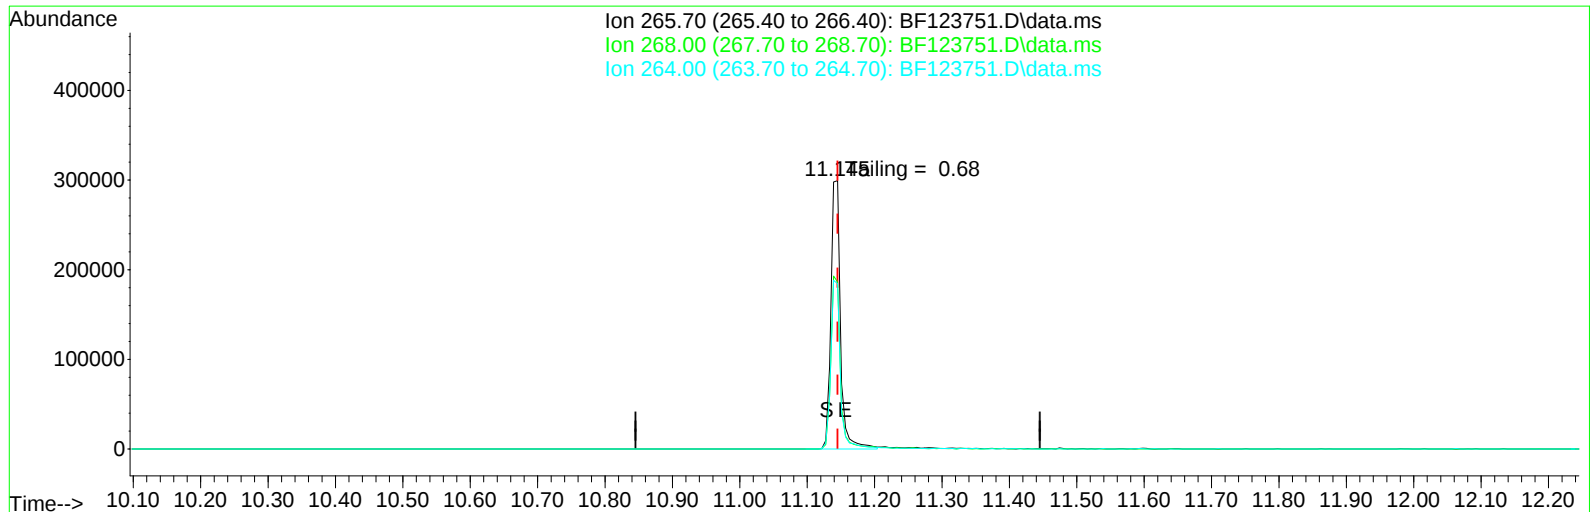

TIC: BF123751.D\data.ms

(70) Pentachlorophenol (C)




11.145min (-0.000) 455708.59 ng

response 300662

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	62.23
264.00	65.70	61.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042821\
Data File : BF123751.D
Acq On : 28 Apr 2021 8:48
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 28 11:13:27 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 27 16:30:39 2021
Response via : Initial Calibration

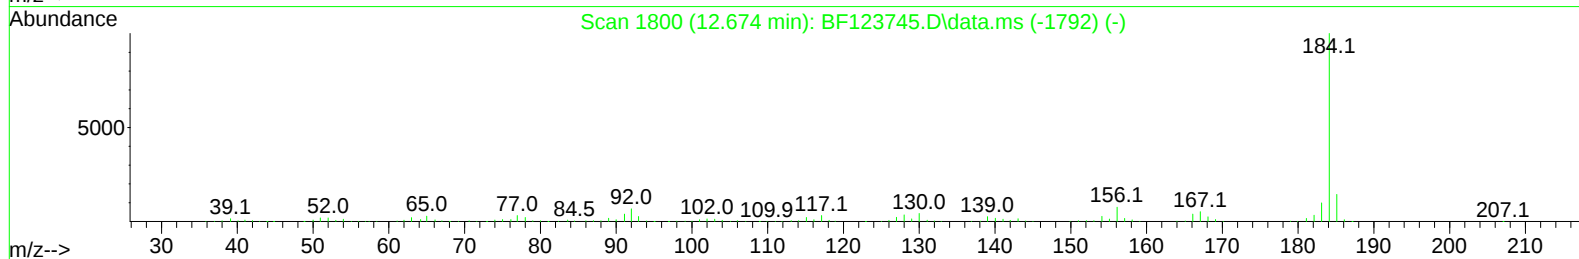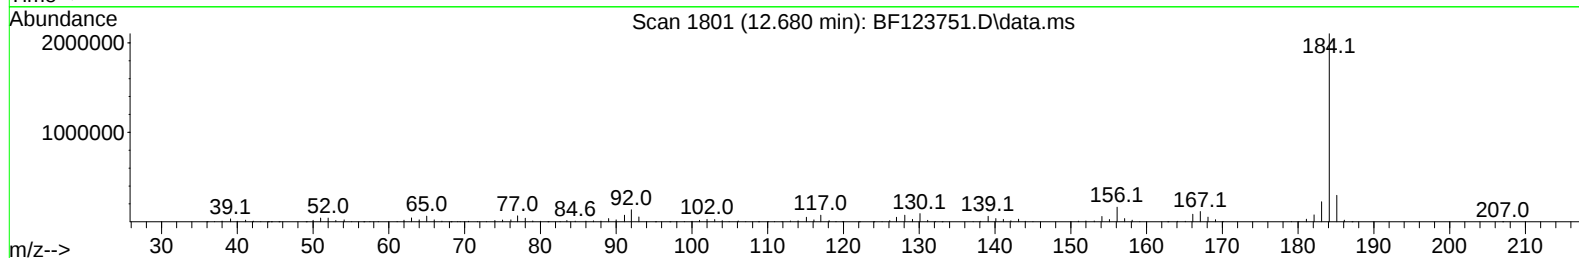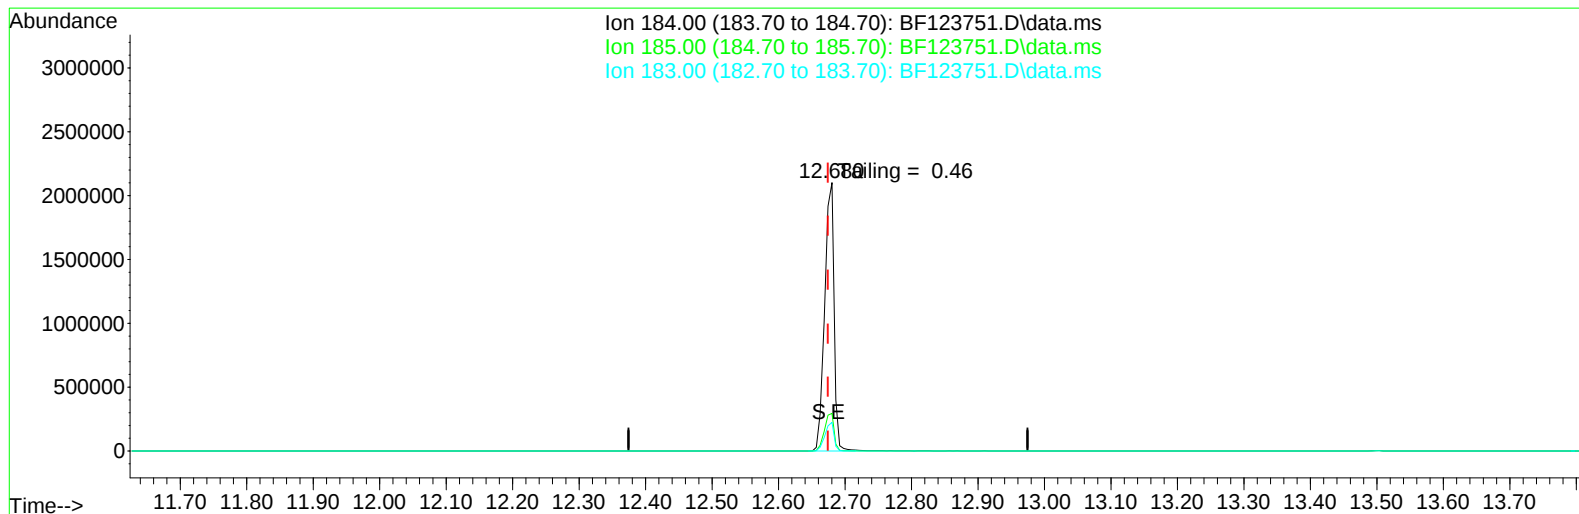

TIC: BF123751.D\data.ms

(77) Benzidine

12.680min (+ 0.006) 61442.29 ng

response 2077997

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.03
183.00	9.80	10.67
0.00	0.00	0.00