
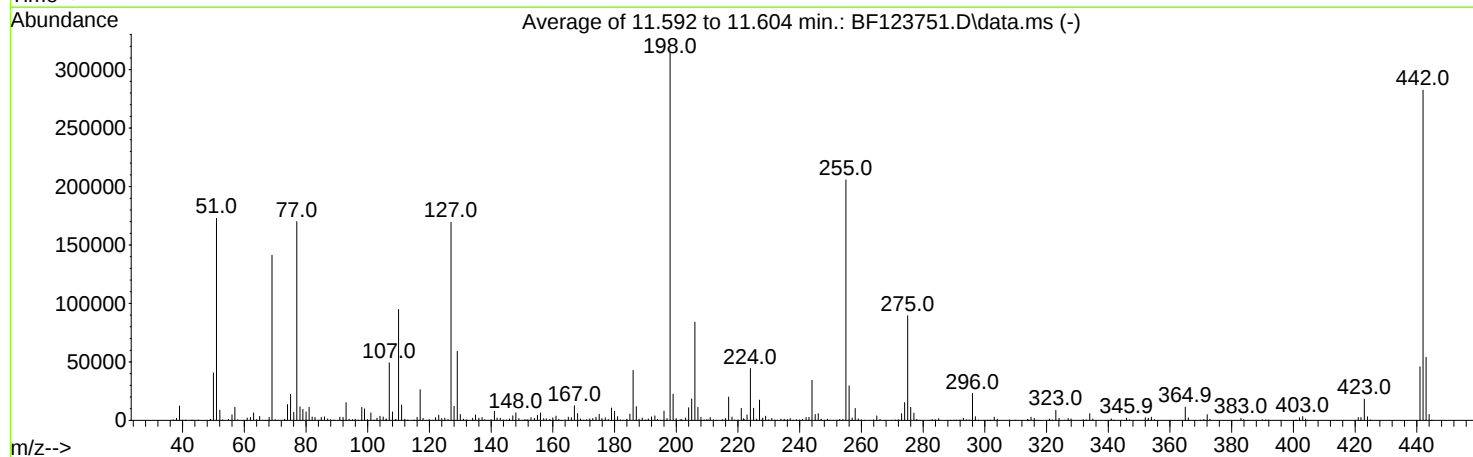


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042821\
 Data File : BF123751.D
 Acq On : 28 Apr 2021 8:48
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 27 16:30:39 2021

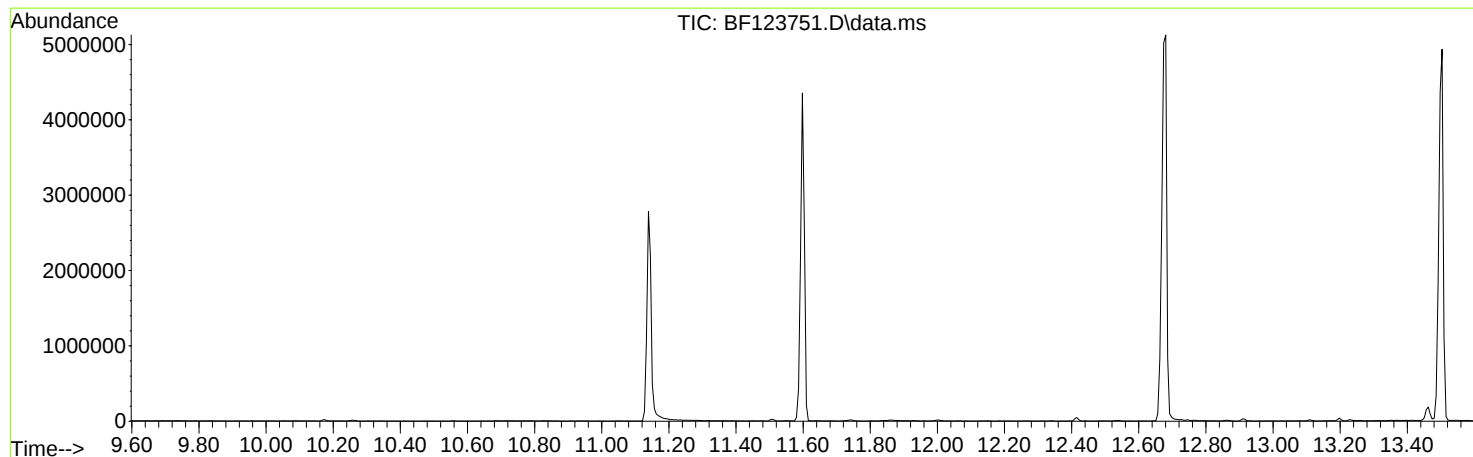

AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.9	172880	PASS
68	69	0.00	2	1.9	2682	PASS
69	198	0.00	100	44.9	141248	PASS
70	69	0.00	2	0.5	662	PASS
127	198	10	80	53.8	169381	PASS
197	198	0.00	2	0.5	1648	PASS
198	198	100	100	100.0	314645	PASS
199	198	5	9	7.2	22520	PASS
275	198	10	60	28.4	89483	PASS
365	198	1	100	3.6	11415	PASS
441	198	0.01	100	14.6	45795	PASS
442	442	50	100	100.0	282493	PASS
443	442	15	24	19.1	53971	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/28/2021	BNA_F	<u>BF123751.D</u>
Compound Name	Response	Retention Time
DDT	813516	13.5
DDD	4977	13.19
DDE	1724	12.86
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6701	820217	0.82

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042821\
 Data File : BF123751.D
 Acq On : 28 Apr 2021 8:48
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Apr 28 11:13:27 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 27 16:30:39 2021
 Response via : Initial Calibration

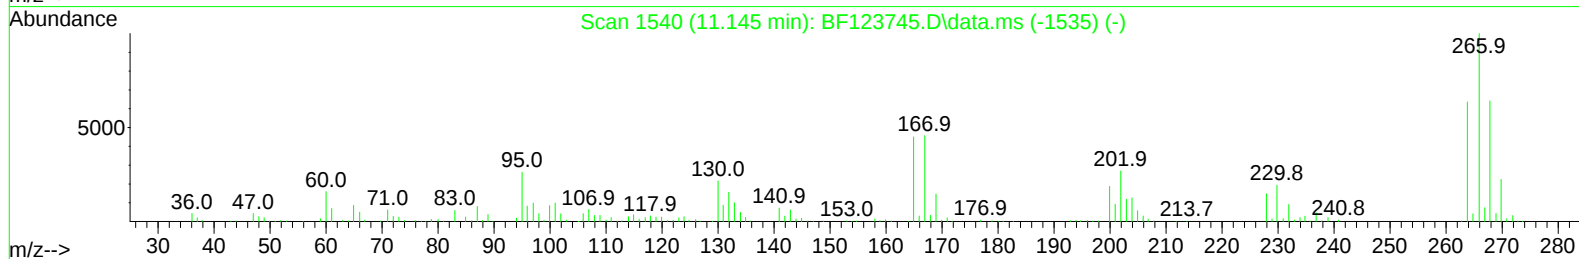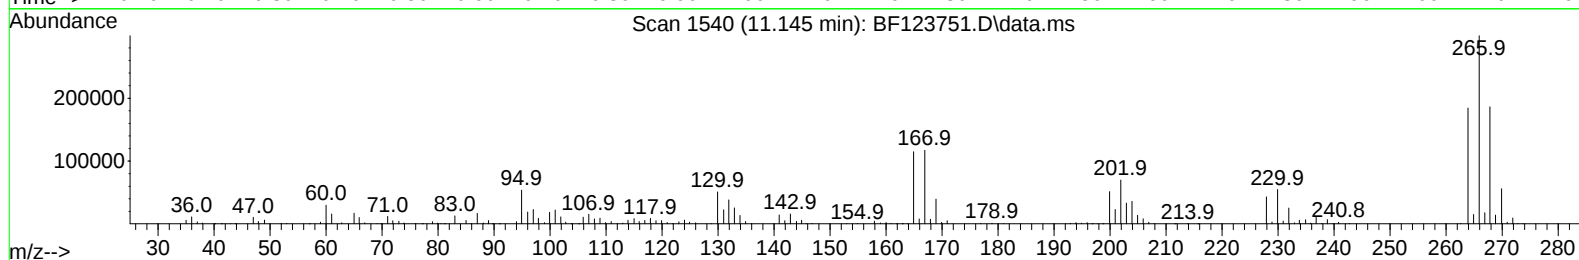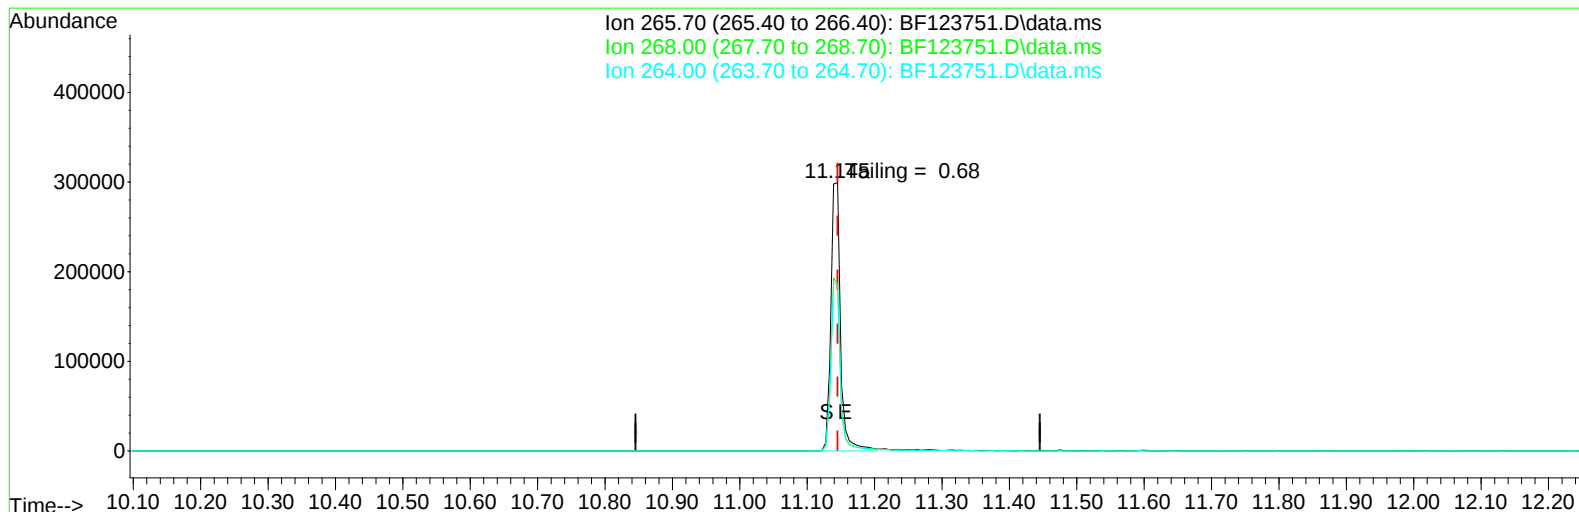

TIC: BF123751.D\data.ms

(70) Pentachlorophenol (C)

11.145min (-0.000) 455708.59 ng




response 300662

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	62.23
264.00	65.70	61.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042821\
Data File : BF123751.D
Acq On : 28 Apr 2021 8:48
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 28 11:13:27 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 27 16:30:39 2021
Response via : Initial Calibration

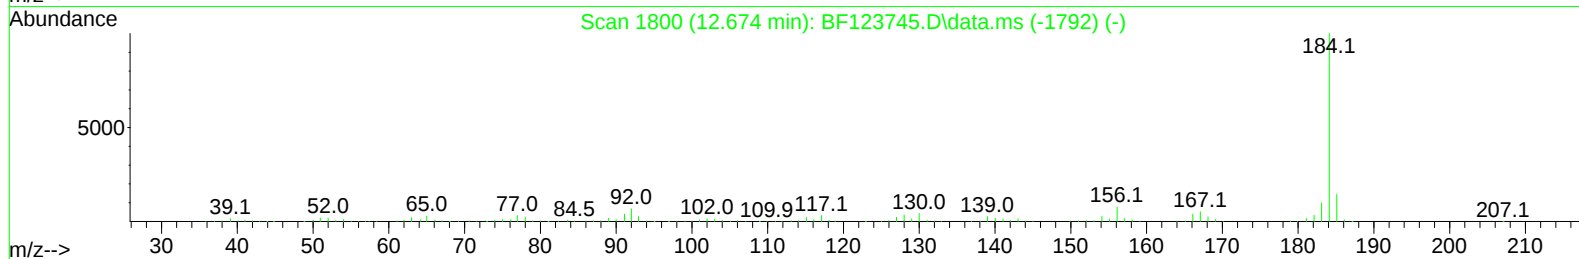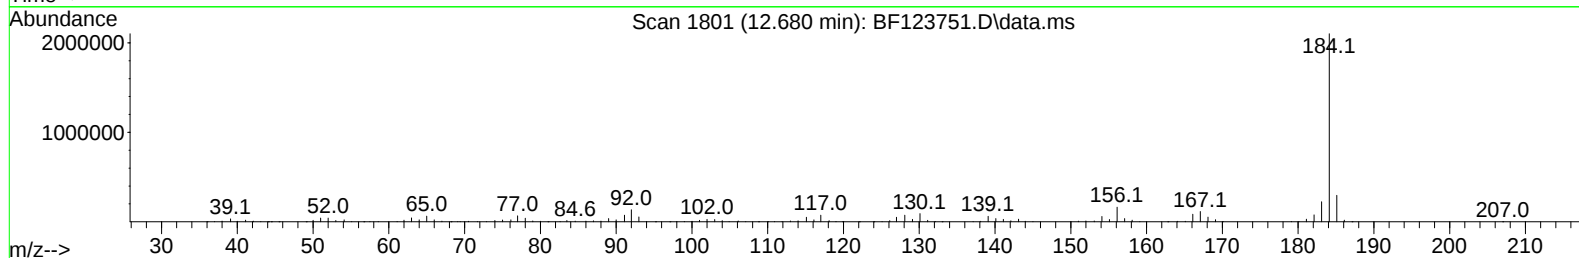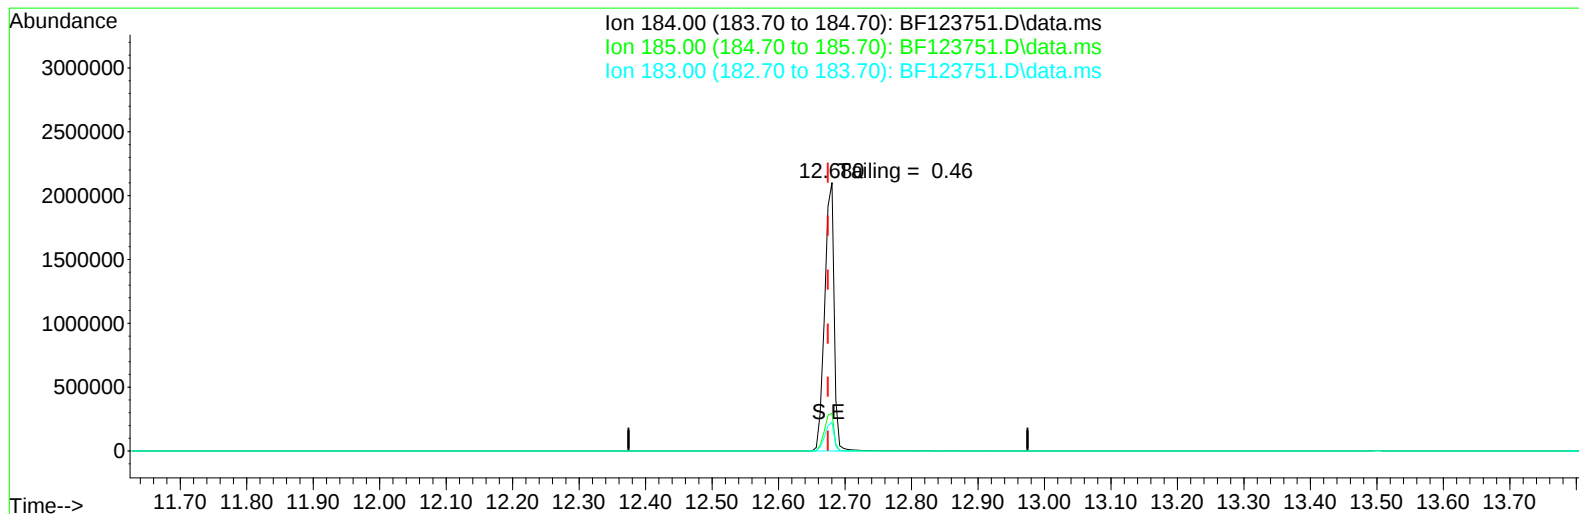

TIC: BF123751.D\data.ms

(77) Benzidine

12.680min (+ 0.006) 61442.29 ng

response 2077997

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.03
183.00	9.80	10.67
0.00	0.00	0.00