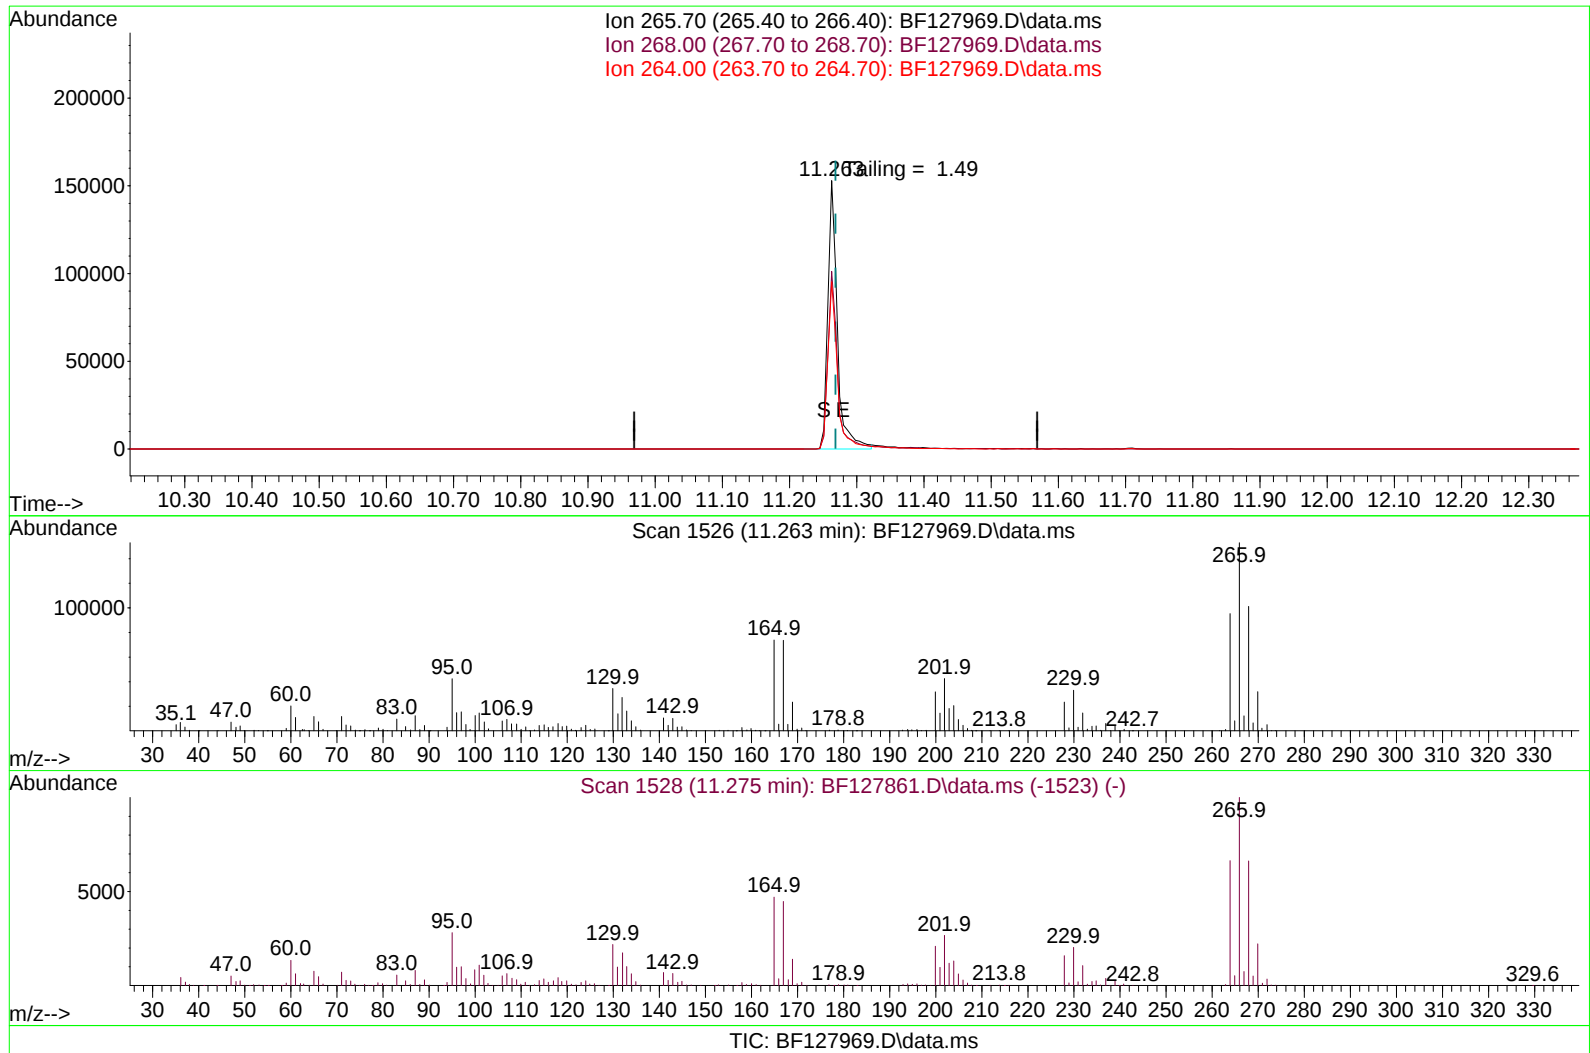


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF042822\  
Data File : BF127969.D  
Acq On : 28 Apr 2022 09:30  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 28 17:39:21 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF042222.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Apr 28 05:13:03 2022  
Response via : Initial Calibration

**(70) Pentachlorophenol (C)****11.263min (-0.006) 28901.39 ng****response 154897**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 66.30  | 66.17  |
| 264.00 | 66.40  | 62.33  |
| 0.00   | 0.00   | 0.00   |