
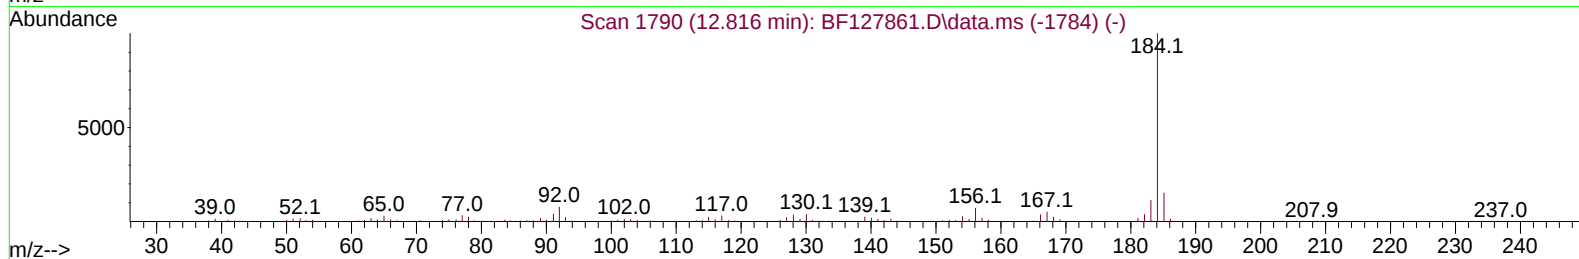
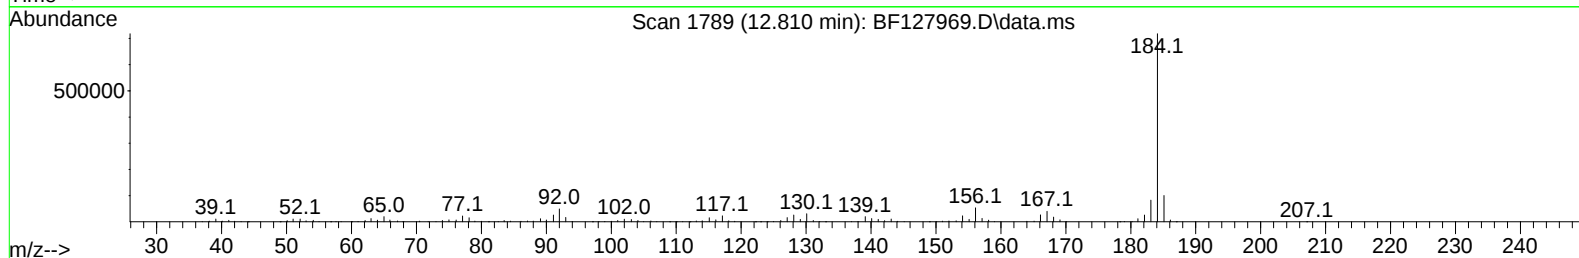


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042822\
 Data File : BF127969.D
 Acq On : 28 Apr 2022 09:30
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 28 17:39:21 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 28 05:13:03 2022
 Response via : Initial Calibration

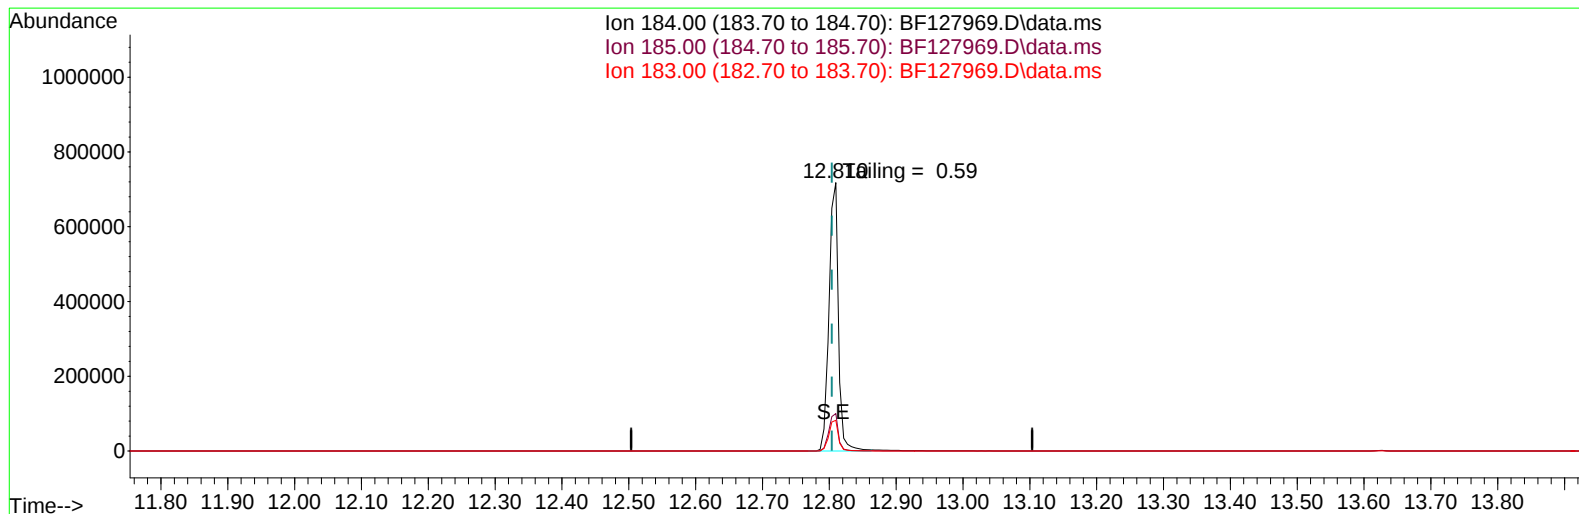

TIC: BF127969.D\data.ms

(77) Benzidine

12.810min (+ 0.006) 0.00 ng

response 709710

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	13.97
183.00	11.20	11.48
0.00	0.00	0.00