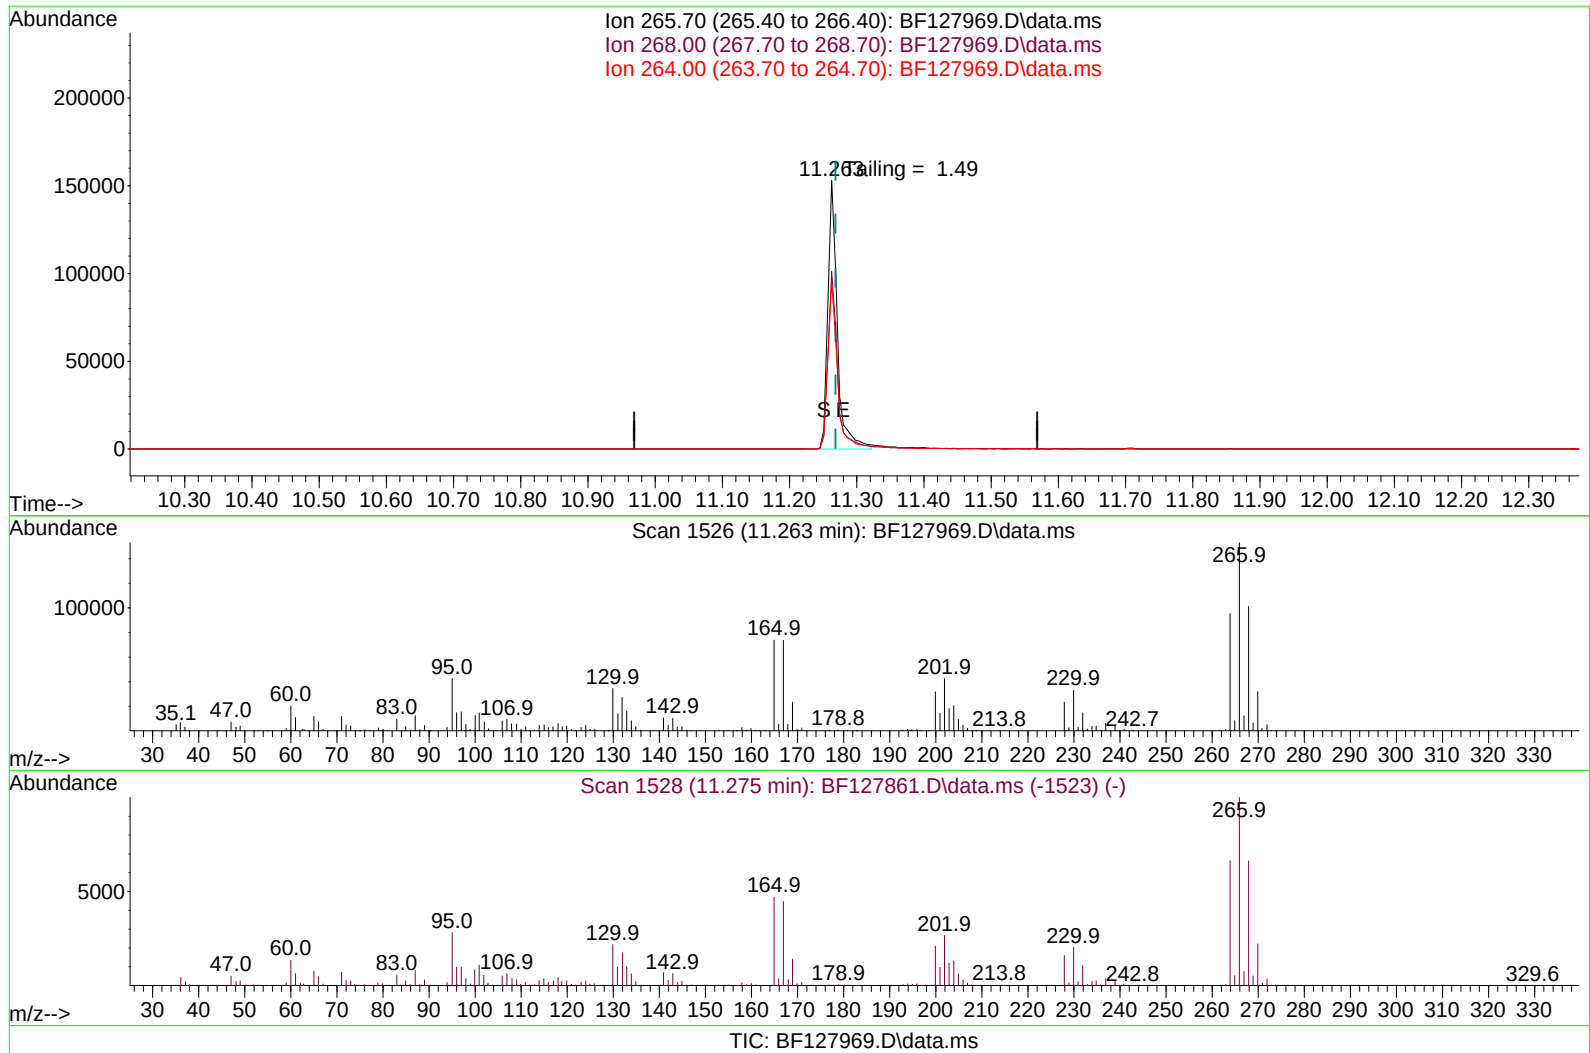


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042822\
Data File : BF127969.D
Acq On : 28 Apr 2022 09:30
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1




Quant Time: Apr 28 17:39:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 28 05:13:03 2022
Response via : Initial Calibration

**(70) Pentachlorophenol (C)****11.263min (-0.006) 28901.39 ng****response 154897**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.30	66.17
264.00	66.40	62.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042822\
 Data File : BF127969.D
 Acq On : 28 Apr 2022 09:30
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 28 17:39:21 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 28 05:13:03 2022
 Response via : Initial Calibration

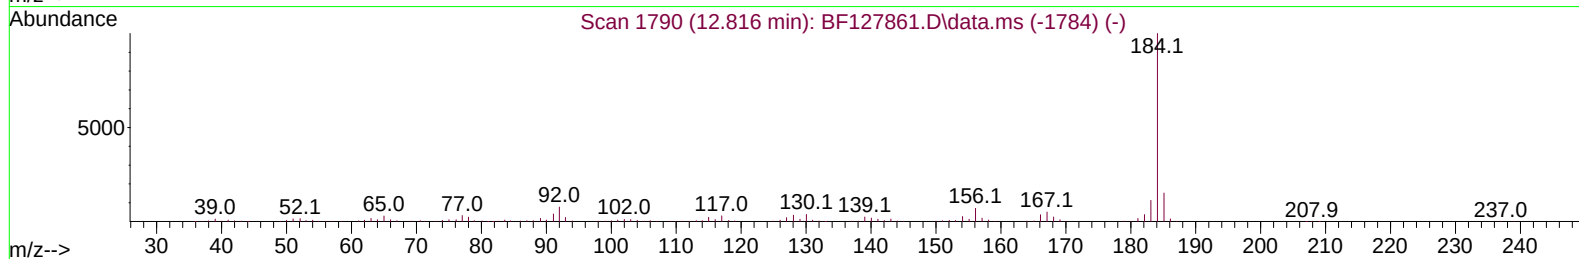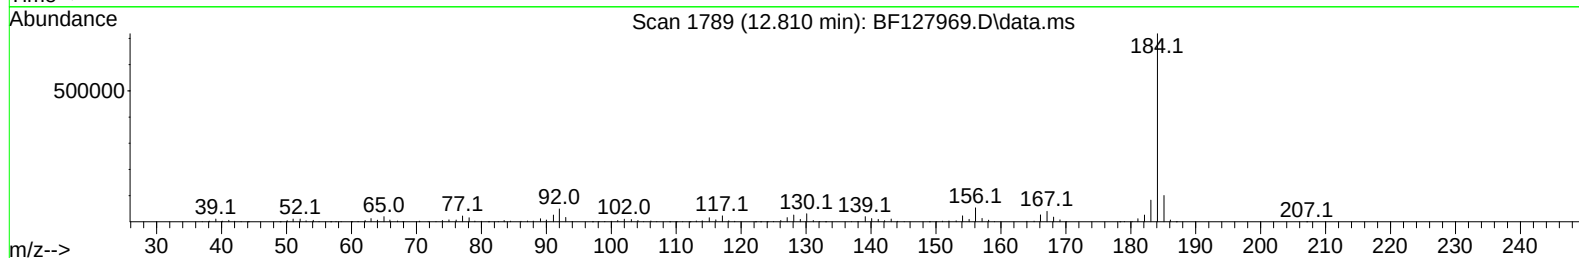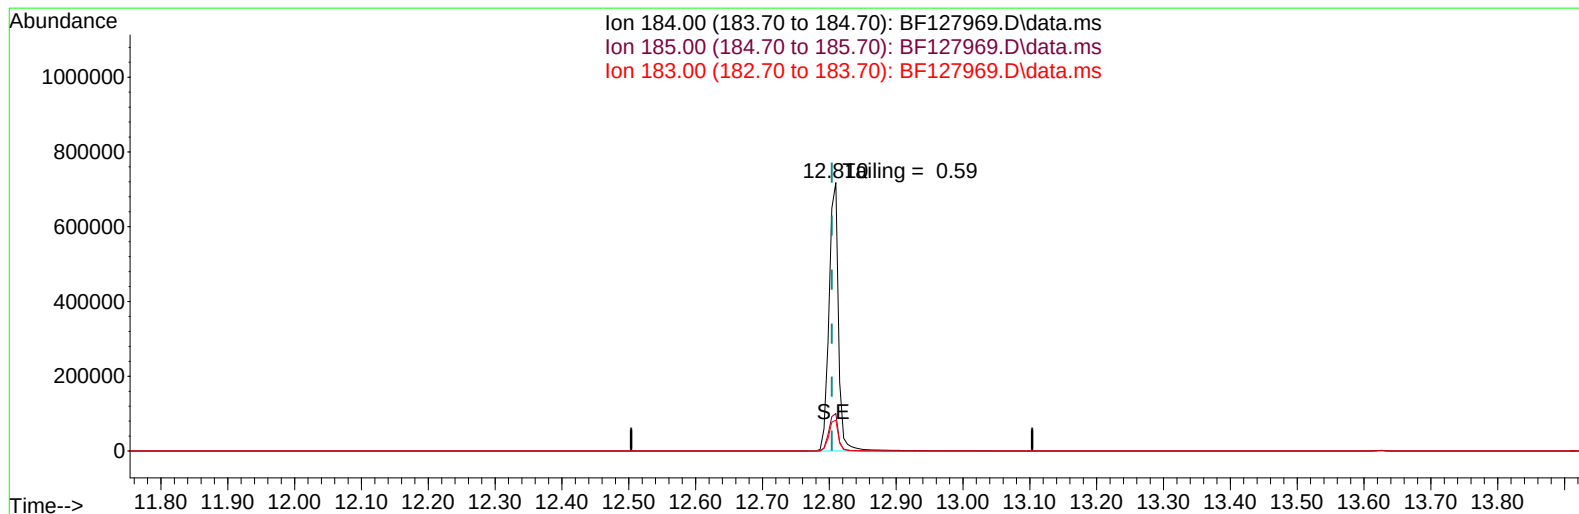

TIC: BF127969.D\data.ms

(77) Benzidine

12.810min (+ 0.006) 0.00 ng

response 709710

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	13.97
183.00	11.20	11.48
0.00	0.00	0.00