
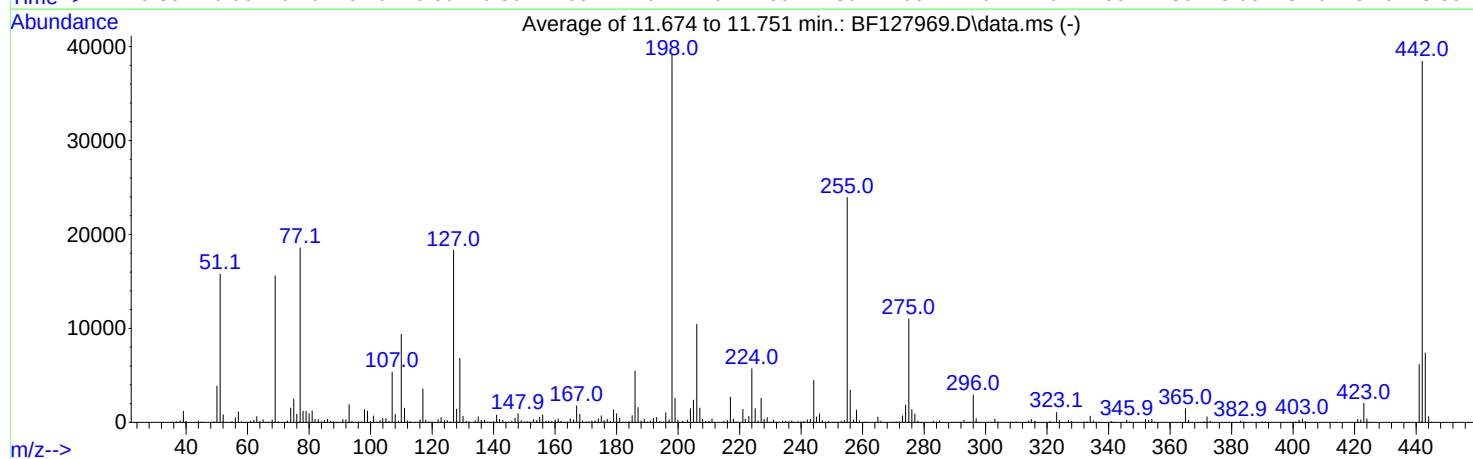


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042822\
 Data File : BF127969.D
 Acq On : 28 Apr 2022 09:30
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 28 05:13:03 2022

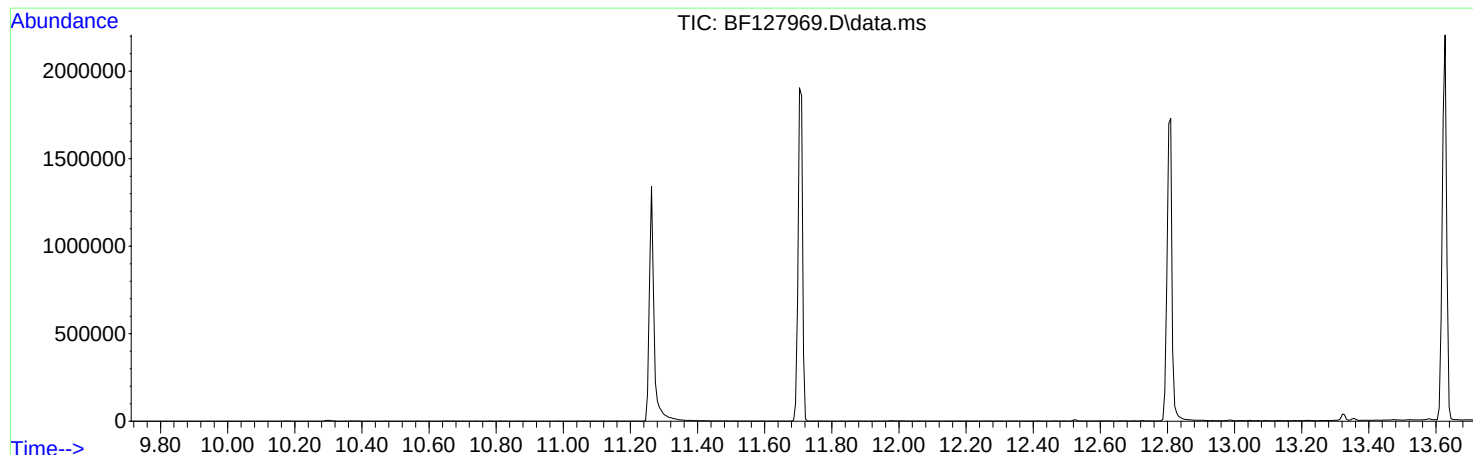


Spectrum Information: Average of 11.674 to 11.751 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.3	15767	PASS
68	69	0.00	2	1.8	279	PASS
69	198	0.00	100	39.9	15605	PASS
70	69	0.00	2	0.4	66	PASS
127	198	10	80	46.7	18302	PASS
197	198	0.00	2	0.7	279	PASS
198	198	100	100	100.0	39156	PASS
199	198	5	9	6.5	2564	PASS
275	198	10	60	28.1	11020	PASS
365	198	1	100	3.8	1472	PASS
441	198	0.01	100	15.7	6155	PASS
442	442	50	100	100.0	38449	PASS
443	442	15	24	19.2	7399	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042822\
Data File : BF127969.D
Acq On : 28 Apr 2022 09:30
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 28 17:39:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 28 05:13:03 2022
Response via : Initial Calibration

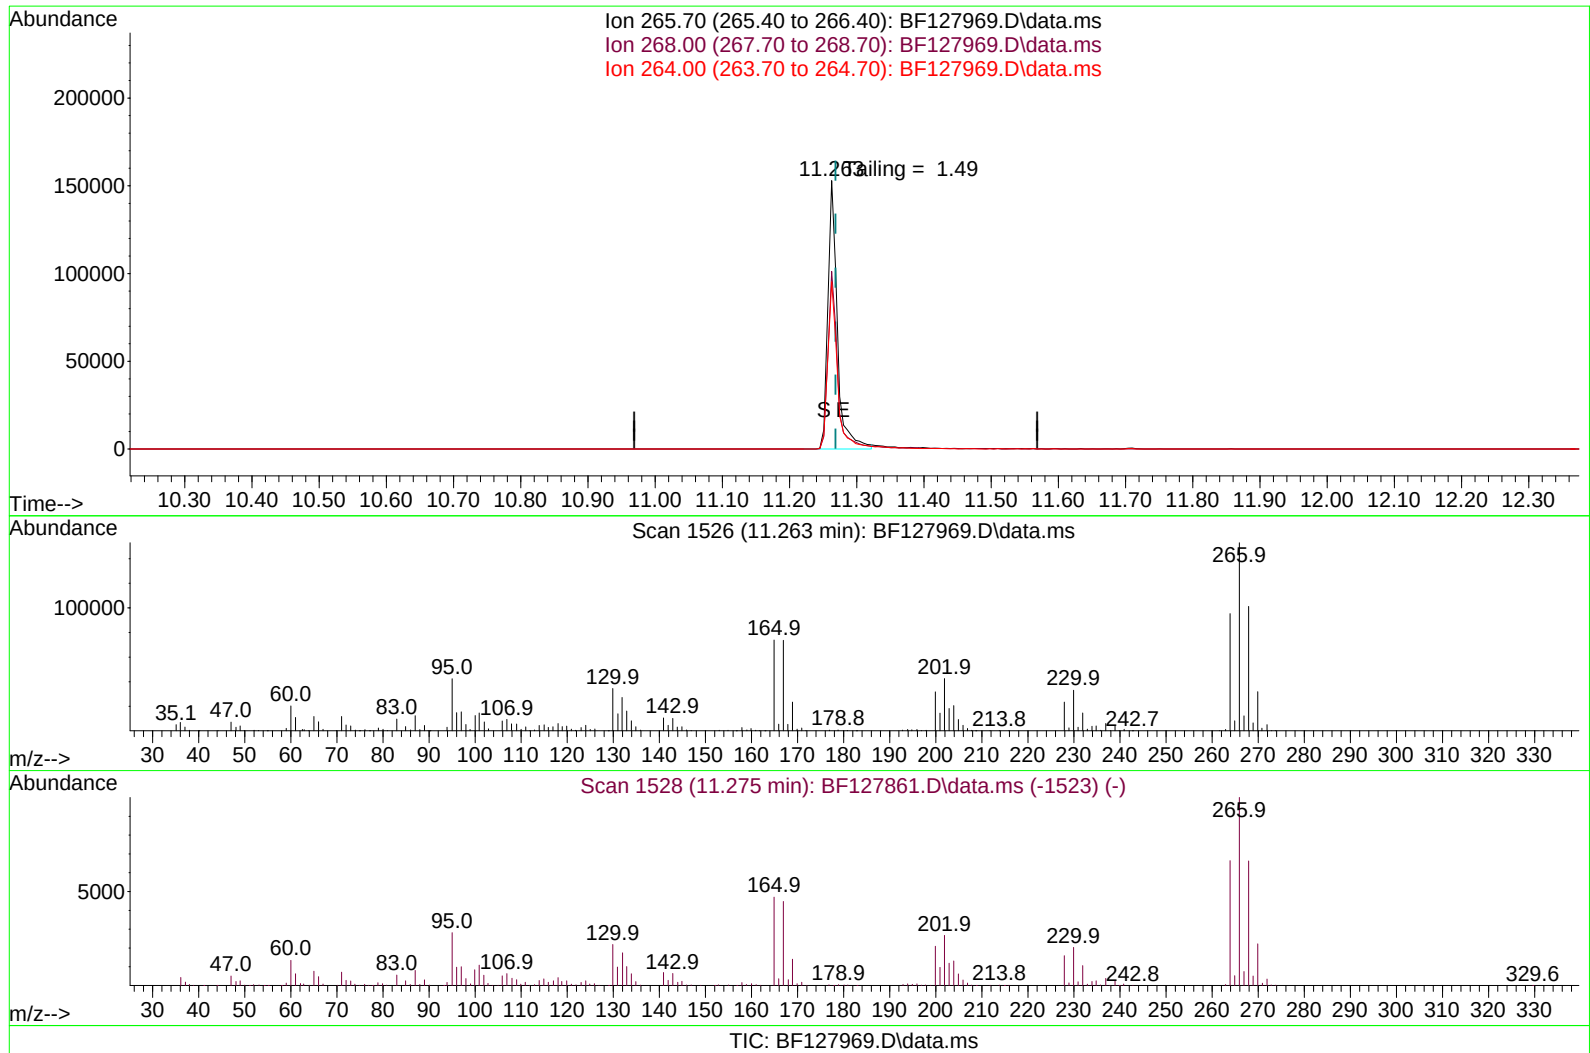

(70) Pentachlorophenol (C)

11.263min (-0.006) 28901.39 ng




response 154897

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.30	66.17
264.00	66.40	62.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042822\
 Data File : BF127969.D
 Acq On : 28 Apr 2022 09:30
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Apr 28 17:39:21 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 28 05:13:03 2022
 Response via : Initial Calibration

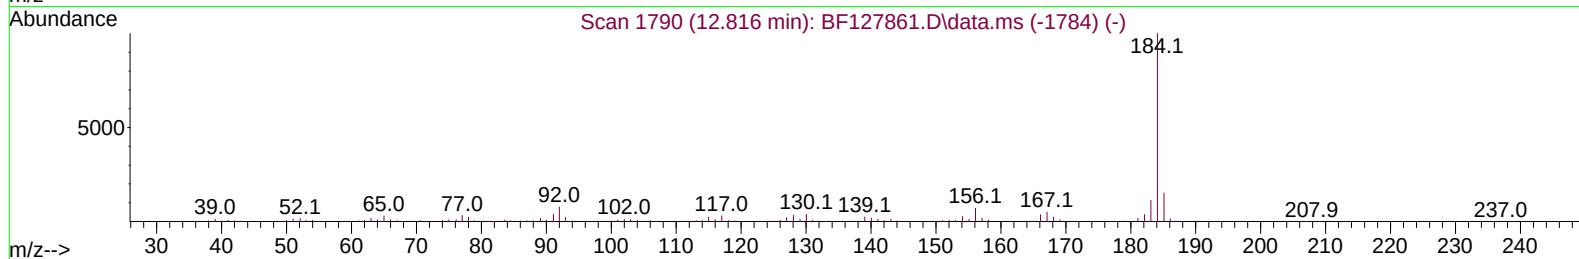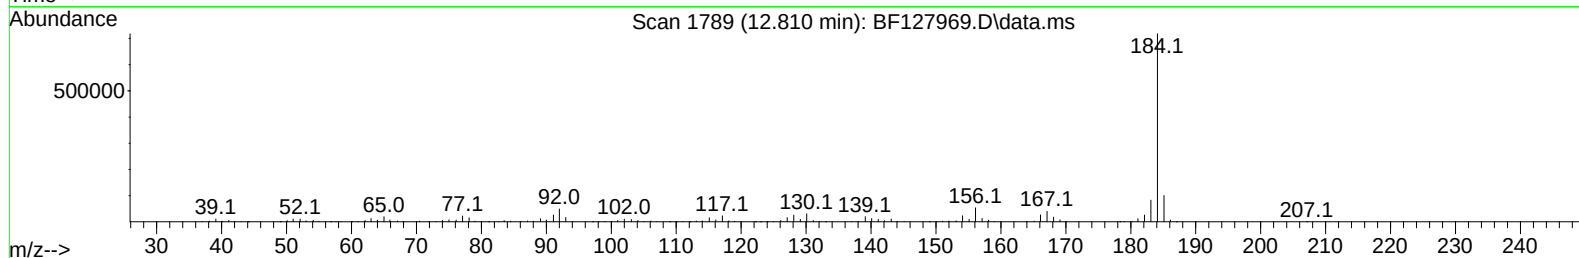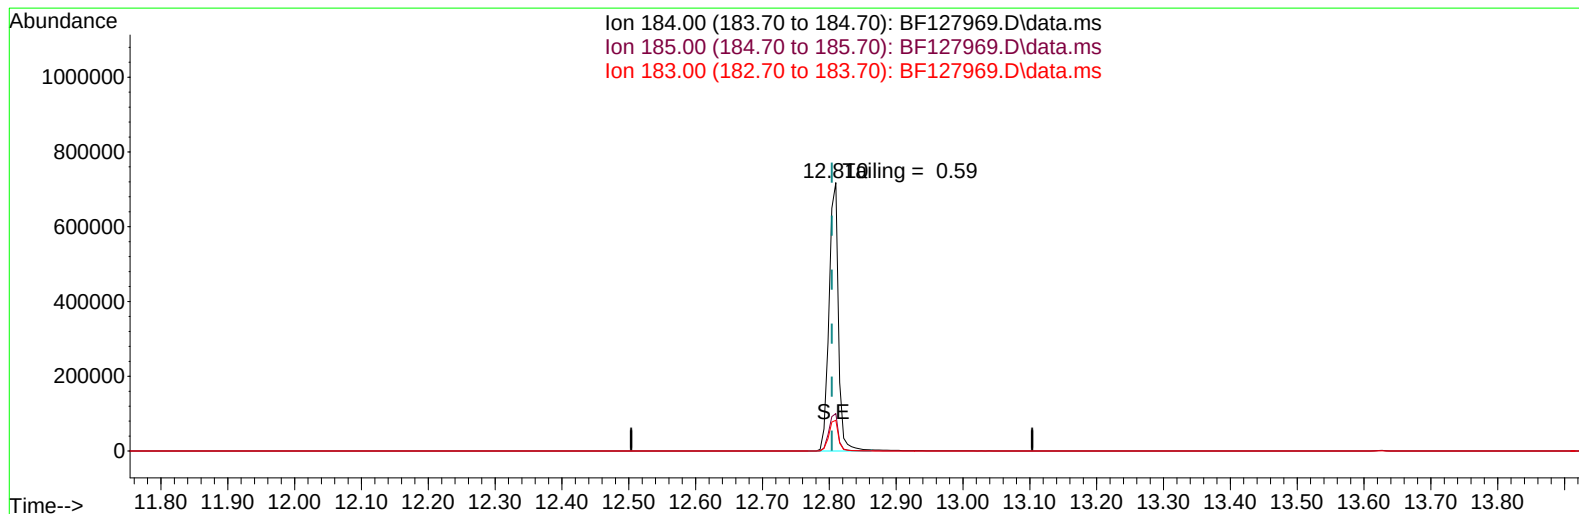

TIC: BF127969.D\data.ms

(77) Benzidine

12.810min (+ 0.006) 0.00 ng

response 709710

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	13.97
183.00	11.20	11.48
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/28/2022	BNA_F	<u>BF127969.D</u>
Compound Name	Response	Retention Time
DDT	381124	13.62
DDD	6859	13.32
DDE	855	12.99
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7714	388838	1.98

Instrument :
BNA_F
ClientSampleId :
DFTPP