
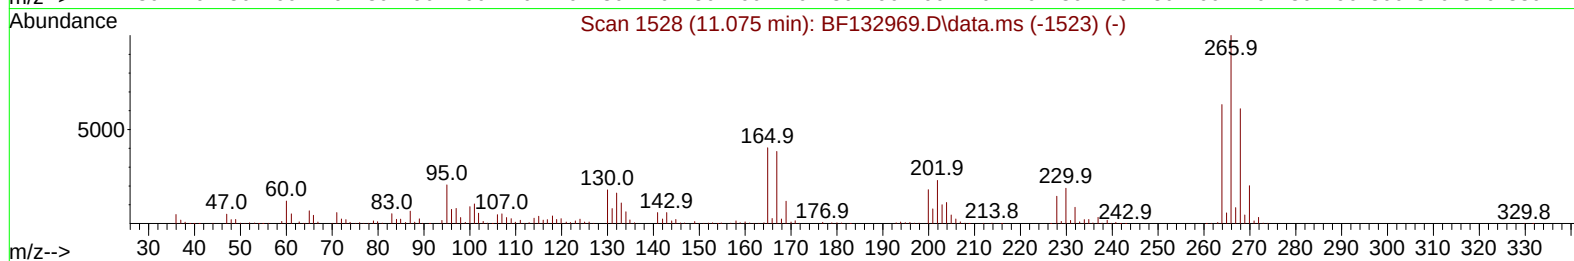
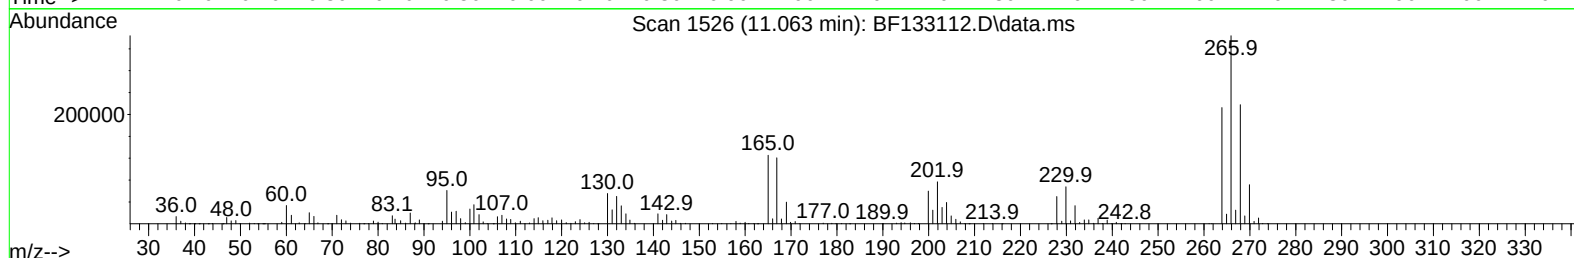


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042823\
 Data File : BF133112.D
 Acq On : 28 Apr 2023 09:14
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 28 11:54:10 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 28 02:00:53 2023
 Response via : Initial Calibration

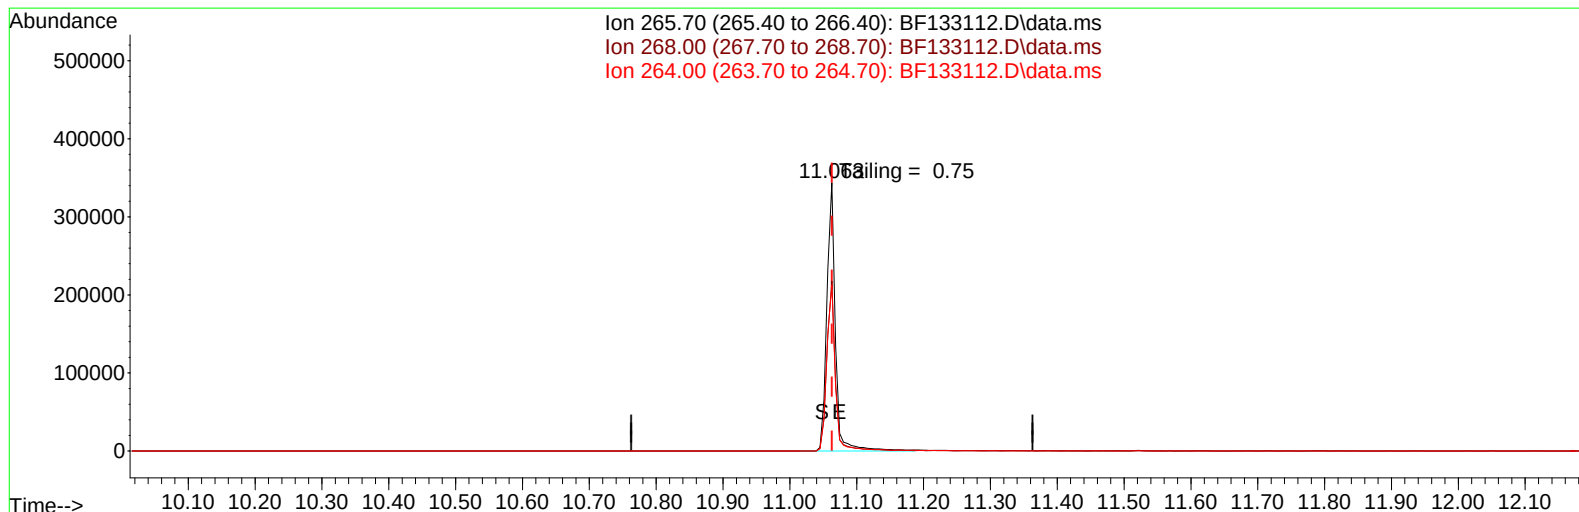

TIC: BF133112.D\data.ms

(70) Pentachlorophenol (C)




11.063min (-0.000) 30088.94 ng

response 307689

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	63.32
264.00	63.30	61.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042823\
 Data File : BF133112.D
 Acq On : 28 Apr 2023 09:14
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 28 11:54:10 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 28 02:00:53 2023
 Response via : Initial Calibration

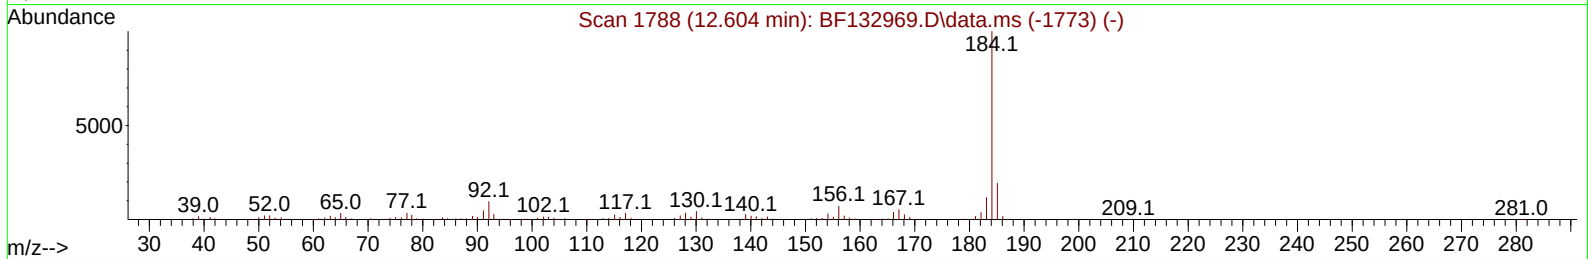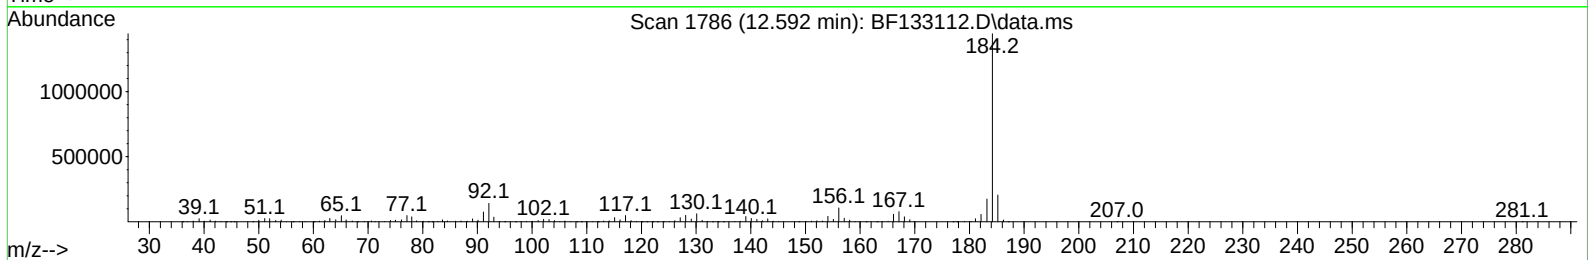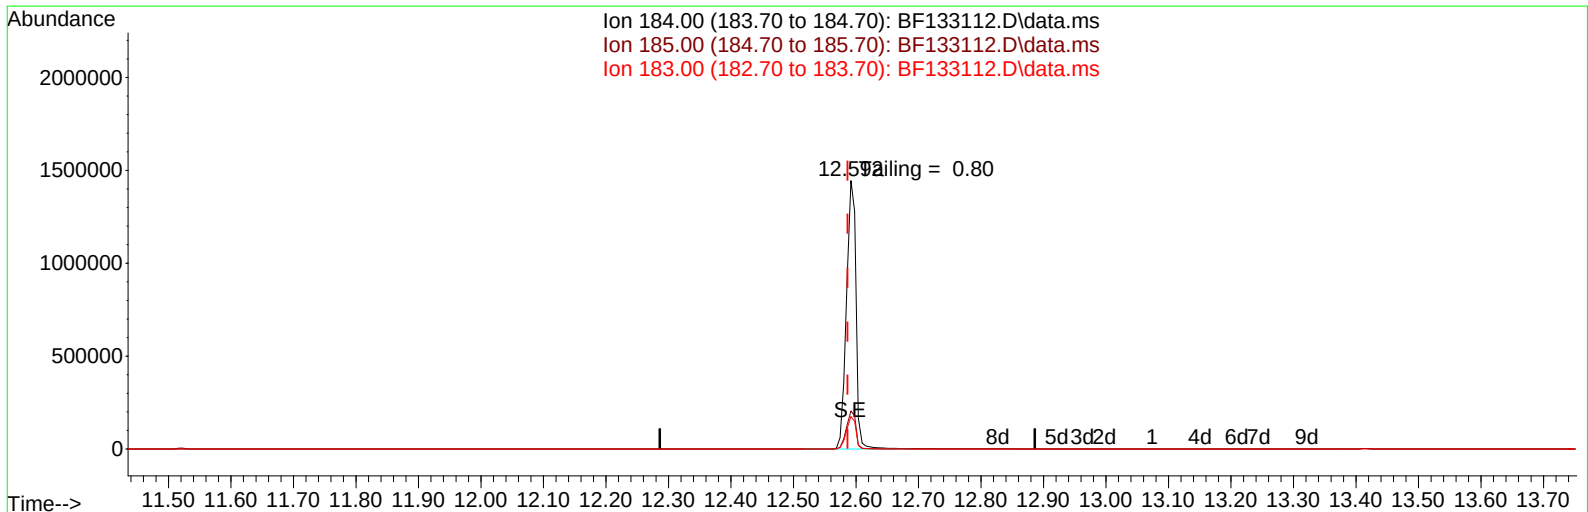

TIC: BF133112.D\data.ms

(77) Benzidine

12.592min (+ 0.006) 1661743.93 ng m

response 1545553

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	19.30	14.23#
183.00	11.70	12.10
0.00	0.00	0.00