
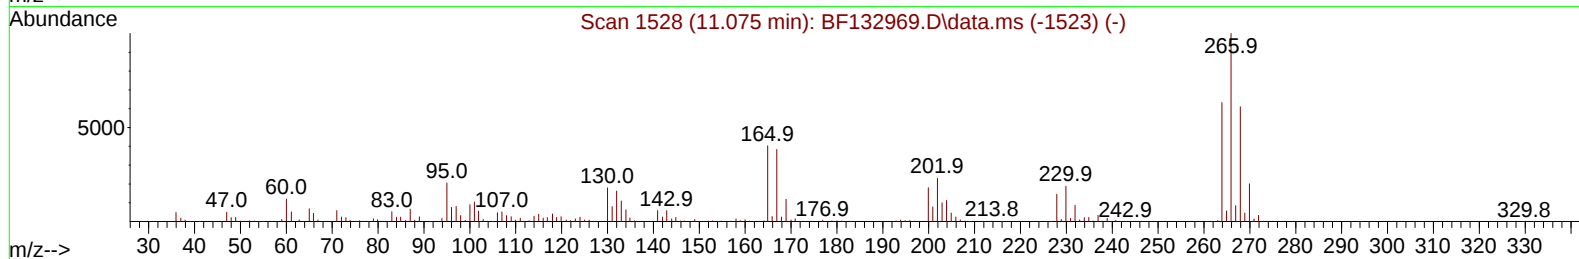
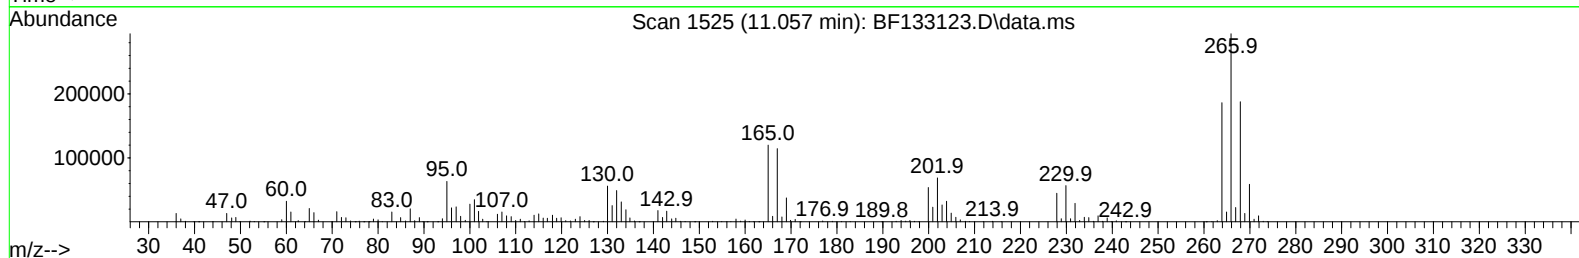


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042823\
Data File : BF133123.D
Acq On : 28 Apr 2023 15:46
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 28 17:13:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 28 12:18:20 2023
Response via : Initial Calibration

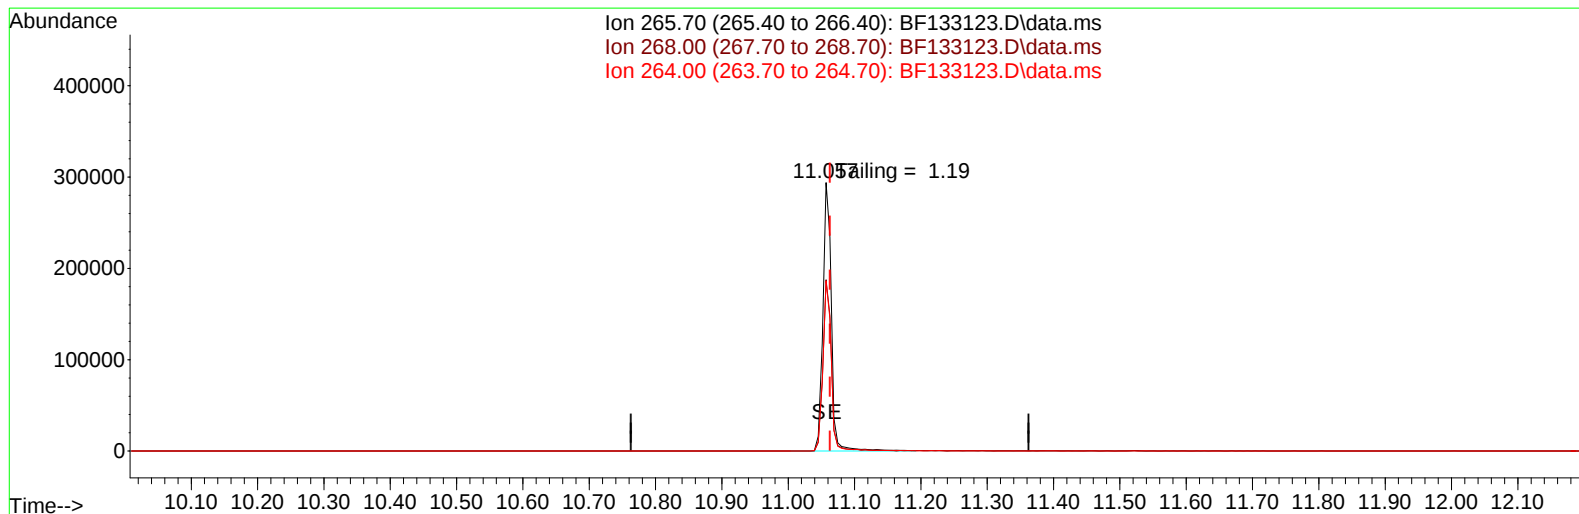

TIC: BF133123.D\data.ms

(70) Pentachlorophenol (C)




11.057min (-0.006) 284562.28 ng m

response 261263

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	63.83
264.00	63.30	63.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042823\
Data File : BF133123.D
Acq On : 28 Apr 2023 15:46
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 28 17:13:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 28 12:18:20 2023
Response via : Initial Calibration

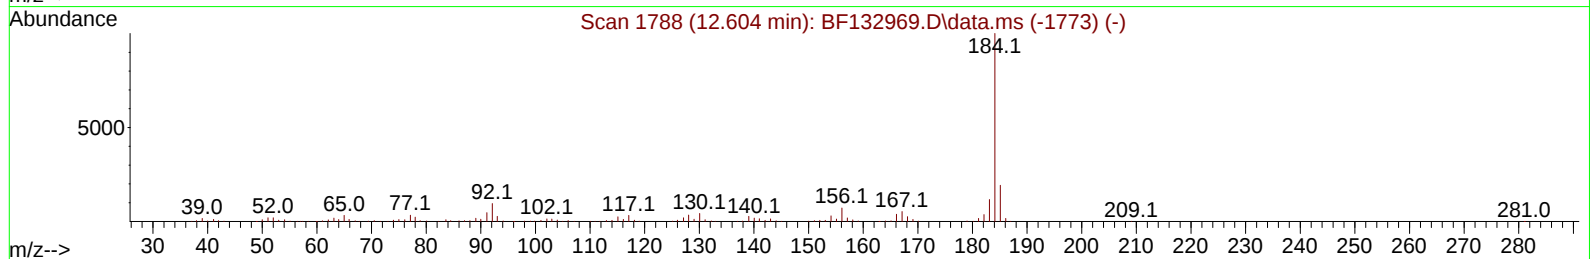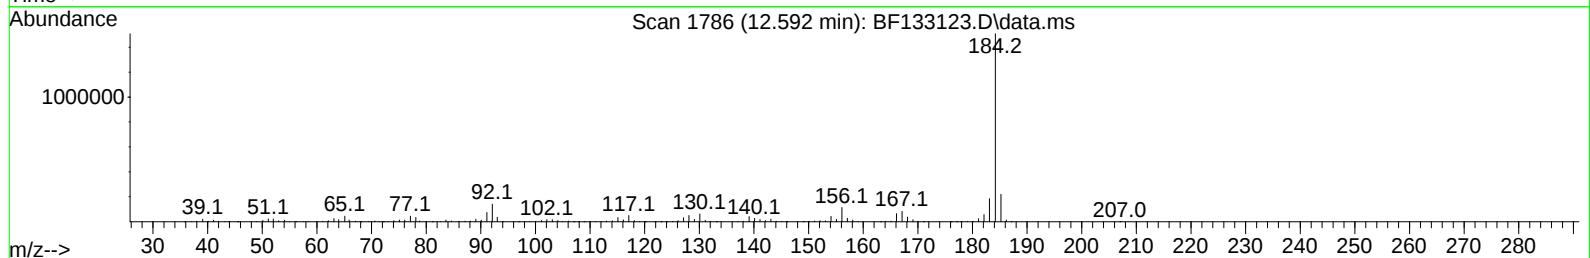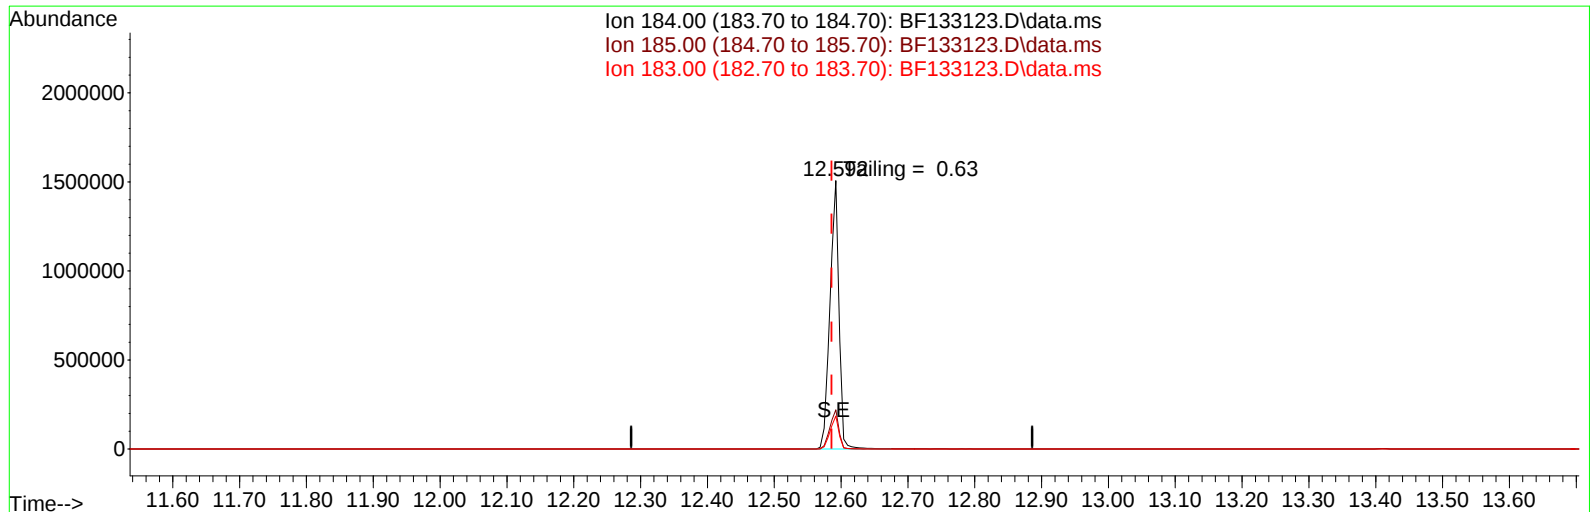

TIC: BF133123.D\data.ms

(77) Benzidine

12.592min (+ 0.006) 1062191.41 ng

response 1419015

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	19.30	14.62#
183.00	11.70	12.30
0.00	0.00	0.00