

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042823\
 Data File : BF133125.D
 Acq On : 28 Apr 2023 16:47
 Operator : CG\JU
 Sample : PB152433TB
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB152433TB

Quant Time: May 01 03:36:49 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 01 03:03:04 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.734	152	206063	20.000	ng	0.00
21) Naphthalene-d8	8.016	136	845279	20.000	ng	0.00
39) Acenaphthene-d10	9.769	164	458079	20.000	ng	0.00
64) Phenanthrene-d10	11.251	188	832705	20.000	ng	0.00
76) Chrysene-d12	13.886	240	601203	20.000	ng	0.00
86) Perylene-d12	15.304	264	539664	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.363	112	1624078	119.058	ng	0.02
7) Phenol-d6	6.381	99	1942806	114.746	ng	0.00
23) Nitrobenzene-d5	7.304	82	1193212	76.195	ng	0.00
42) 2,4,6-Tribromophenol	10.563	330	529989	115.043	ng	0.00
45) 2-Fluorobiphenyl	9.098	172	2047555	74.781	ng	0.00
79) Terphenyl-d14	12.845	244	2463863	70.681	ng	0.00


Target Compounds Qvalue


 (#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042823\
Data File : BF133125.D
Acq On : 28 Apr 2023 16:47
Operator : CG\JU
Sample : PB152433TB
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB152433TB

Quant Time: May 01 03:36:49 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 01 03:03:04 2023
Response via : Initial Calibration




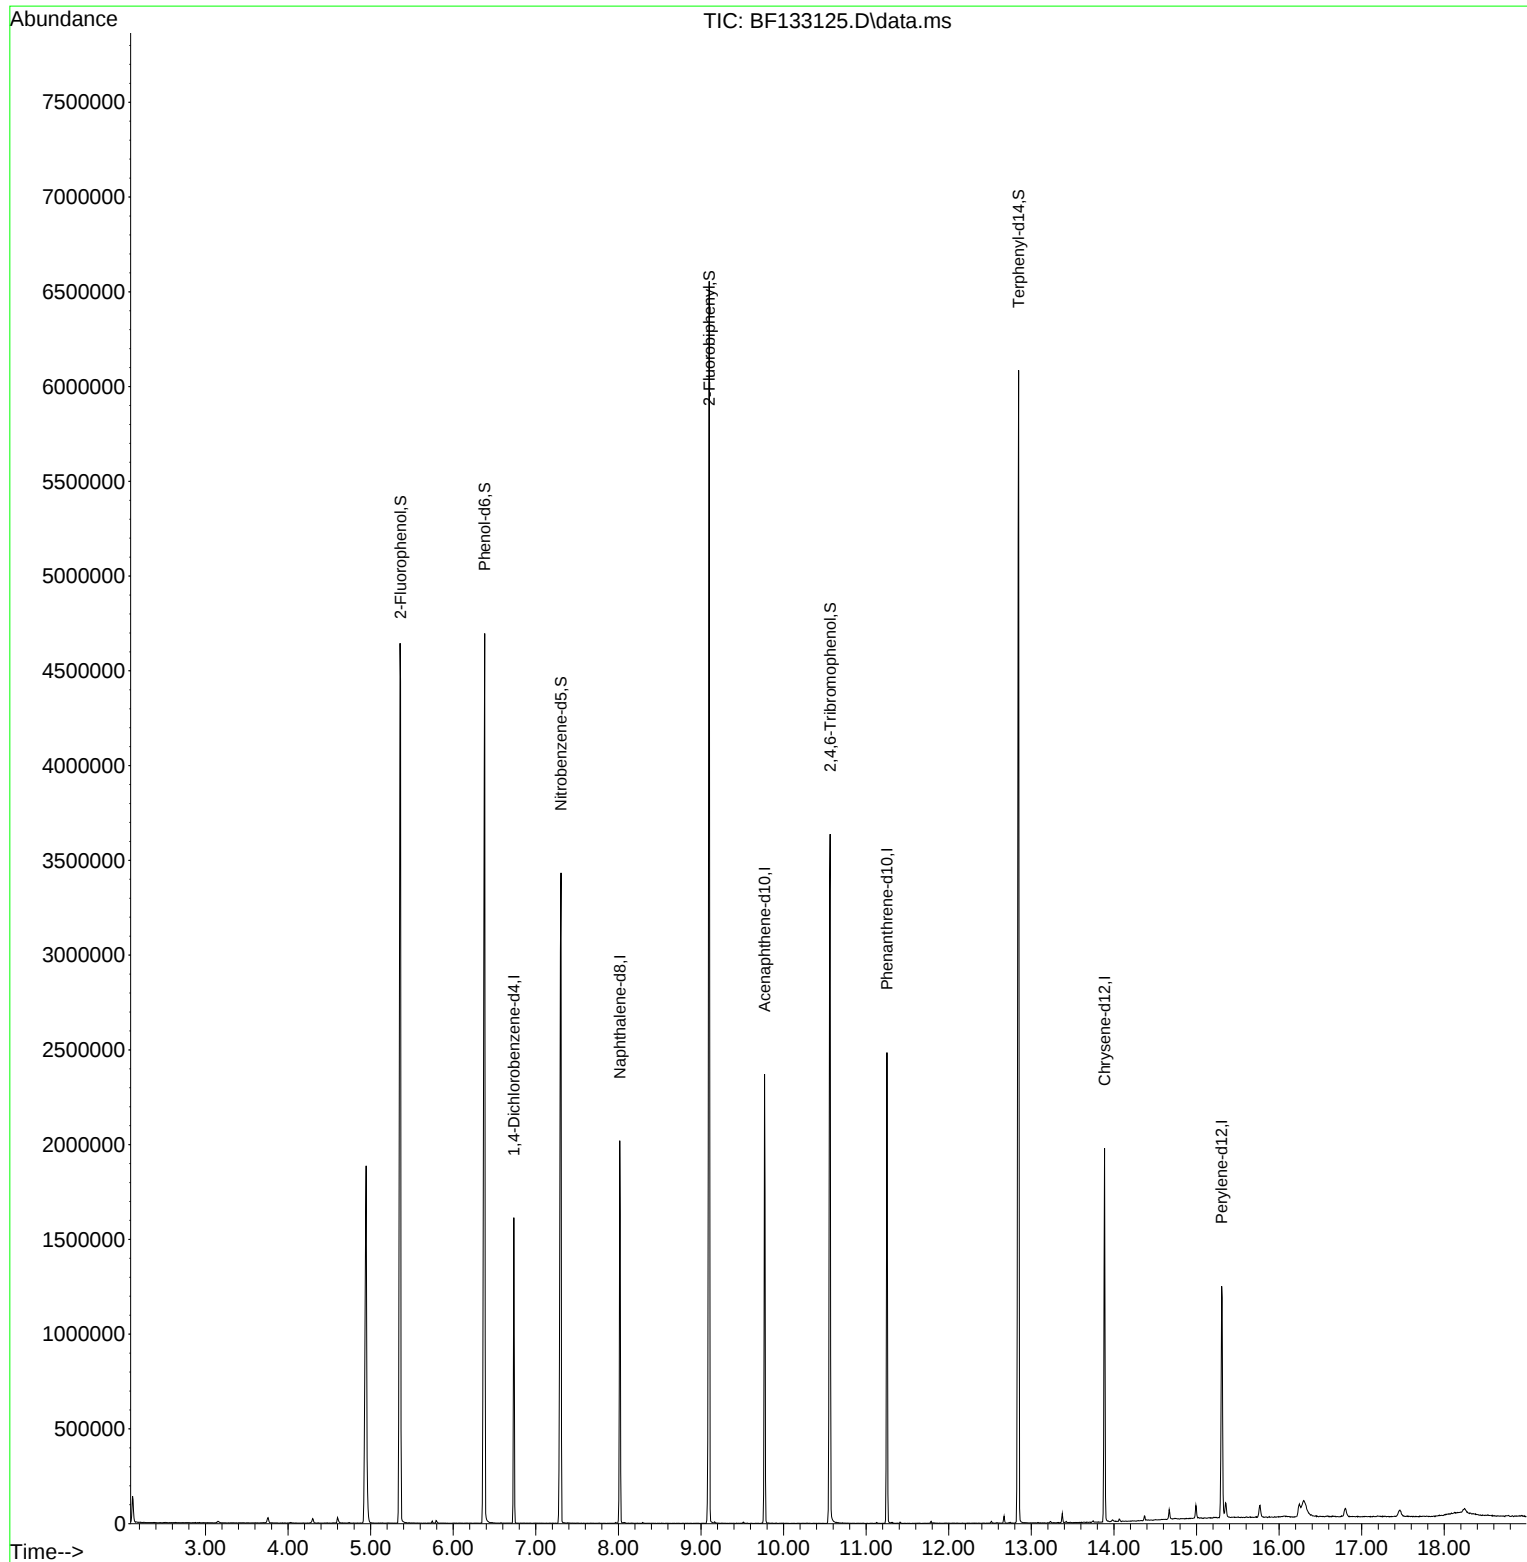


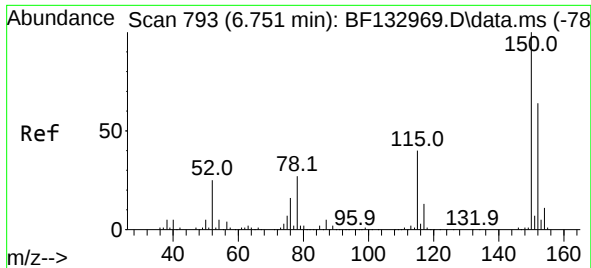

#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.734 min Scan# 793
 Delta R.T. -0.005 min
 Lab File: BF133125.D
 Acq: 28 Apr 2023 16:47




Instrument :
 BNA_F
 ClientSampleId :
 PB152433TB


Tgt Ion:152 Resp: 206063
 Ion Ratio Lower Upper
 152 100
 150 159.9 124.8 187.2
 115 62.8 49.9 74.9

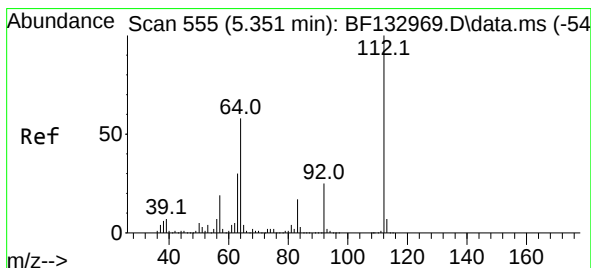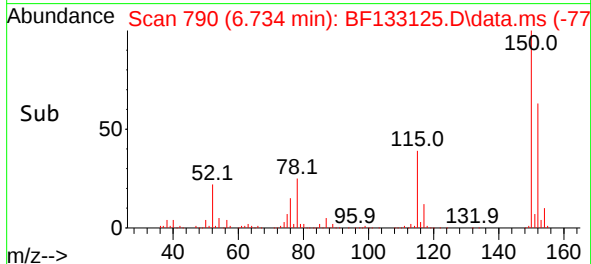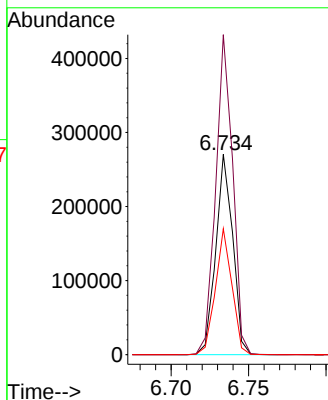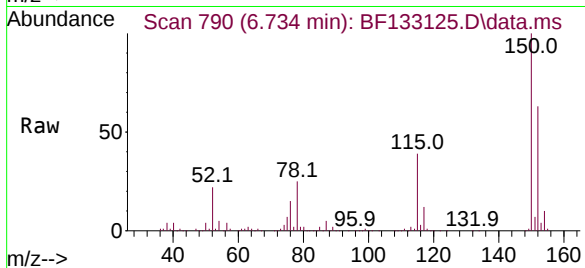

#5
 2-Fluorophenol
 Concen: 119.058 ng
 RT: 5.363 min Scan# 557
 Delta R.T. 0.024 min
 Lab File: BF133125.D
 Acq: 28 Apr 2023 16:47

Tgt Ion:112 Resp: 1624078
 Ion Ratio Lower Upper
 112 100
 64 52.9 46.8 70.2
 63 26.9 23.8 35.8


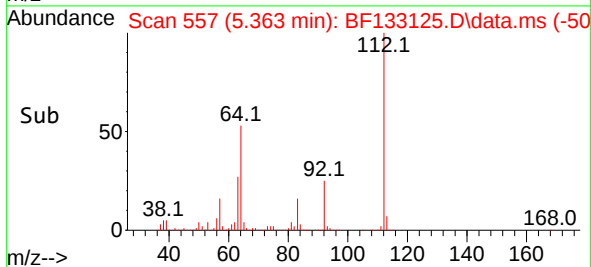
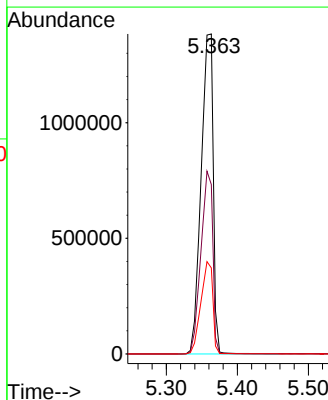
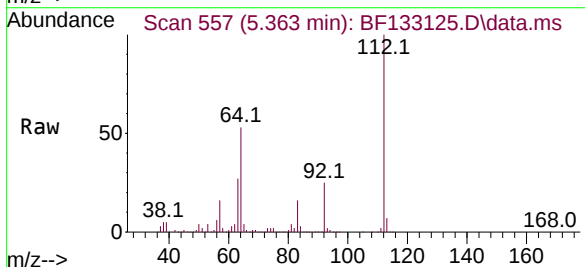


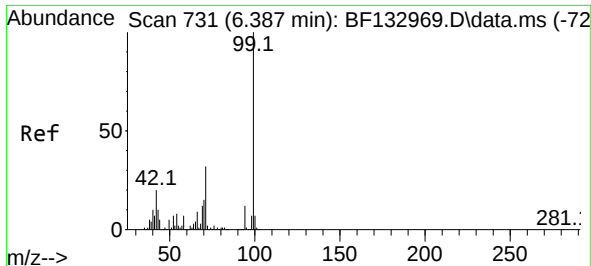

#7
Phenol-d6
Concen: 114.746 ng
RT: 6.381 min Scan# 731
Delta R.T. 0.000 min
Lab File: BF133125.D
Acq: 28 Apr 2023 16:47




Instrument :
BNA_F
ClientSampleId :
PB152433TB


Tgt Ion: 99 Resp: 1942806
Ion Ratio Lower Upper
99 100
42 18.3 16.3 24.5
71 32.0 25.6 38.4

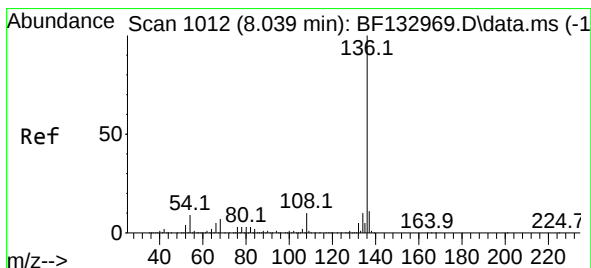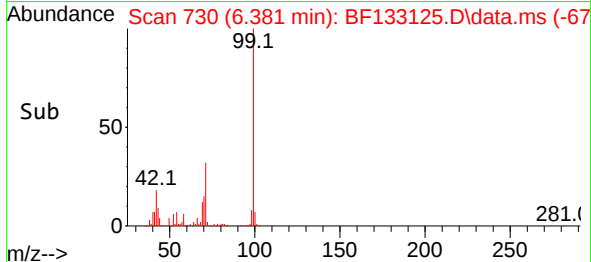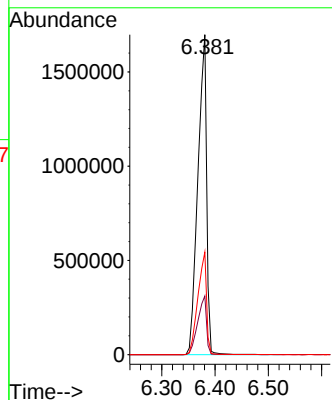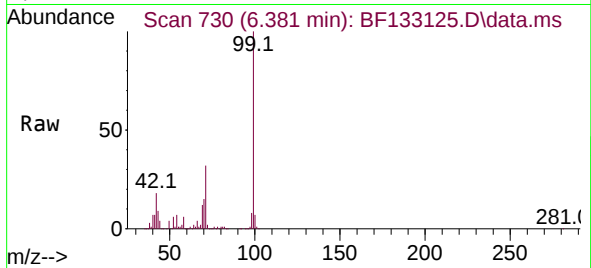

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.016 min Scan# 1008
Delta R.T. -0.006 min
Lab File: BF133125.D
Acq: 28 Apr 2023 16:47

Tgt Ion: 136 Resp: 845279
Ion Ratio Lower Upper
136 100
137 11.2 8.6 13.0
54 9.5 7.0 10.4
68 7.5 5.4 8.2

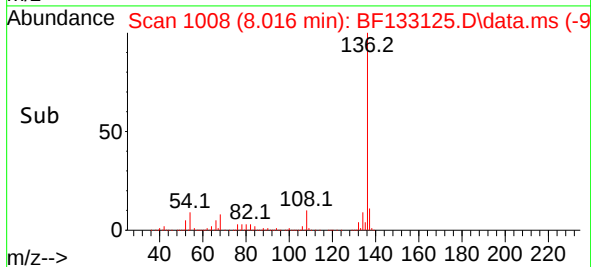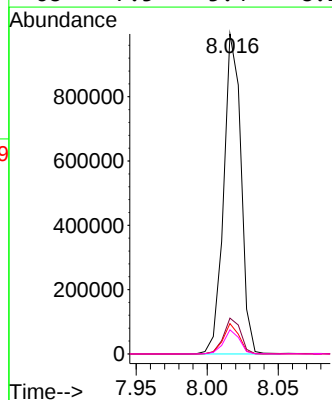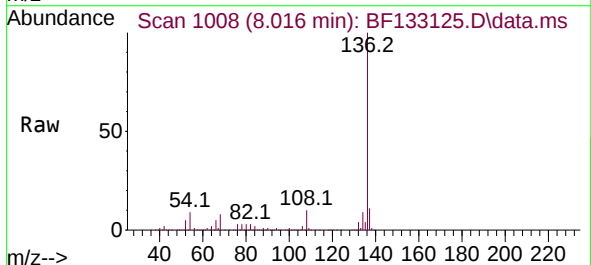




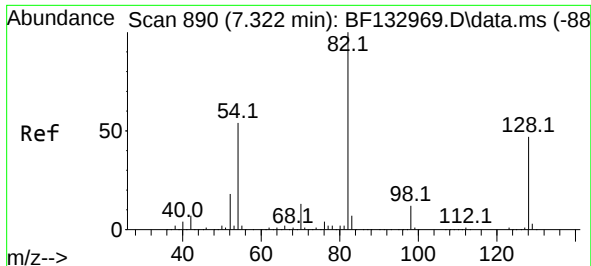


#23
Nitrobenzene-d5
Concen: 76.195 ng
RT: 7.304 min Scan# 81
Delta R.T. 0.000 min
Lab File: BF133125.D
Acq: 28 Apr 2023 16:47

Instrument :
BNA_F
ClientSampleId :
PB152433TB

Tgt Ion: 82 Resp: 1193212




Ion	Ratio	Lower	Upper
82	100		
128	49.2	37.7	56.5
54	50.4	43.0	64.4

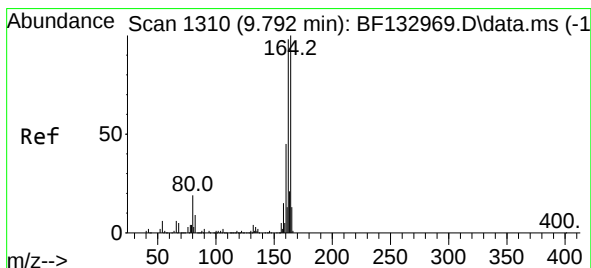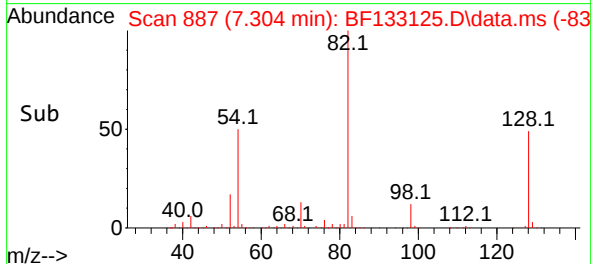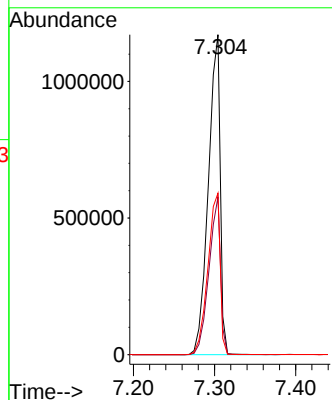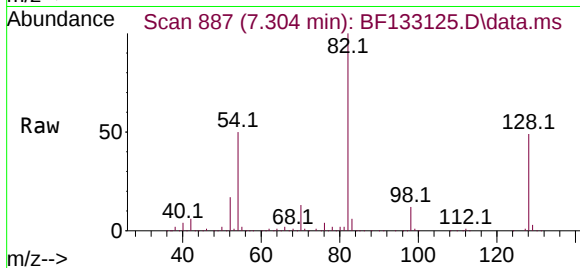


#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.769 min Scan# 1306
Delta R.T. -0.006 min
Lab File: BF133125.D
Acq: 28 Apr 2023 16:47

Tgt Ion:164 Resp: 458079


Ion	Ratio	Lower	Upper
164	100		
162	96.7	78.7	118.1
160	43.3	35.8	53.6

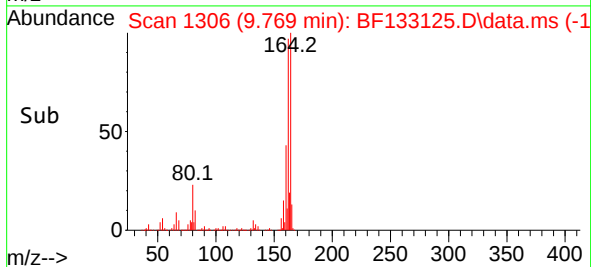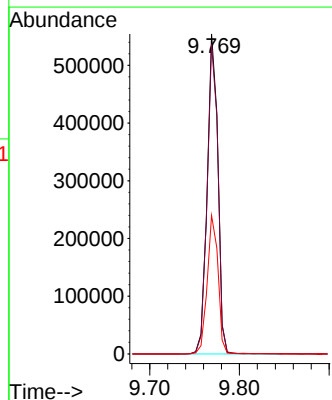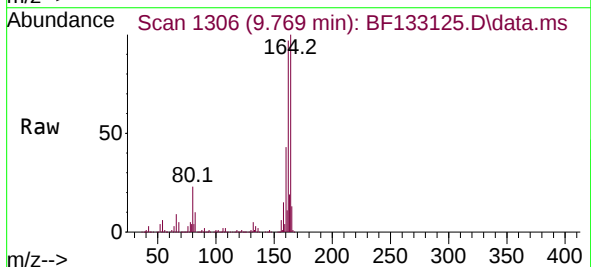



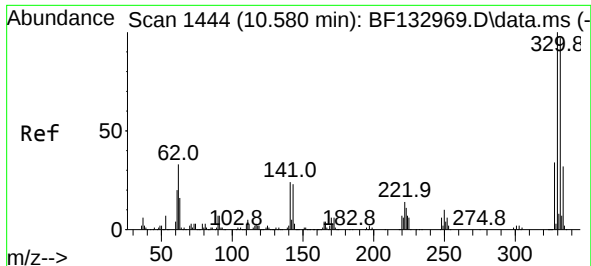


#42
2,4,6-Tribromophenol
Concen: 115.043 ng
RT: 10.563 min Scan# 1444
Delta R.T. 0.000 min
Lab File: BF133125.D
Acq: 28 Apr 2023 16:47

Instrument :
BNA_F
ClientSampleId :
PB152433TB



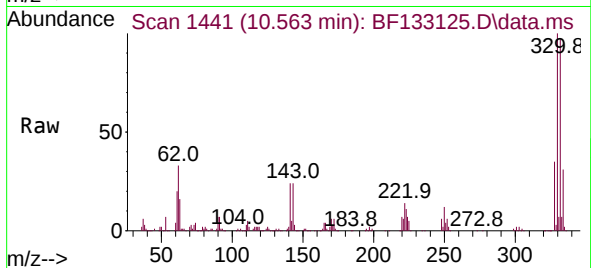



Tgt Ion:330 Resp: 529989
Ion Ratio Lower Upper
330 100
332 96.8 77.1 115.7
141 28.5 25.8 38.8

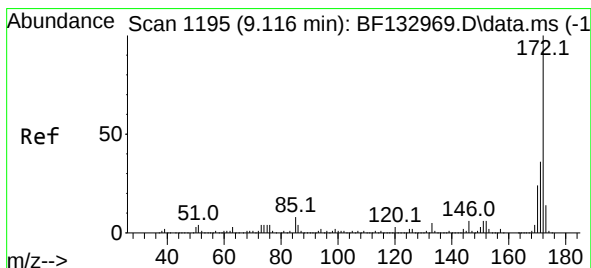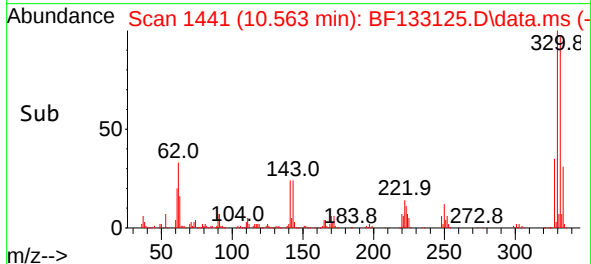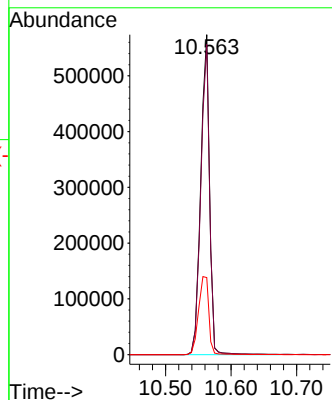

#45
2-Fluorobiphenyl
Concen: 74.781 ng
RT: 9.098 min Scan# 1192
Delta R.T. 0.000 min
Lab File: BF133125.D
Acq: 28 Apr 2023 16:47

Tgt Ion:172 Resp: 2047555
Ion Ratio Lower Upper
172 100
171 36.7 28.8 43.2
170 23.9 19.4 29.2


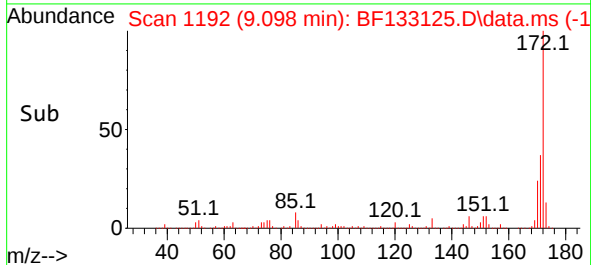
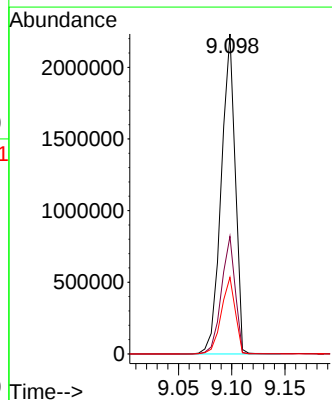
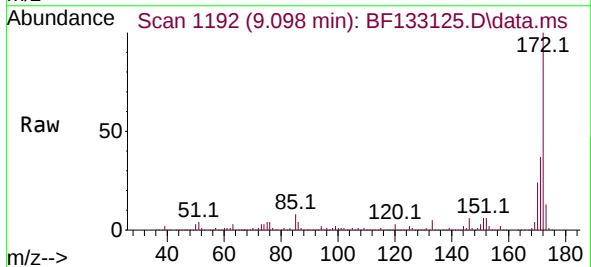


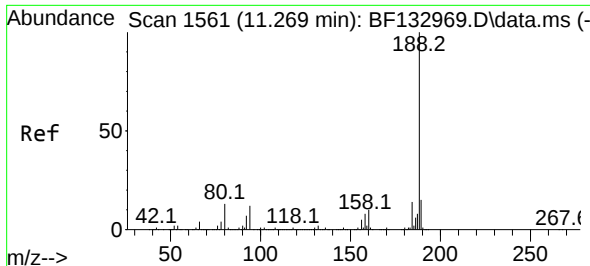

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.251 min Scan# 11
Delta R.T. 0.000 min
Lab File: BF133125.D
Acq: 28 Apr 2023 16:47




Instrument :
BNA_F
ClientSampleId :
PB152433TB


Tgt Ion:188 Resp: 832705
Ion Ratio Lower Upper
188 100
94 11.3 9.7 14.5
80 12.2 10.4 15.6

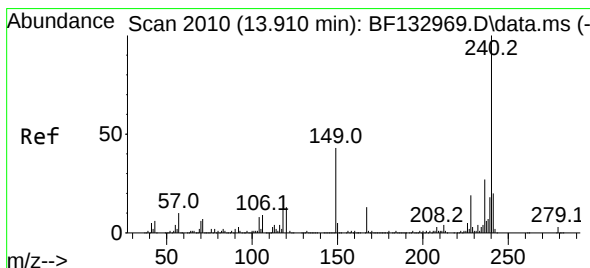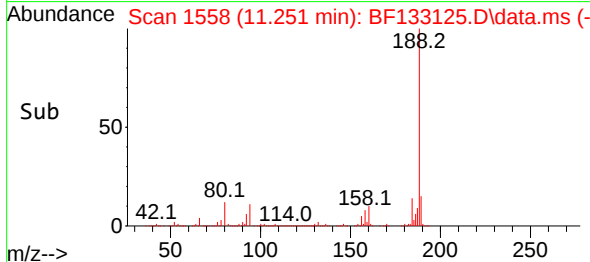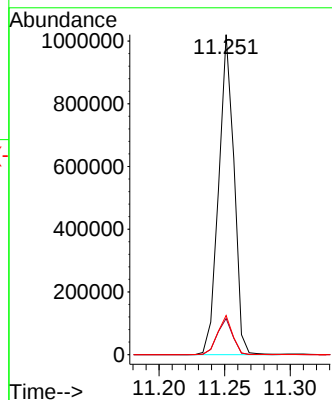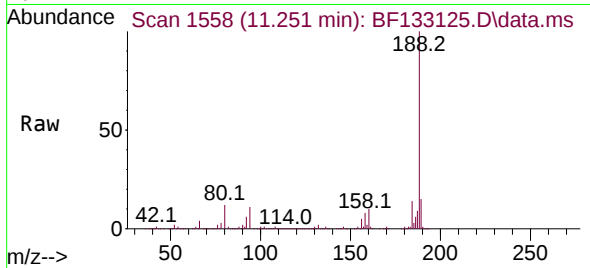

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.886 min Scan# 2006
Delta R.T. -0.006 min
Lab File: BF133125.D
Acq: 28 Apr 2023 16:47

Tgt Ion:240 Resp: 601203
Ion Ratio Lower Upper
240 100
120 13.7 10.5 15.7
236 25.7 21.5 32.3

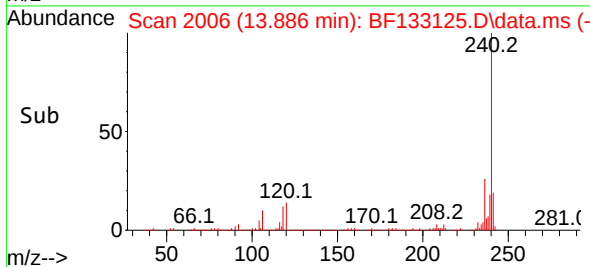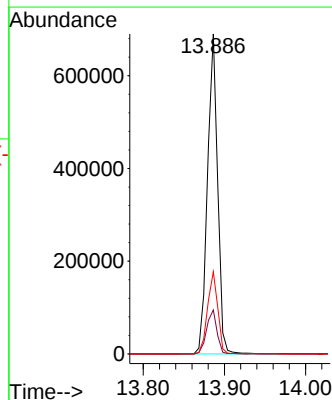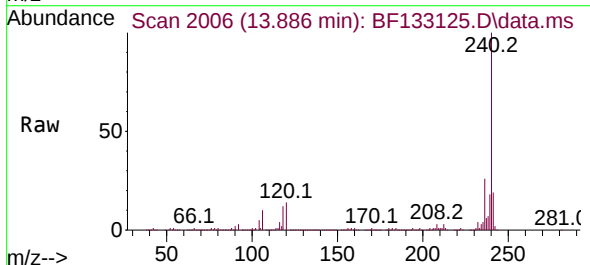

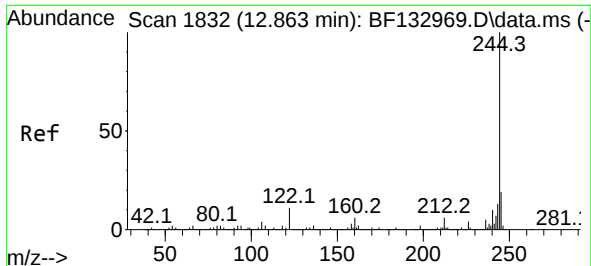

#79

Terphenyl-d14

Concen: 70.681 ng

RT: 12.845 min Scan# 1832

Delta R.T. 0.006 min

Lab File: BF133125.D

Acq: 28 Apr 2023 16:47

Instrument :

BNA_F

ClientSampleId :

PB152433TB





Tgt Ion:244 Resp: 2463863

Ion Ratio Lower Upper

244 100

212 6.4 5.1 7.7

122 11.5 8.6 13.0

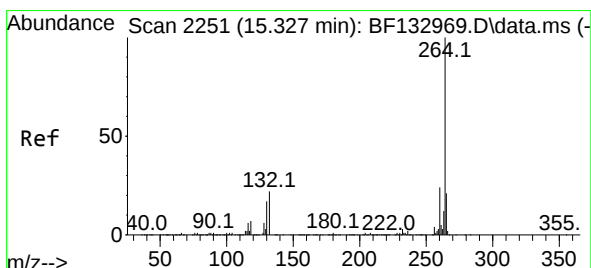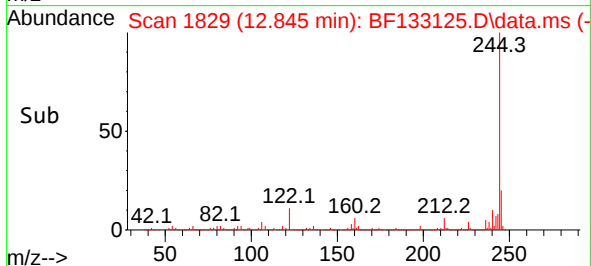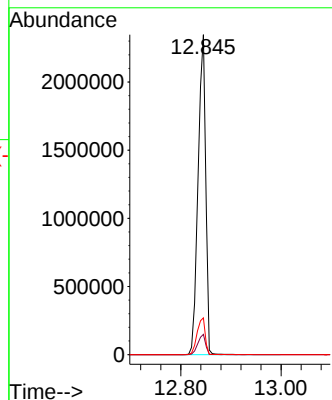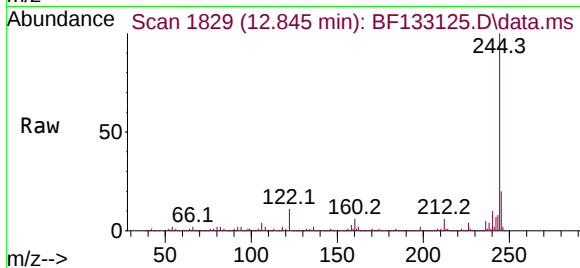

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.304 min Scan# 2247

Delta R.T. -0.006 min

Lab File: BF133125.D

Acq: 28 Apr 2023 16:47

Tgt Ion:264 Resp: 539664

Ion Ratio Lower Upper

264 100

260 24.1 18.8 28.2

265 21.9 17.0 25.4

