

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042823\
 Data File : BF133135.D
 Acq On : 28 Apr 2023 22:27
 Operator : CG\JU
 Sample : 02504-16
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 BU-512-COMP-03

Quant Time: May 01 03:09:02 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 01 03:03:04 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.734	152	174675	20.000	ng	0.00
21) Naphthalene-d8	8.016	136	695867	20.000	ng	0.00
39) Acenaphthene-d10	9.769	164	362320	20.000	ng	0.00
64) Phenanthrene-d10	11.251	188	658226	20.000	ng	0.00
76) Chrysene-d12	13.880	240	492366	20.000	ng	-0.01
86) Perylene-d12	15.304	264	379092	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.357	112	1468198	126.971	ng	0.02
7) Phenol-d6	6.375	99	1654070	115.247	ng	0.00
23) Nitrobenzene-d5	7.298	82	1210457	93.892	ng	0.00
42) 2,4,6-Tribromophenol	10.557	330	527272	144.703	ng	0.00
45) 2-Fluorobiphenyl	9.098	172	1964393	90.705	ng	0.00
79) Terphenyl-d14	12.839	244	2442252	85.548	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042823\
Data File : BF133135.D
Acq On : 28 Apr 2023 22:27
Operator : CG\JU
Sample : 02504-16
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BU-512-COMP-03

Quant Time: May 01 03:09:02 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 01 03:03:04 2023
Response via : Initial Calibration




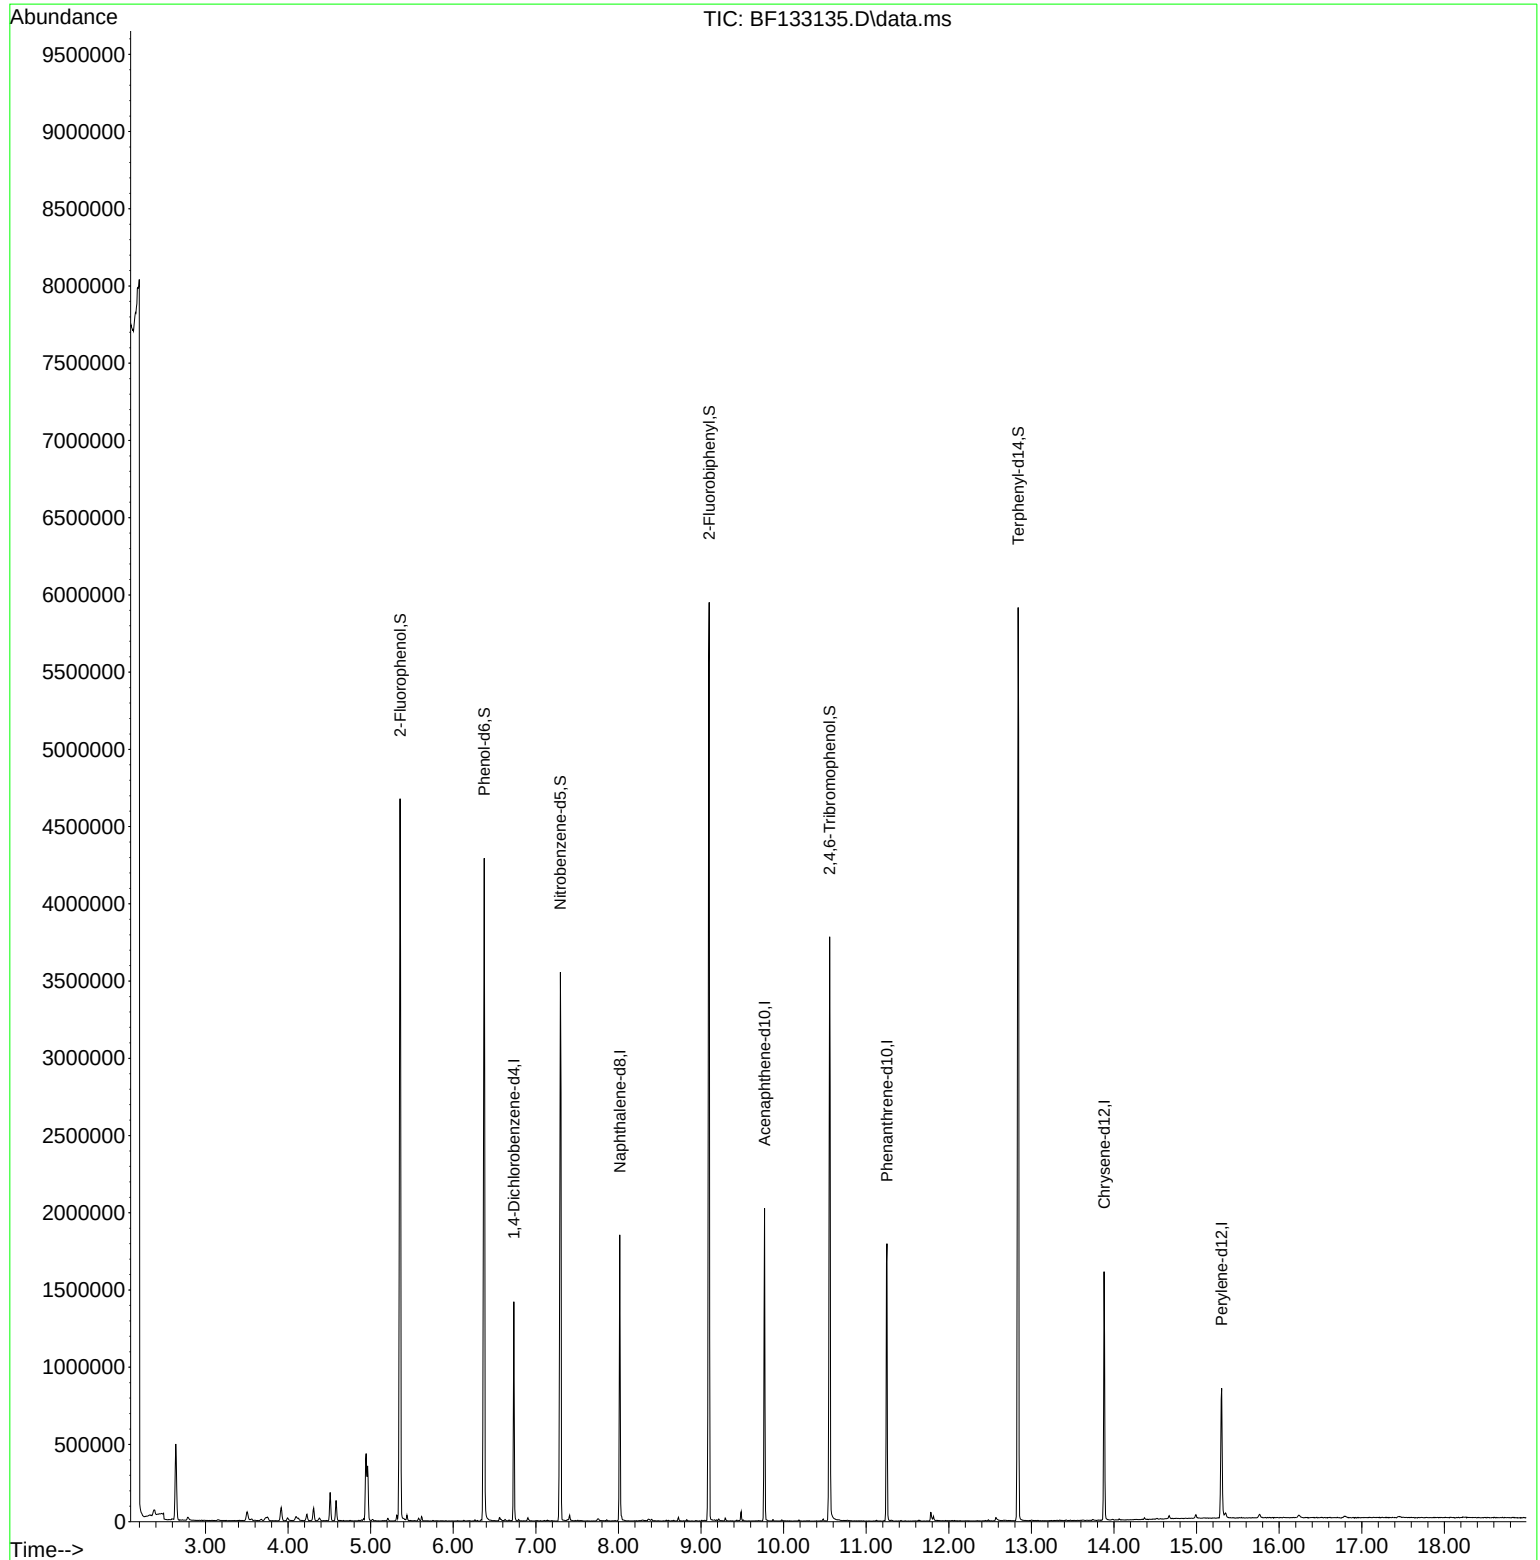


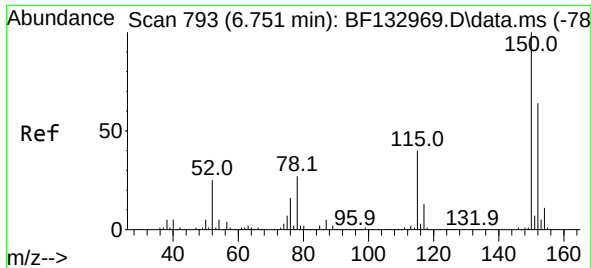

#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.734 min Scan# 793
 Delta R.T. -0.005 min
 Lab File: BF133135.D
 Acq: 28 Apr 2023 22:27




Instrument :
 BNA_F
 ClientSampleId :
 BU-512-COMP-03


Tgt Ion:152 Resp: 174675
 Ion Ratio Lower Upper
 152 100
 150 157.6 124.8 187.2
 115 63.8 49.9 74.9

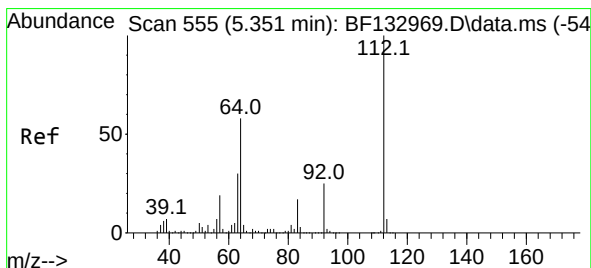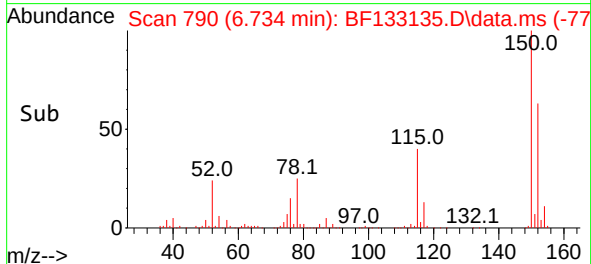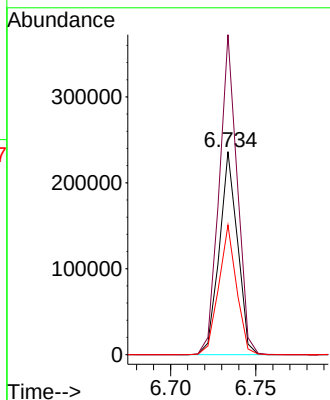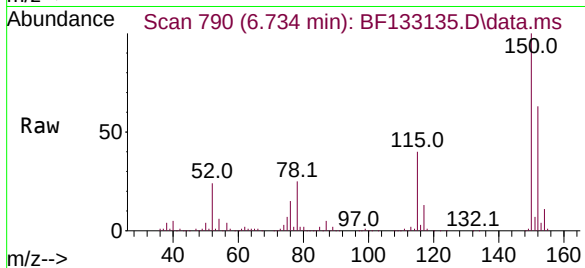

#5
 2-Fluorophenol
 Concen: 126.971 ng
 RT: 5.357 min Scan# 556
 Delta R.T. 0.018 min
 Lab File: BF133135.D
 Acq: 28 Apr 2023 22:27

Tgt Ion:112 Resp: 1468198
 Ion Ratio Lower Upper
 112 100
 64 57.0 46.8 70.2
 63 29.5 23.8 35.8


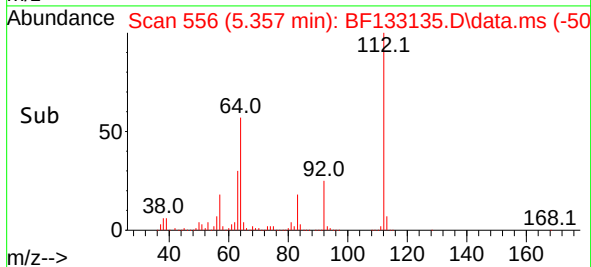
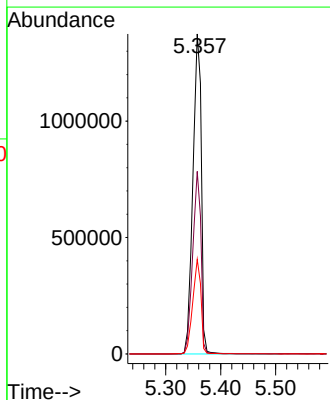
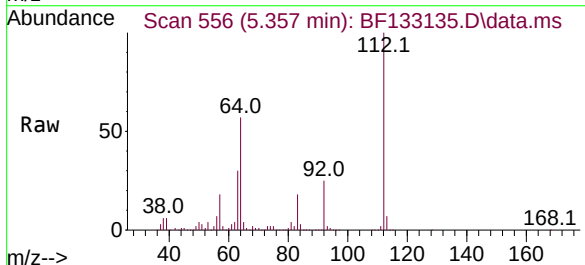


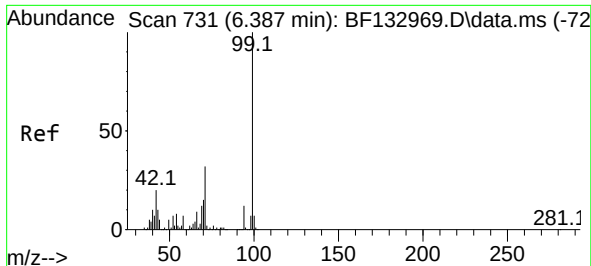

#7
Phenol-d6
Concen: 115.247 ng
RT: 6.375 min Scan# 71
Delta R.T. -0.006 min
Lab File: BF133135.D
Acq: 28 Apr 2023 22:27




Instrument :
BNA_F
ClientSampleId :
BU-512-COMP-03


Tgt Ion: 99 Resp: 1654070
Ion Ratio Lower Upper
99 100
42 19.3 16.3 24.5
71 32.7 25.6 38.4

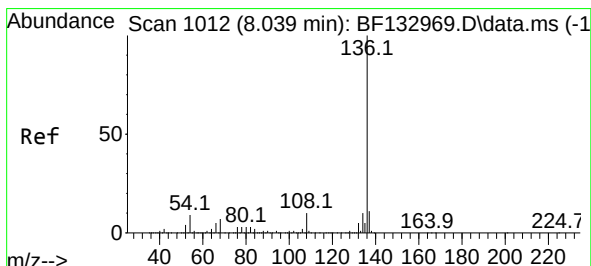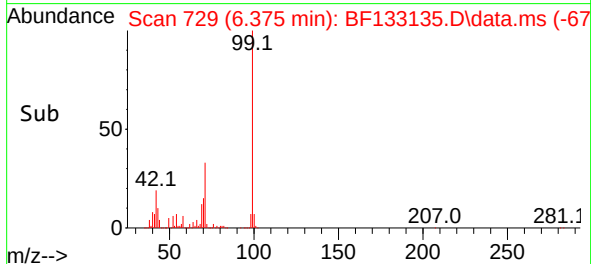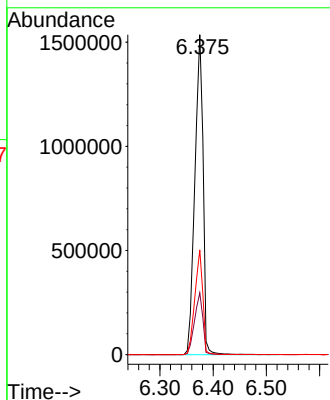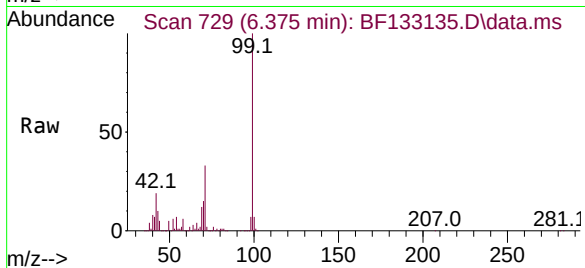

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.016 min Scan# 1008
Delta R.T. -0.006 min
Lab File: BF133135.D
Acq: 28 Apr 2023 22:27

Tgt Ion: 136 Resp: 695867
Ion Ratio Lower Upper
136 100
137 10.8 8.6 13.0
54 8.8 7.0 10.4
68 7.0 5.4 8.2

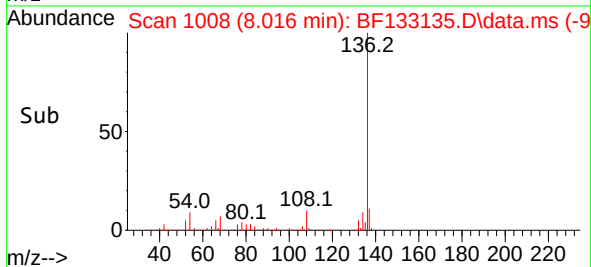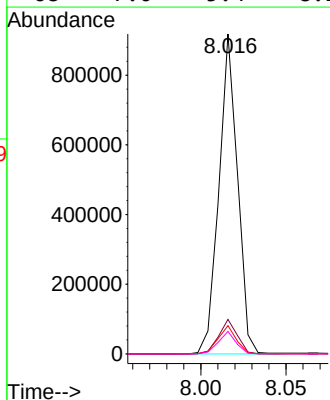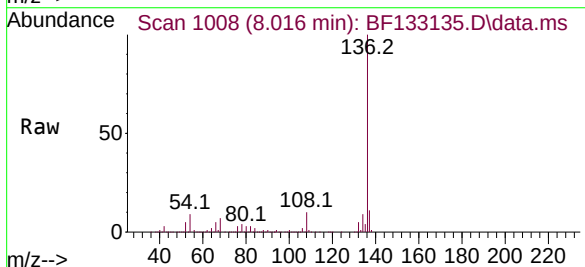

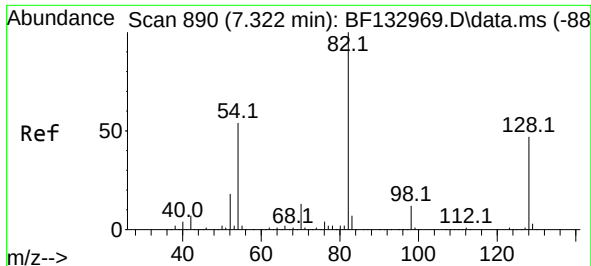

#23

Nitrobenzene-d5

Concen: 93.892 ng

RT: 7.298 min Scan# 81

Delta R.T. -0.006 min

Lab File: BF133135.D

Acq: 28 Apr 2023 22:27

Instrument :





BNA_F

ClientSampleId :

BU-512-COMP-03

Tgt Ion: 82 Resp: 1210457

Ion	Ratio	Lower	Upper
82	100		
128	46.1	37.7	56.5
54	52.9	43.0	64.4

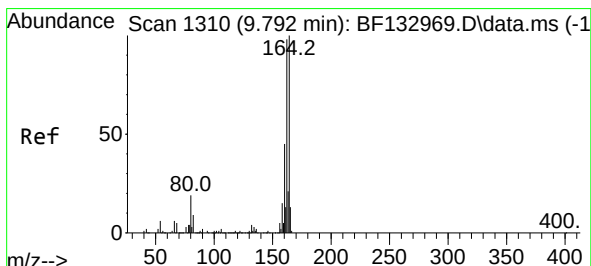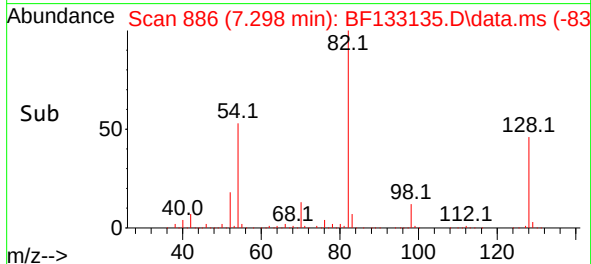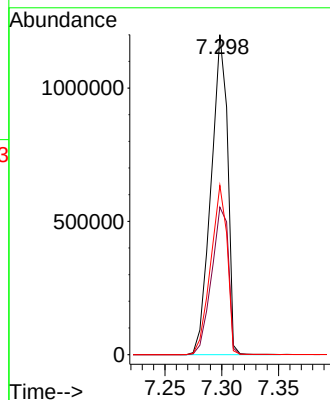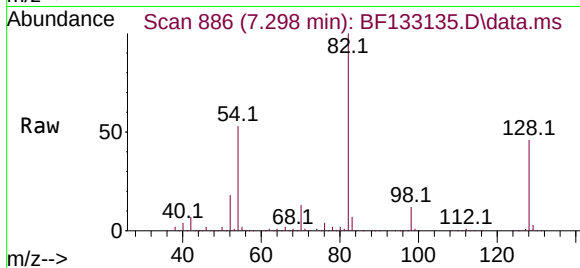

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.769 min Scan# 1306




Delta R.T. -0.006 min


Lab File: BF133135.D

Acq: 28 Apr 2023 22:27

Tgt Ion:164 Resp: 362320

Ion	Ratio	Lower	Upper
164	100		
162	99.3	78.7	118.1
160	44.6	35.8	53.6


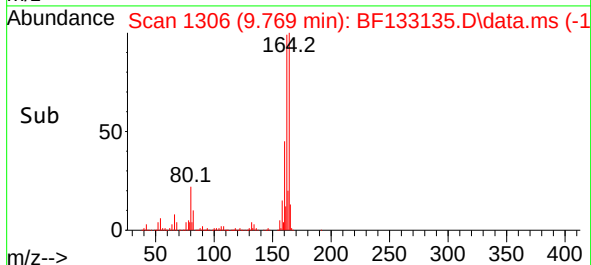
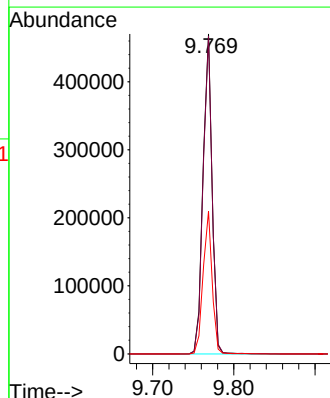
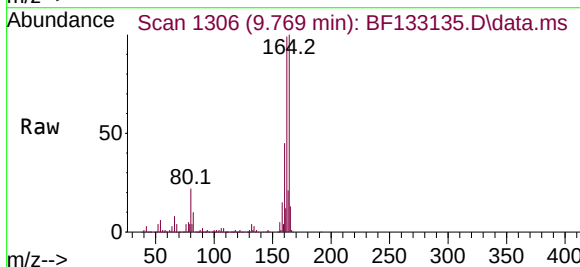


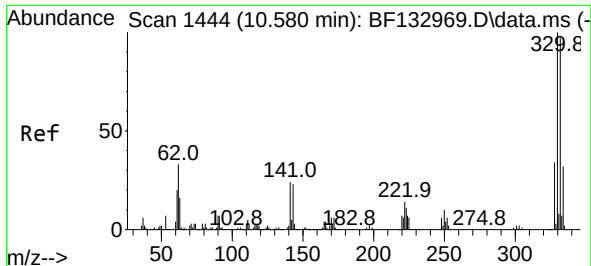

#42
2,4,6-Tribromophenol
Concen: 144.703 ng
RT: 10.557 min Scan# 1444
Delta R.T. -0.006 min
Lab File: BF133135.D
Acq: 28 Apr 2023 22:27




Instrument :
BNA_F
ClientSampleId :
BU-512-COMP-03


Tgt Ion:330 Resp: 527272
Ion Ratio Lower Upper
330 100
332 95.4 77.1 115.7
141 29.7 25.8 38.8

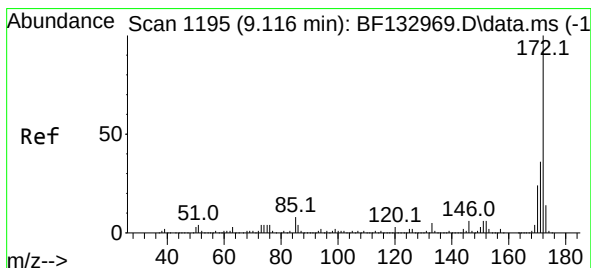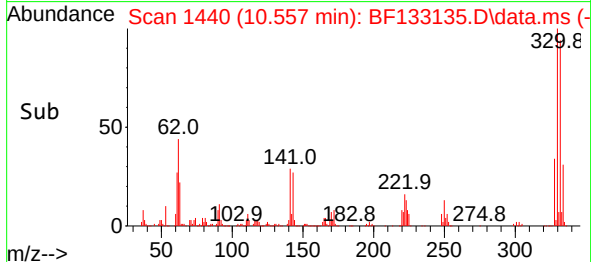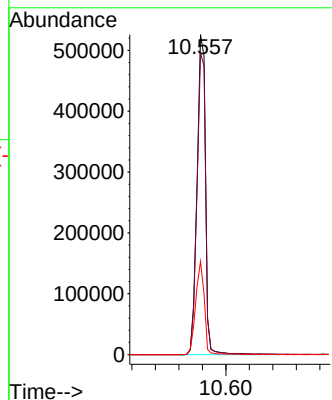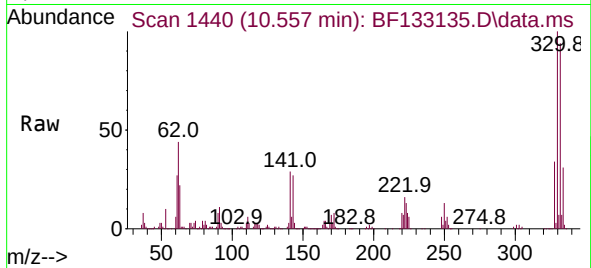

#45
2-Fluorobiphenyl
Concen: 90.705 ng
RT: 9.098 min Scan# 1192
Delta R.T. 0.000 min
Lab File: BF133135.D
Acq: 28 Apr 2023 22:27

Tgt Ion:172 Resp: 1964393
Ion Ratio Lower Upper
172 100
171 36.0 28.8 43.2
170 24.4 19.4 29.2

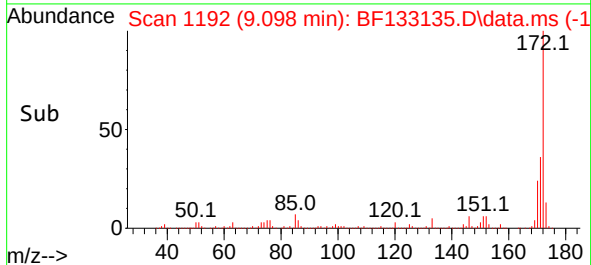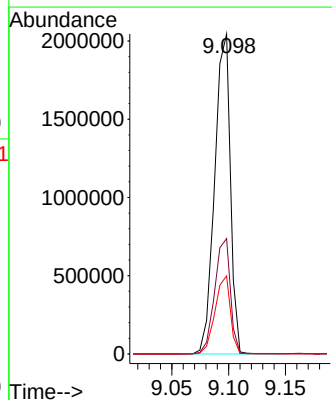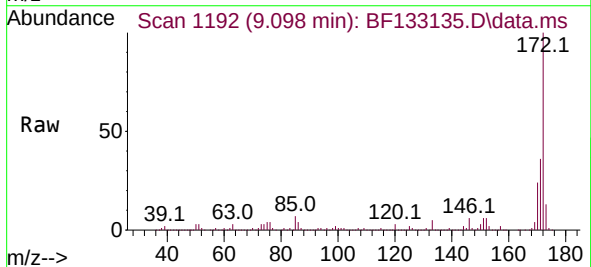

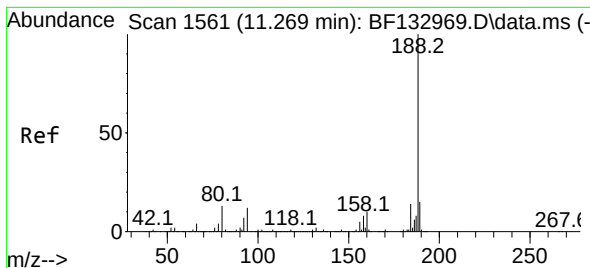

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.251 min Scan# 11

Delta R.T. 0.000 min

Lab File: BF133135.D

Acq: 28 Apr 2023 22:27

Instrument :

BNA_F

ClientSampleId :

BU-512-COMP-03





Tgt Ion:188 Resp: 658226

Ion Ratio Lower Upper

188 100

94 10.2 9.7 14.5

80 10.6 10.4 15.6

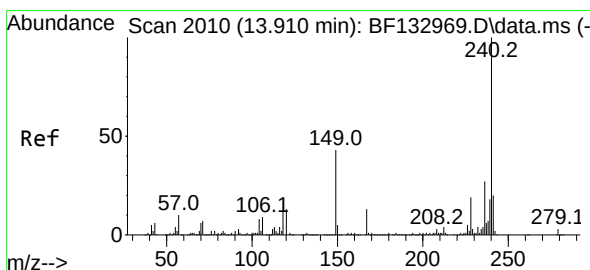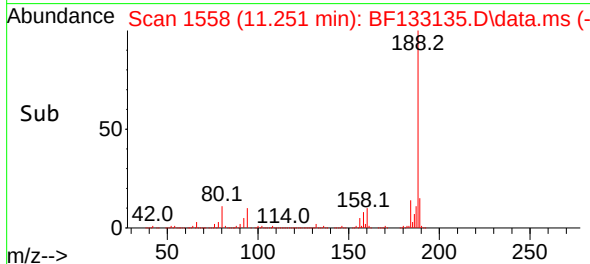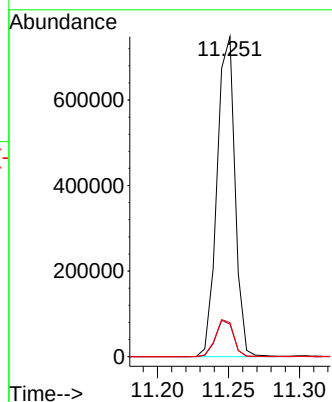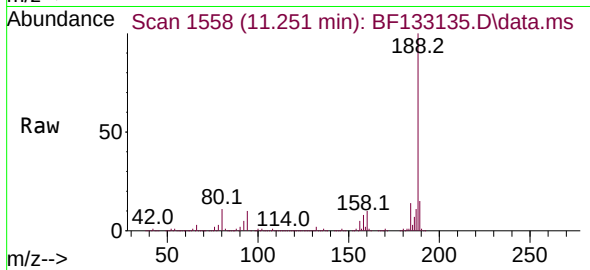

#76

Chrysene-d12

Concen: 20.000 ng

RT: 13.880 min Scan# 2005

Delta R.T. -0.012 min

Lab File: BF133135.D

Acq: 28 Apr 2023 22:27




Tgt Ion:240 Resp: 492366


Ion Ratio Lower Upper

240 100

120 14.4 10.5 15.7

236 26.3 21.5 32.3

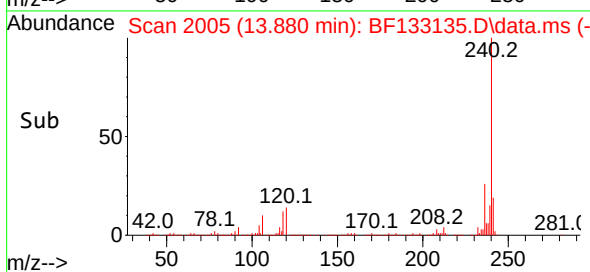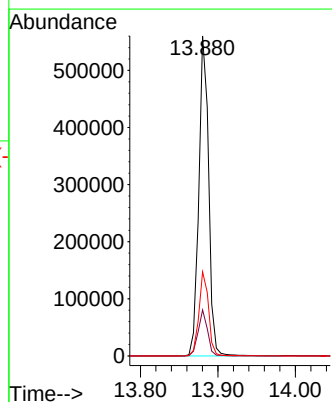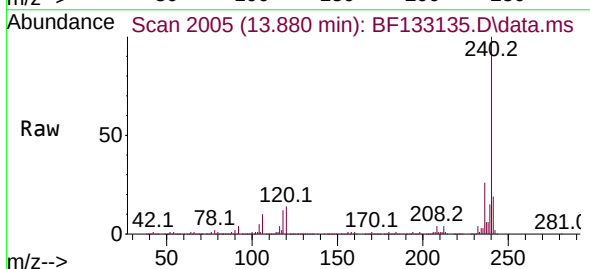

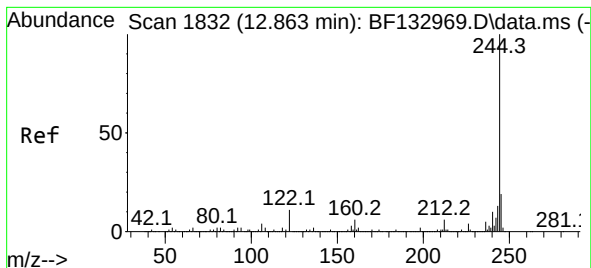

#79

Terphenyl-d14

Concen: 85.548 ng

RT: 12.839 min Scan# 1832

Delta R.T. 0.000 min

Lab File: BF133135.D

Acq: 28 Apr 2023 22:27

Instrument :

BNA_F

ClientSampleId :

BU-512-COMP-03





Tgt Ion:244 Resp: 2442252

Ion Ratio Lower Upper

244 100

212 6.6 5.1 7.7

122 12.2 8.6 13.0

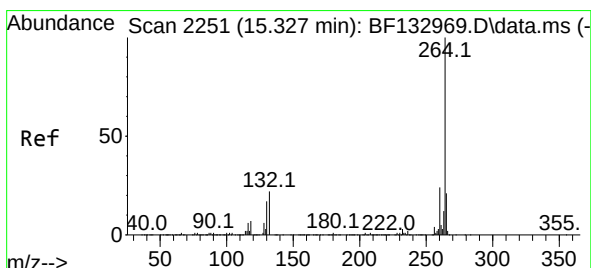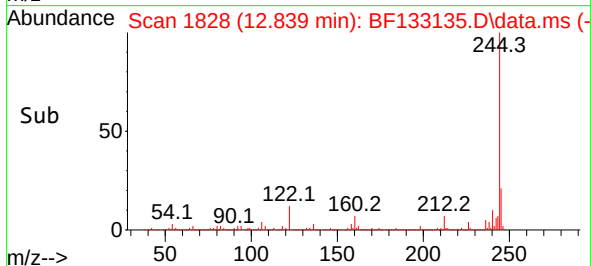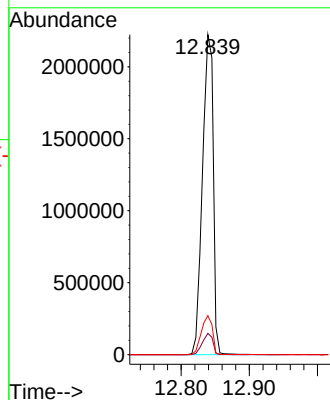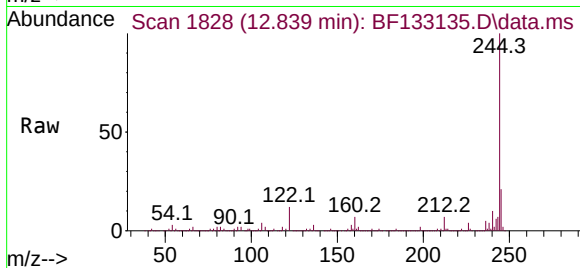

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.304 min Scan# 2247

Delta R.T. -0.006 min

Lab File: BF133135.D

Acq: 28 Apr 2023 22:27

Tgt Ion:264 Resp: 379092

Ion Ratio Lower Upper

264 100

260 24.2 18.8 28.2

265 22.7 17.0 25.4

