


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042823\
Data File : BF133112.D
Acq On : 28 Apr 2023 09:14
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon May 01 12:55:30 2023

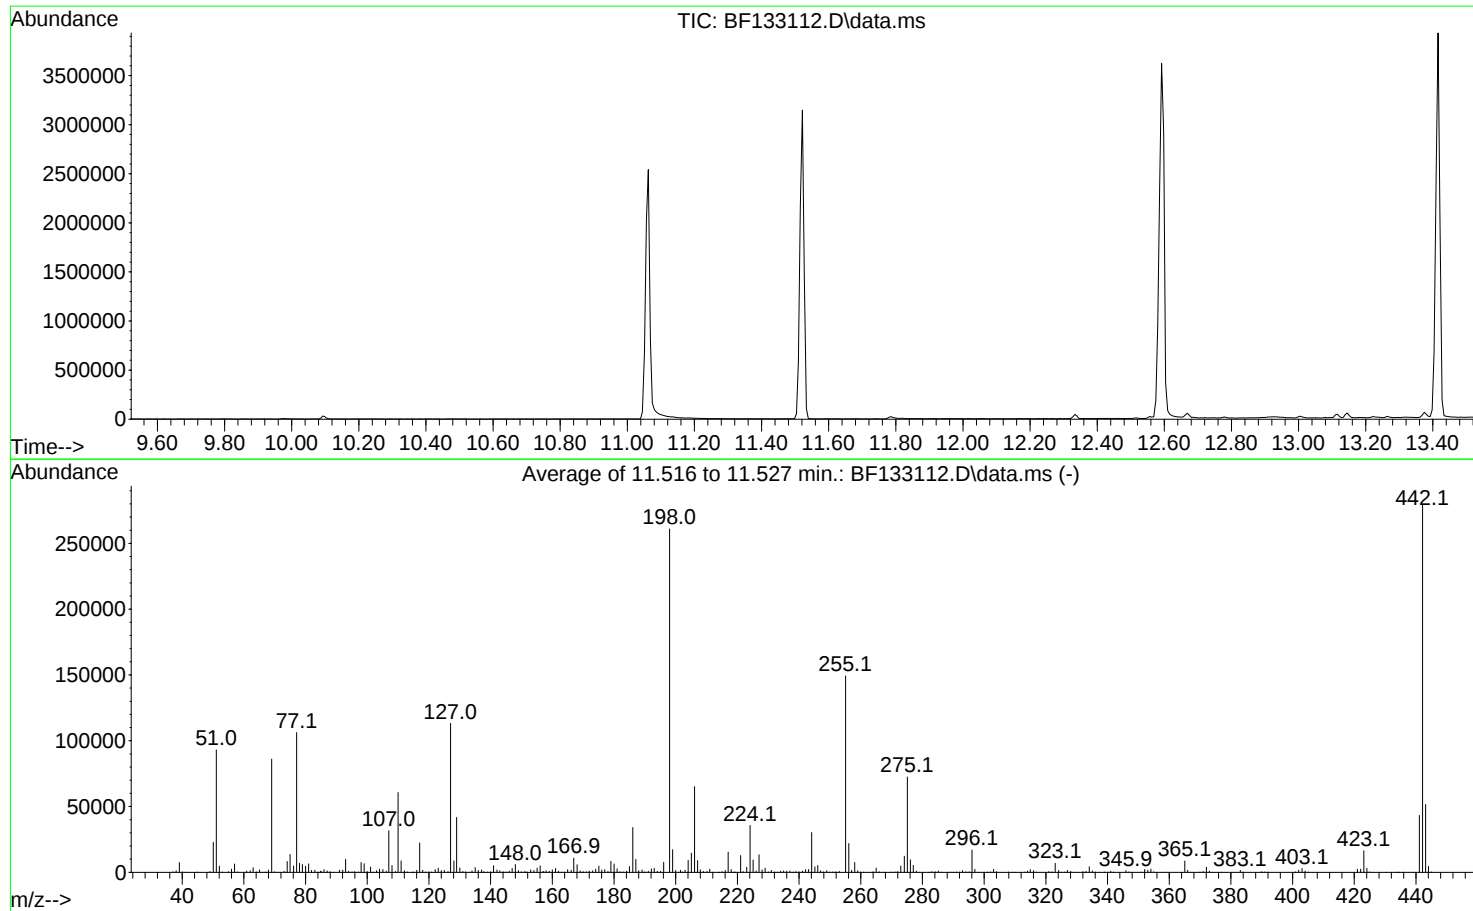




AutoFind: Scans 1603, 1604, 1605; Background Corrected with Scan 1597

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.7	93029	PASS
68	69	0.00	2	1.9	1611	PASS
69	198	0.00	100	33.0	86101	PASS
70	69	0.00	2	0.5	472	PASS
127	198	10	80	43.4	113221	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	260949	PASS
199	198	5	9	6.6	17265	PASS
275	198	10	60	27.8	72488	PASS
365	198	1	100	3.3	8564	PASS
441	198	0.01	100	16.6	43189	PASS
442	442	50	100	100.0	279616	PASS
443	442	15	24	18.4	51557	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042823\
Data File : BF133112.D
Acq On : 28 Apr 2023 09:14
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 28 11:54:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 28 02:00:53 2023
Response via : Initial Calibration

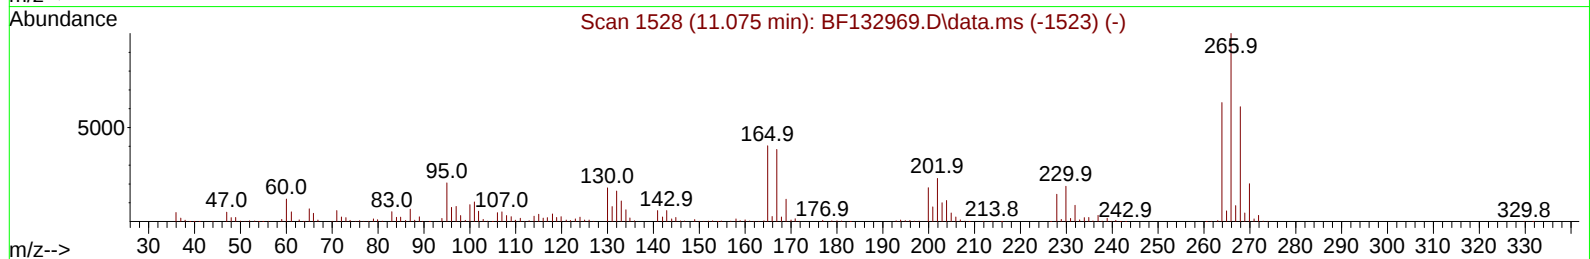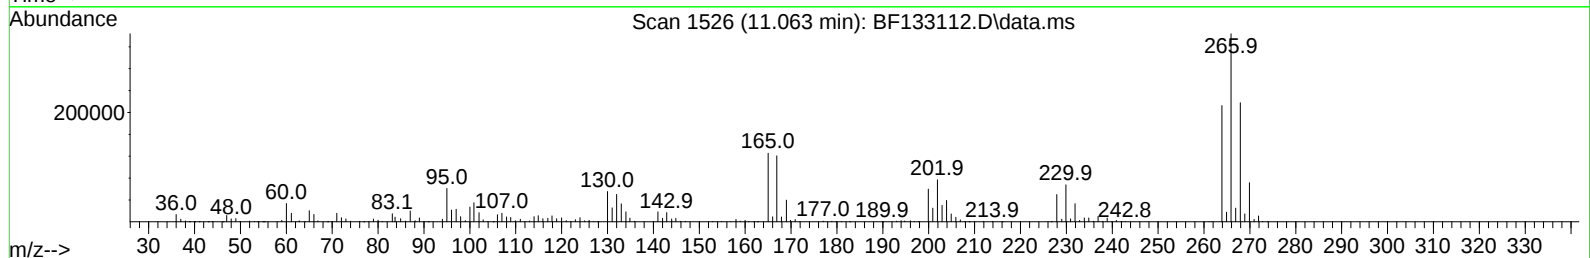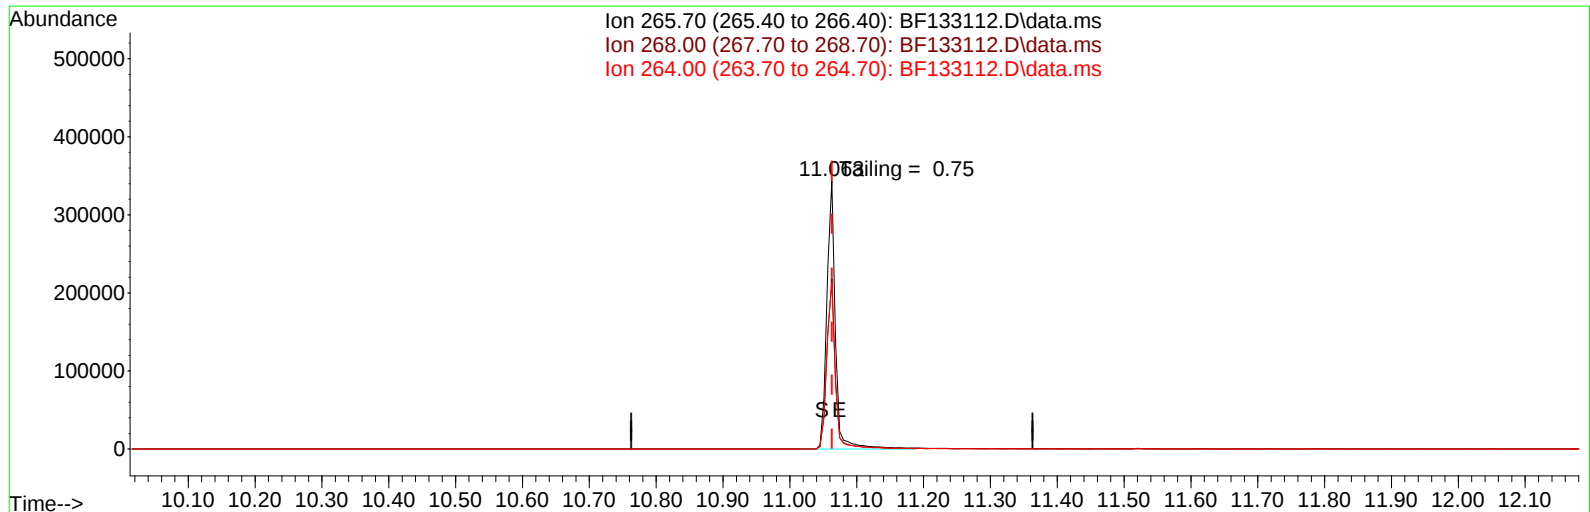

TIC: BF133112.D\data.ms

(70) Pentachlorophenol (C)

11.063min (-0.000) 30088.94 ng


response 307689

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	63.32
264.00	63.30	61.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042823\
Data File : BF133112.D
Acq On : 28 Apr 2023 09:14
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 28 11:54:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 28 02:00:53 2023
Response via : Initial Calibration

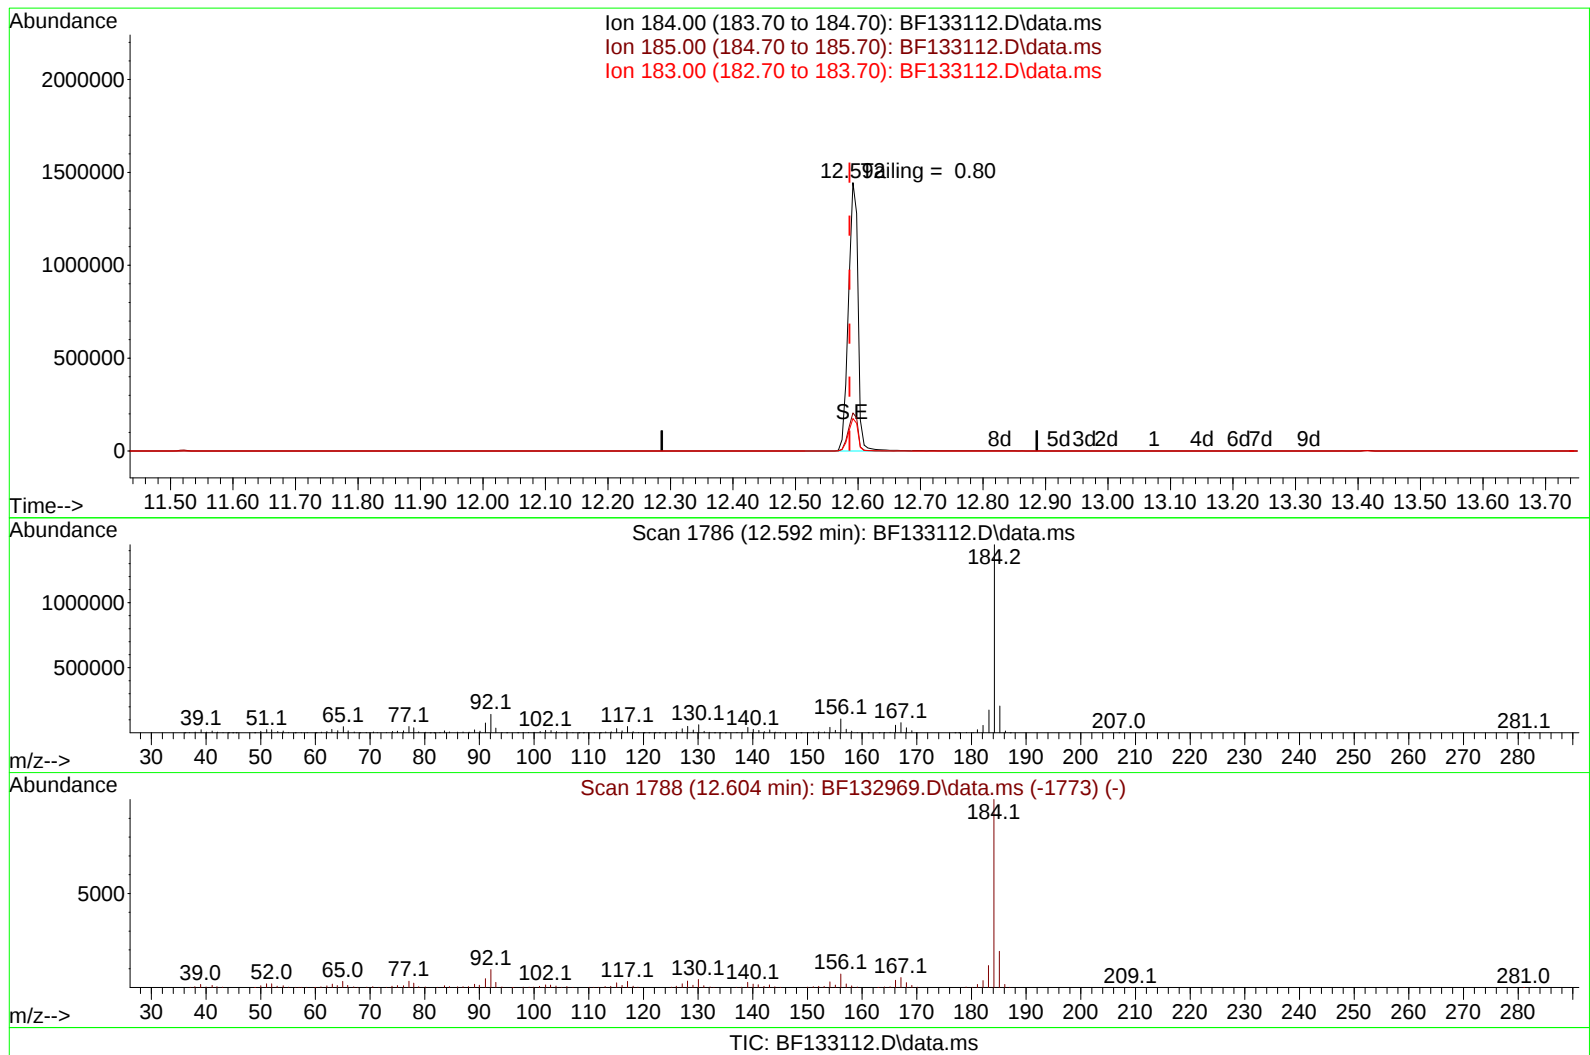

(77) Benzidine

12.592min (+ 0.006) 1661743.93 ng m

response 1545553

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	19.30	14.23#
183.00	11.70	12.10
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/28/2023	BNA_F	<u>BF133112.D</u>
Compound Name	Response	Retention Time
DDT	669748	13.415
DDD	13251	13.145
DDE	1776	12.78
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15027	684775	2.19

Instrument :
BNA_F
ClientSampleId :
DFTPP