
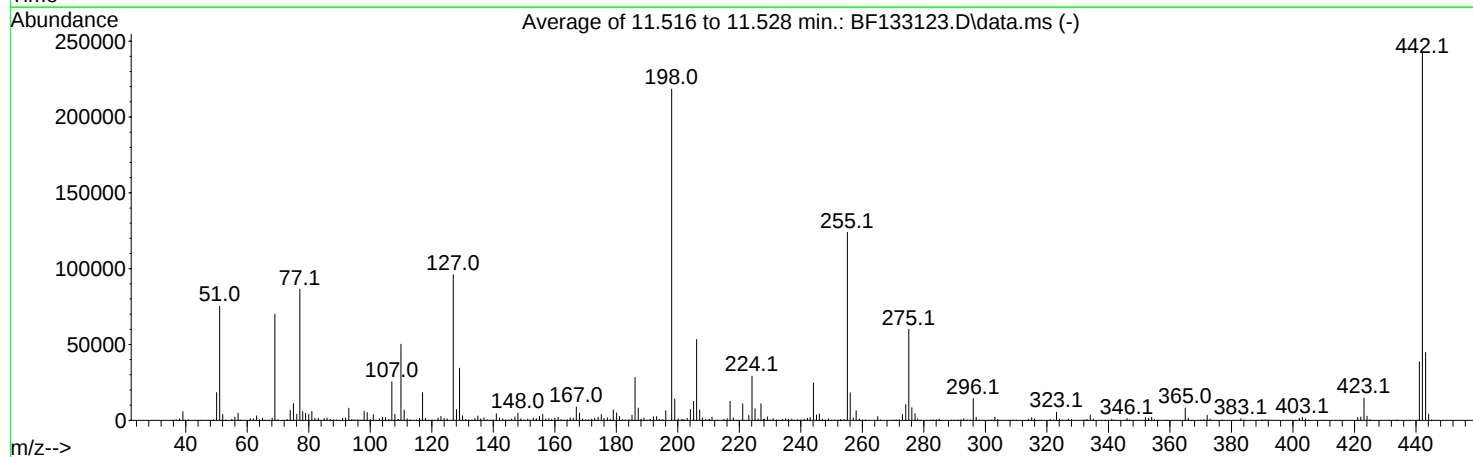


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042823\
Data File : BF133123.D
Acq On : 28 Apr 2023 15:46
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon May 01 12:55:30 2023

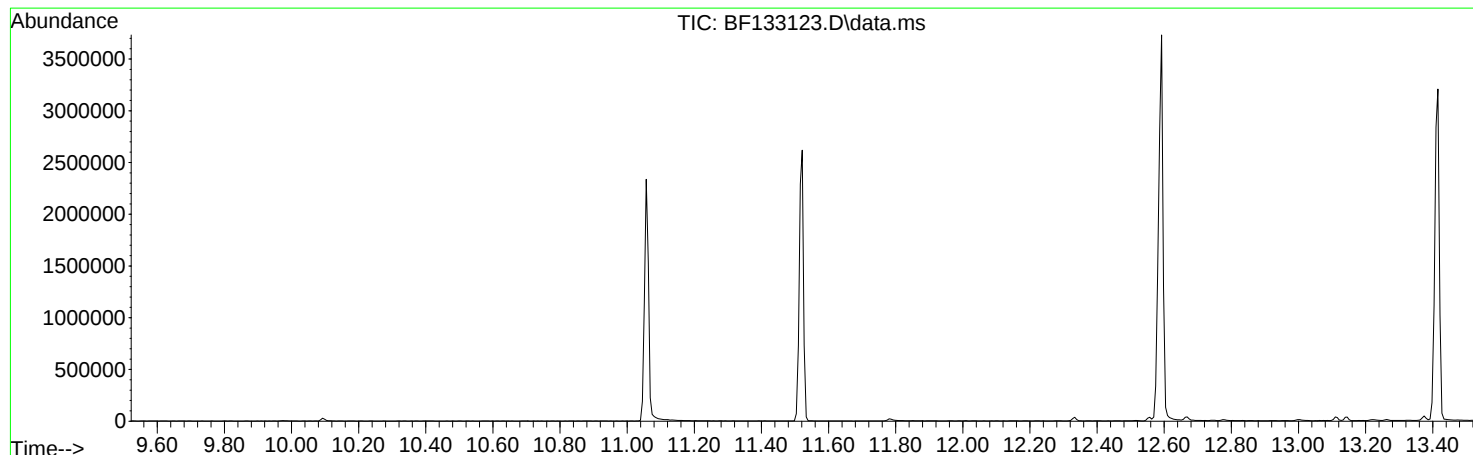




AutoFind: Scans 1603, 1604, 1605; Background Corrected with Scan 1597

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.4	75181	PASS
68	69	0.00	2	2.0	1396	PASS
69	198	0.00	100	32.1	70053	PASS
70	69	0.00	2	0.5	340	PASS
127	198	10	80	44.0	96112	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	218408	PASS
199	198	5	9	6.5	14129	PASS
275	198	10	60	27.5	60021	PASS
365	198	1	100	3.8	8209	PASS
441	198	0.01	100	17.7	38613	PASS
442	442	50	100	100.0	242581	PASS
443	442	15	24	18.4	44728	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042823\
 Data File : BF133123.D
 Acq On : 28 Apr 2023 15:46
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Apr 28 17:13:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 28 12:18:20 2023
 Response via : Initial Calibration

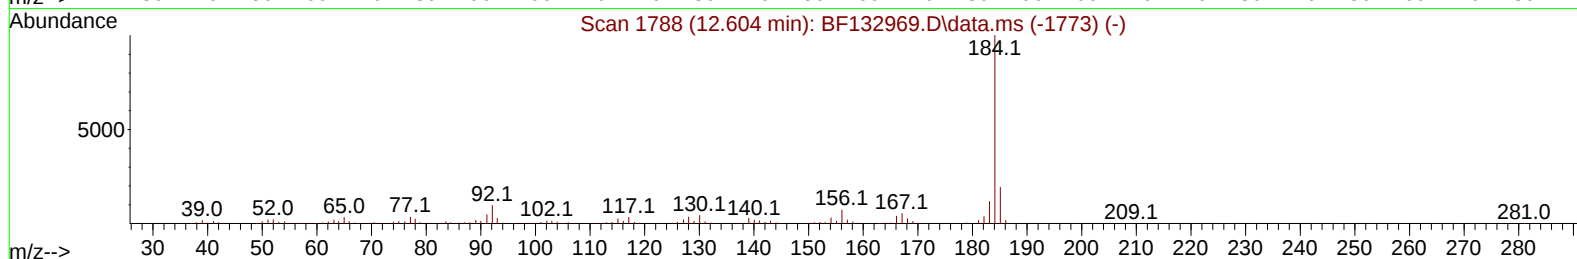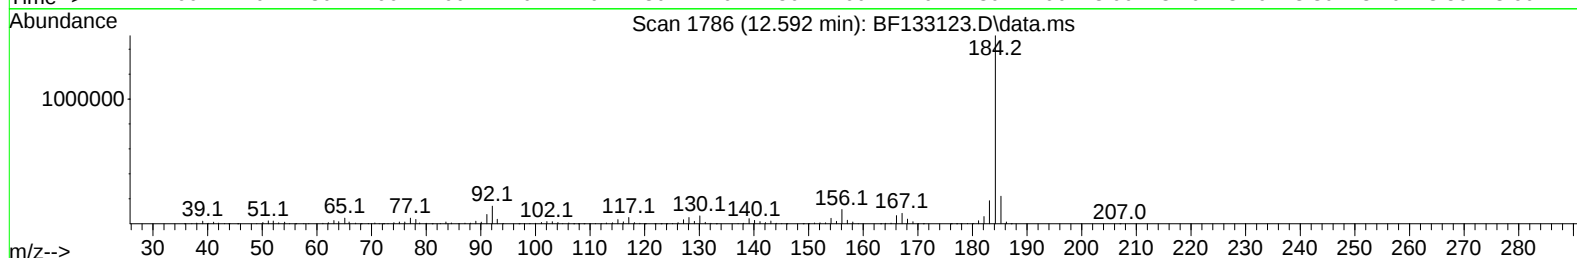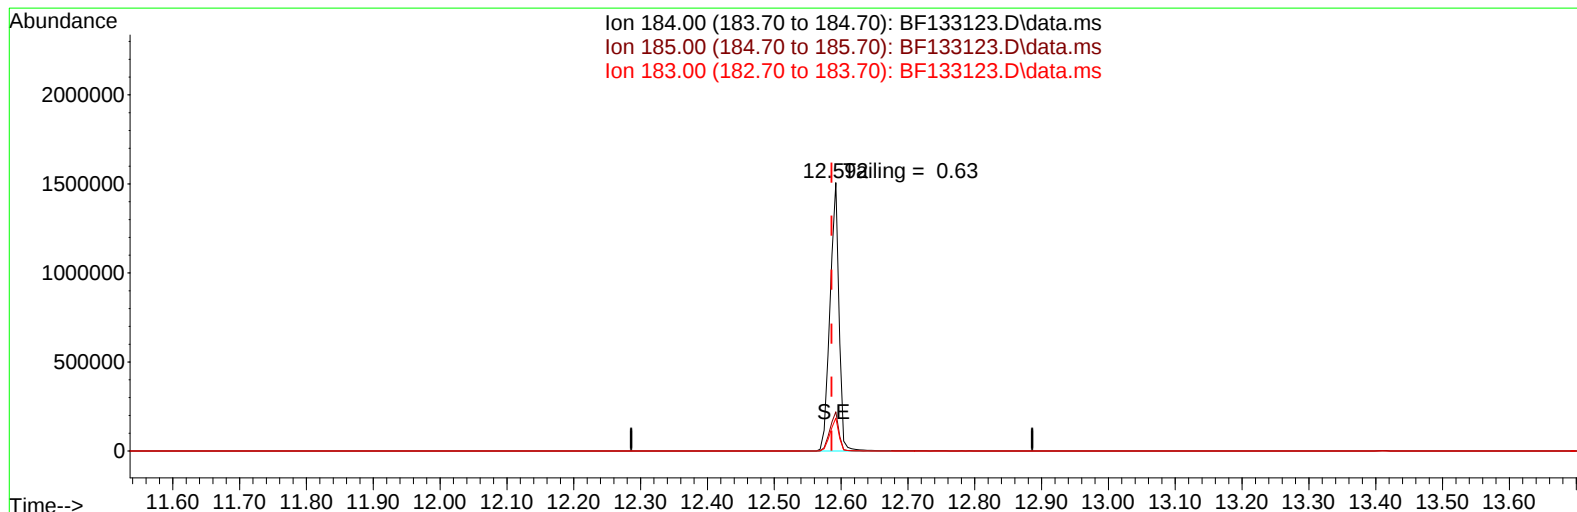

TIC: BF133123.D\data.ms

(77) Benzidine

12.592min (+ 0.006) 1062191.41 ng

response 1419015

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	19.30	14.62#
183.00	11.70	12.30
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/28/2023	BNA_F	<u>BF133123.D</u>
Compound Name	Response	Retention Time
DDT	605004	13.416
DDD	12718	13.11
DDE	1458	12.78
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14176	619180	2.29

Instrument :
BNA_F
ClientSampleId :
DFTPP