

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF042915\
 Data File : BF078816.D
 Acq On : 29 Apr 2015 16:35
 Operator : TP/IZ
 Sample : PB83015BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB83015BL

Quant Time: Apr 30 01:14:11 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042815.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 30 00:55:08 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.38	152	75320	20.00	ng	0.00
21) Naphthalene-d8	8.96	136	305844	20.00	ng	0.00
38) Acenaphthene-d10	11.14	164	138596	20.00	ng	0.00
63) Phenanthrene-d10	12.98	188	272894	20.00	ng	0.00
75) Chrysene-d12	16.29	240	275821	20.00	ng	-0.01
86) Perylene-d12	18.06	264	267095	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.68	112	538937	131.42	ng	0.00
7) Phenol-d6	6.92	99	673356	122.94	ng	0.00
23) Nitrobenzene-d5	8.07	82	364136	85.72	ng	0.00
41) 2,4,6-Tribromophenol	12.11	330	162234	118.23	ng	-0.01
44) 2-Fluorobiphenyl	10.31	172	805401	79.58	ng	0.00
78) Terphenyl-d14	14.98	244	933987	80.64	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF042915\
Data File : BF078816.D
Acq On : 29 Apr 2015 16:35
Operator : TP/IZ
Sample : PB83015BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB83015BL

Quant Time: Apr 30 01:14:11 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 30 00:55:08 2015
Response via : Initial Calibration

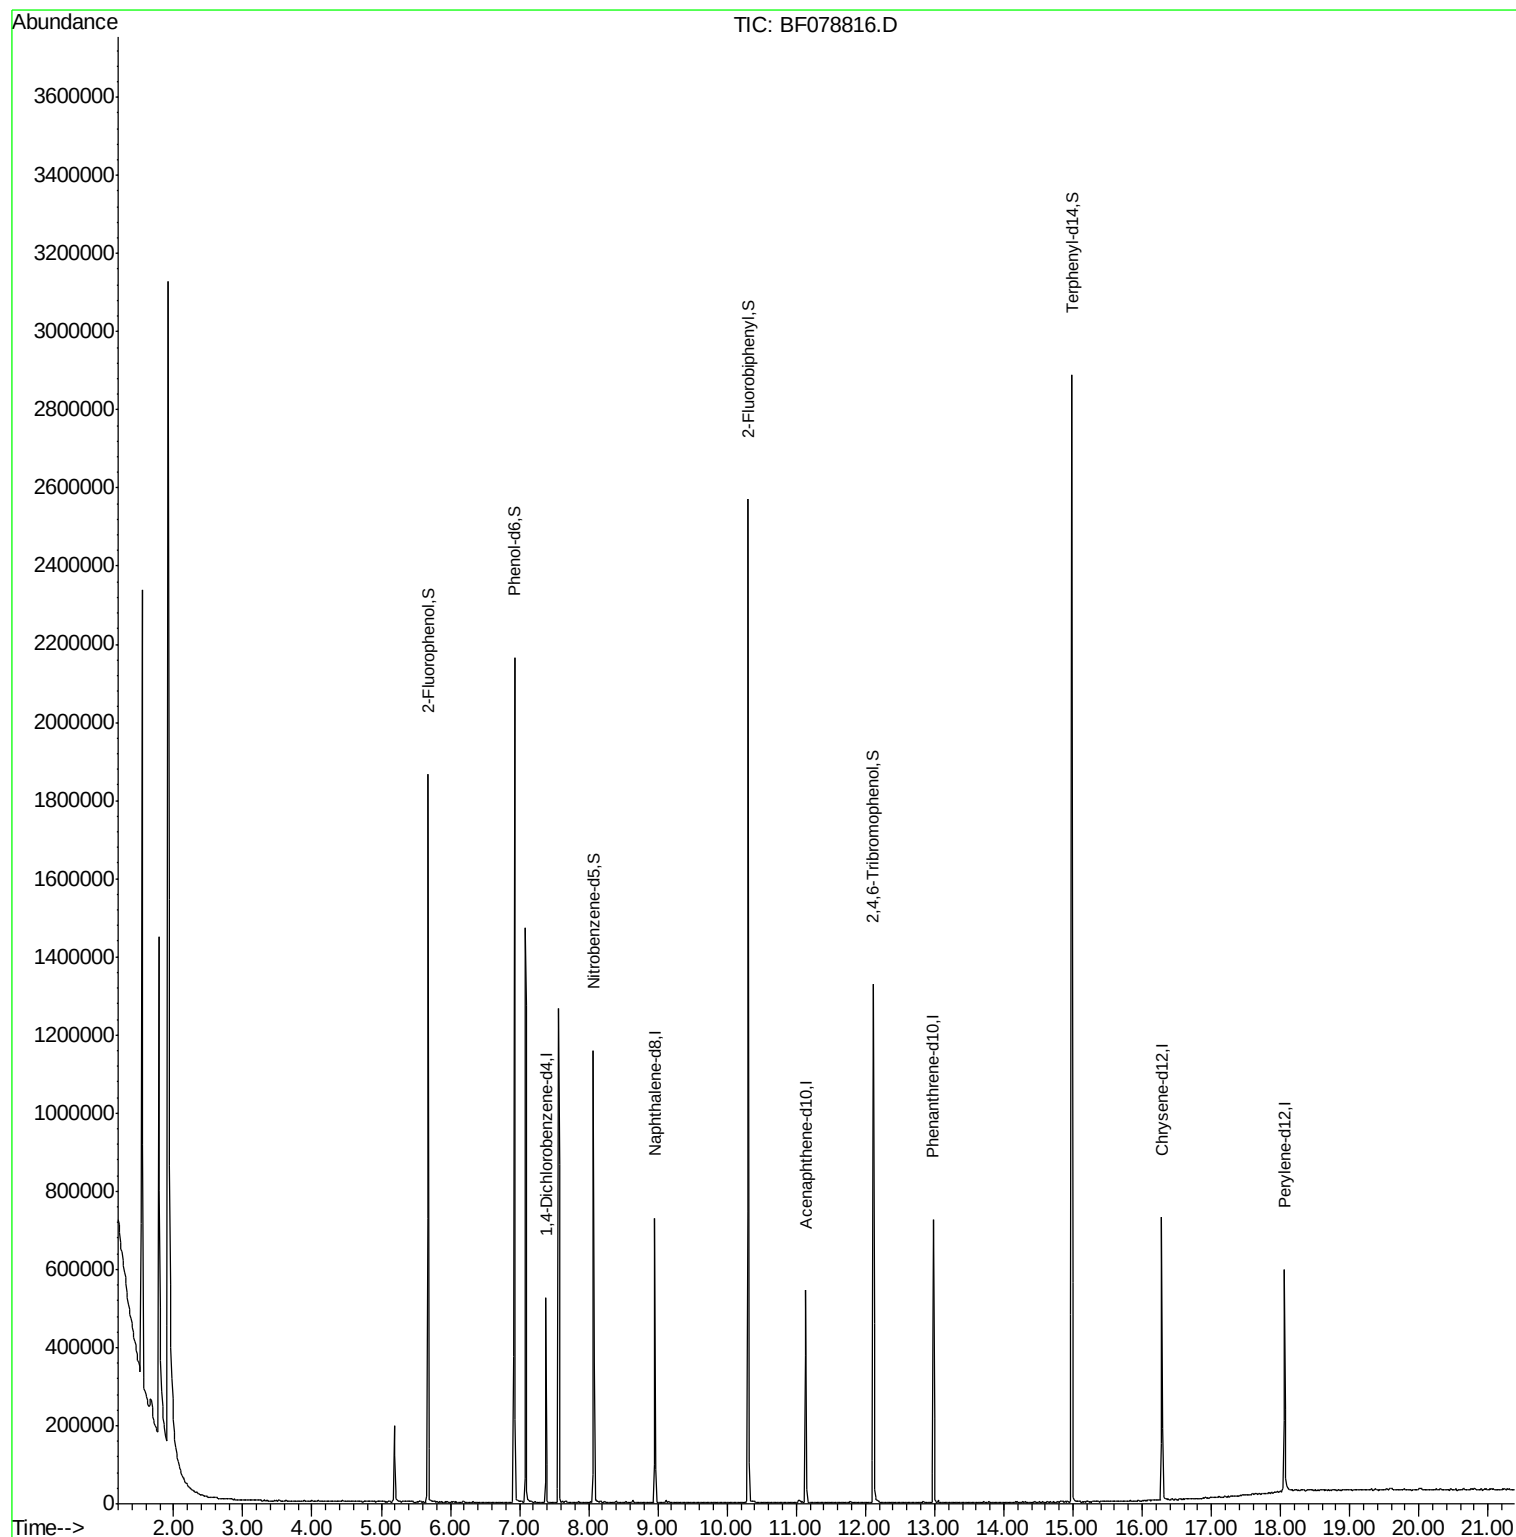




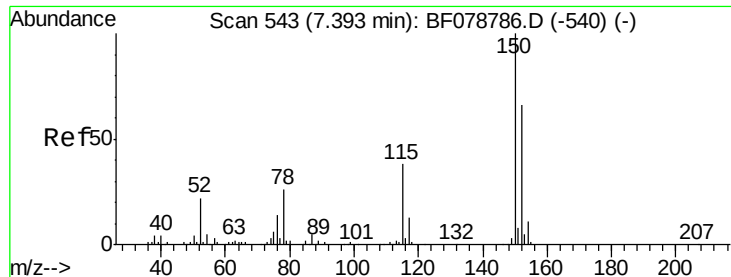


#1

1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.38 min Scan# 542
Delta R.T. -0.00 min
Lab File: BF078816.D
Acq: 29 Apr 2015 16:35

Instrument :
BNA_F
ClientSampleId :
PB83015BL




Tgt Ion:152 Resp: 75320
Ion Ratio Lower Upper
152 100
150 156.3 122.0 183.0
115 61.7 46.3 69.5

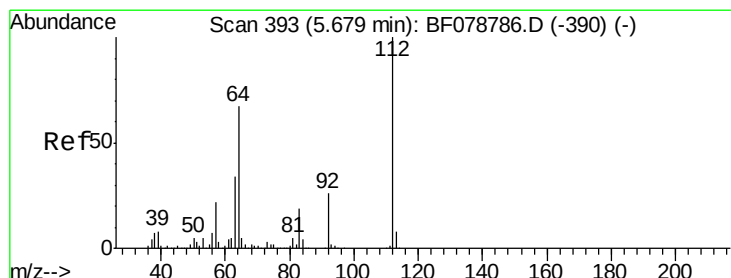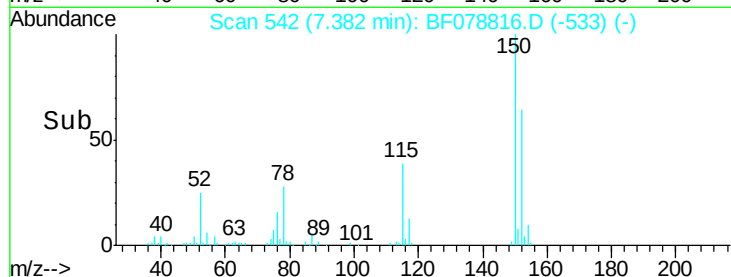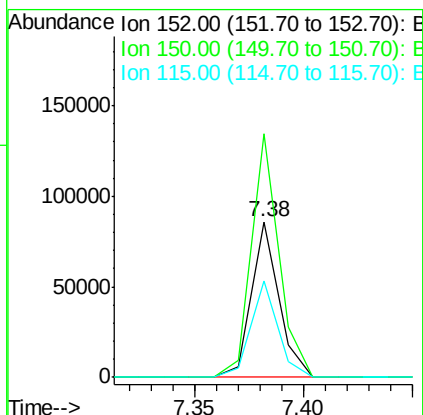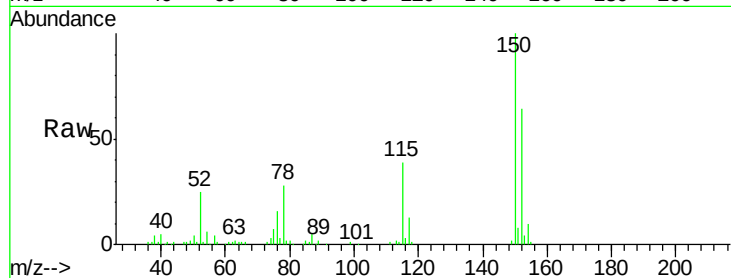


#5

2-Fluorophenol
Concen: 131.42 ng
RT: 5.68 min Scan# 393
Delta R.T. -0.00 min
Lab File: BF078816.D
Acq: 29 Apr 2015 16:35

Tgt Ion:112 Resp: 538937
Ion Ratio Lower Upper
112 100
64 57.4 53.5 80.3
63 29.4 27.5 41.3

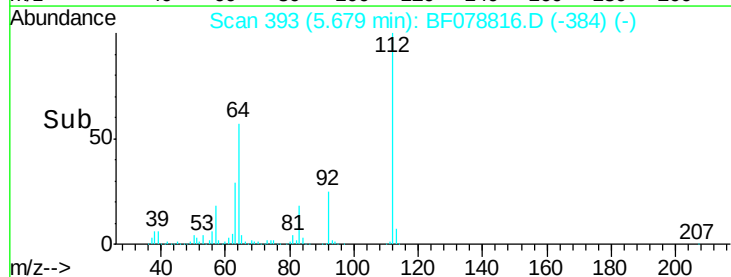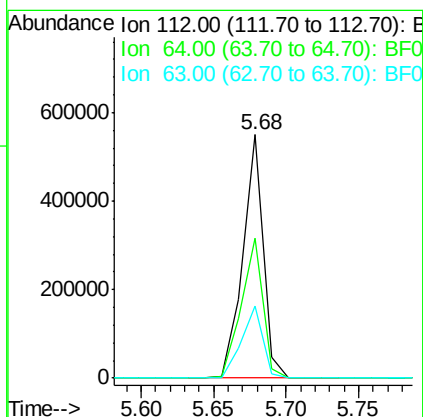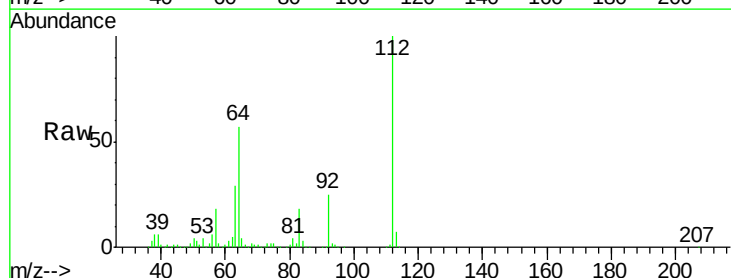

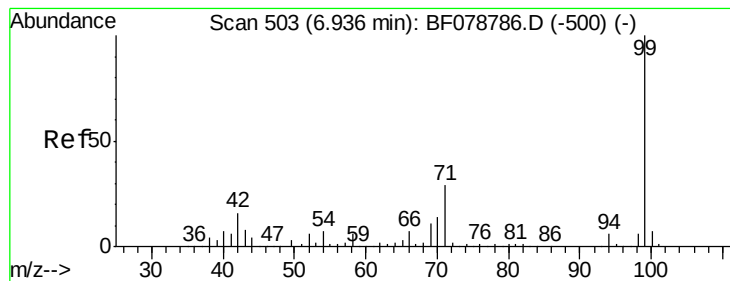

#7

Phenol-d6

Concen: 122.94 ng

RT: 6.92 min Scan# 502

Delta R.T. -0.00 min

Lab File: BF078816.D

Acq: 29 Apr 2015 16:35

Instrument :

BNA_F

ClientSampled :

PB83015BL


Tgt Ion: 99 Resp: 673356

Ion Ratio Lower Upper

99 100

42 20.0 12.8 19.2#




71 32.9 23.4 35.2

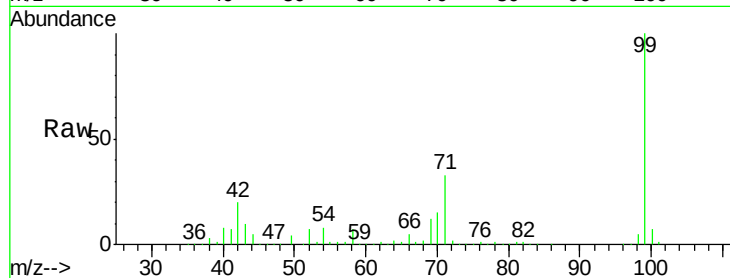

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

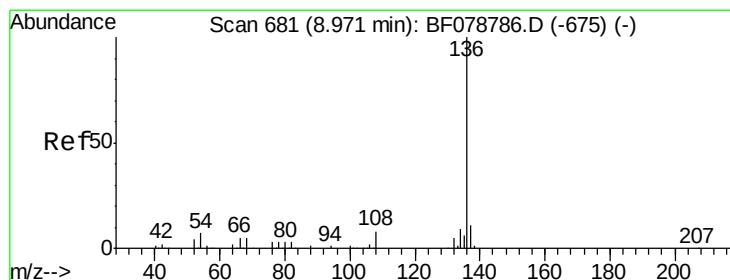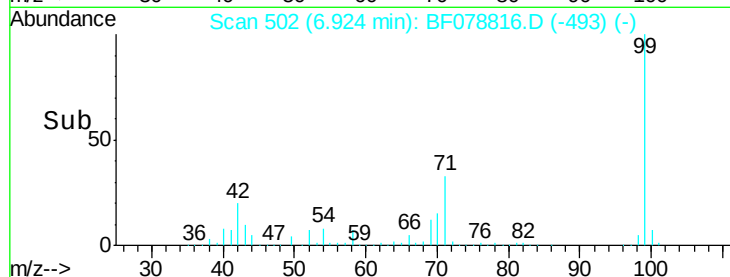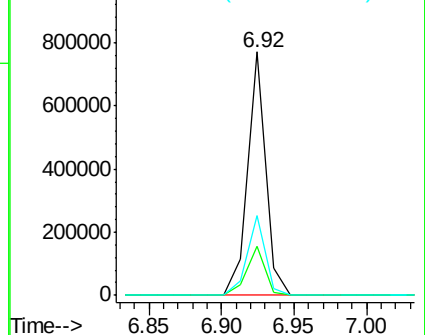

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.96 min Scan# 680

Delta R.T. -0.00 min

Lab File: BF078816.D

Acq: 29 Apr 2015 16:35

Tgt Ion: 136 Resp: 305844


Ion Ratio Lower Upper

136 100

137 10.9 8.7 13.1

54 8.6 5.8 8.8

68 5.8 4.2 6.4


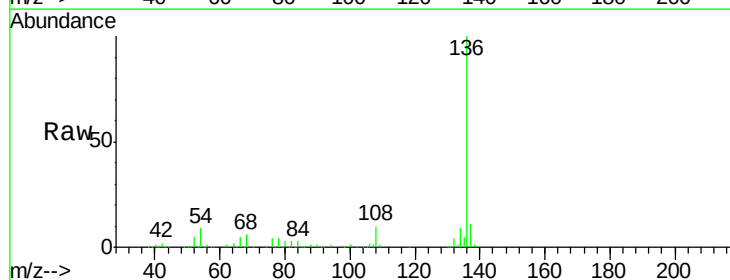



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

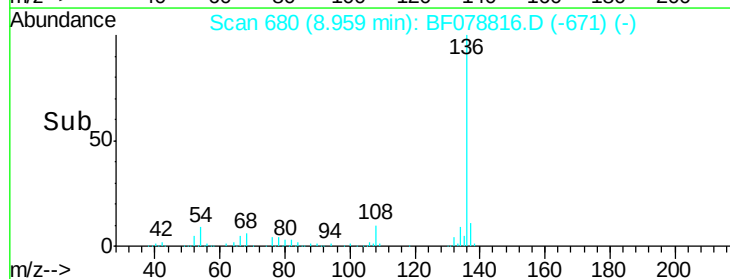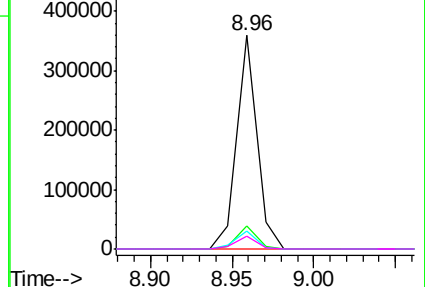


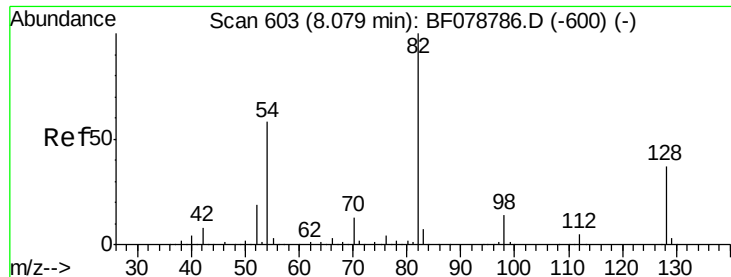




#23
 Nitrobenzene-d5
 Concen: 85.72 ng
 RT: 8.07 min Scan# 602
 Delta R.T. -0.00 min
 Lab File: BF078816.D
 Acq: 29 Apr 2015 16:35

Instrument :
 BNA_F
 ClientSampleId :
 PB83015BL

Tgt Ion: 82 Resp: 364136
 Ion Ratio Lower Upper
 82 100
 128 36.8 30.0 45.0
 54 57.7 46.4 69.6

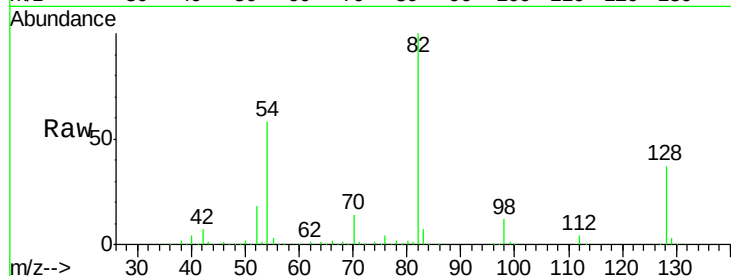


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF0

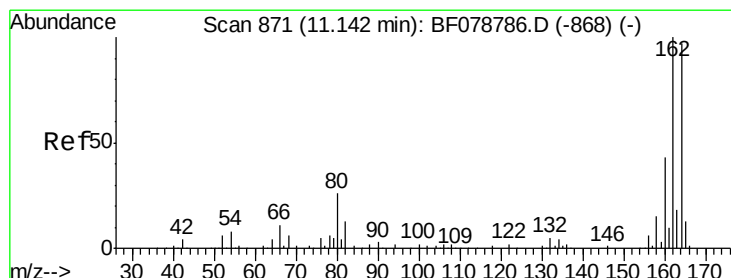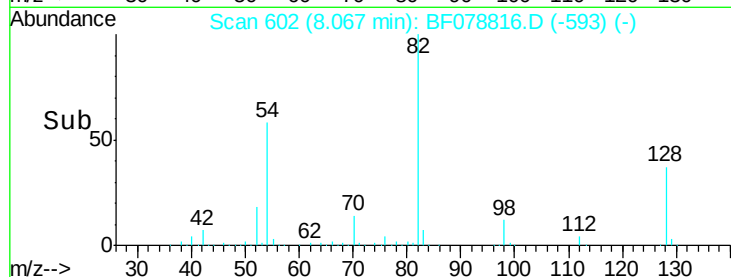
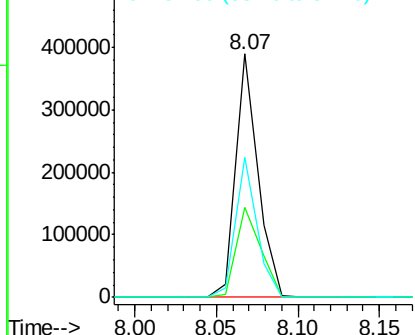



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 11.14 min Scan# 871
 Delta R.T. -0.00 min
 Lab File: BF078816.D
 Acq: 29 Apr 2015 16:35

Tgt Ion: 164 Resp: 138596
 Ion Ratio Lower Upper
 164 100
 162 106.6 82.7 124.1
 160 47.9 35.8 53.8

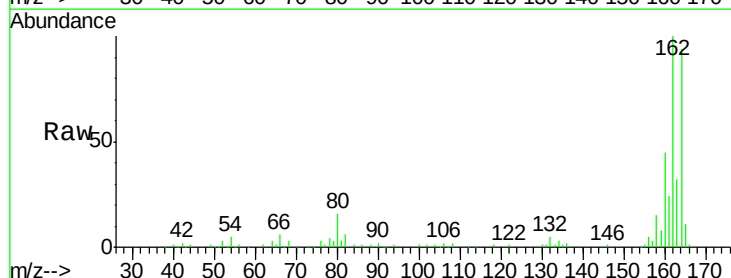

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E



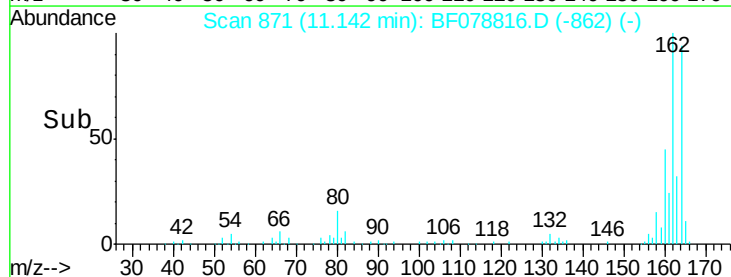
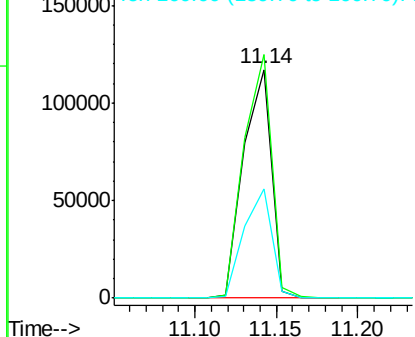


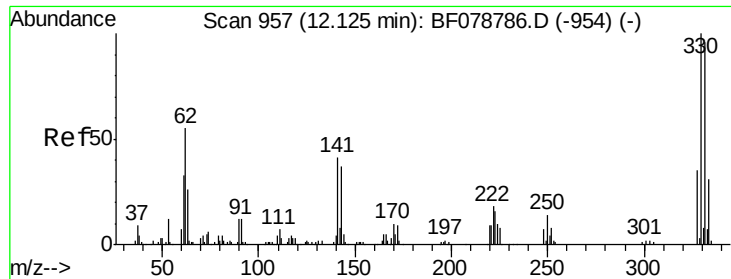

#41
 2,4,6-Tribromophenol
 Concen: 118.23 ng
 RT: 12.11 min Scan# 956
 Delta R.T. -0.01 min
 Lab File: BF078816.D
 Acq: 29 Apr 2015 16:35




Instrument :
 BNA_F
 ClientSampleId :
 PB83015BL


Tgt Ion:330 Resp: 162234
 Ion Ratio Lower Upper
 330 100
 332 96.0 0.0 0.0#
 141 37.3 0.0 0.0#

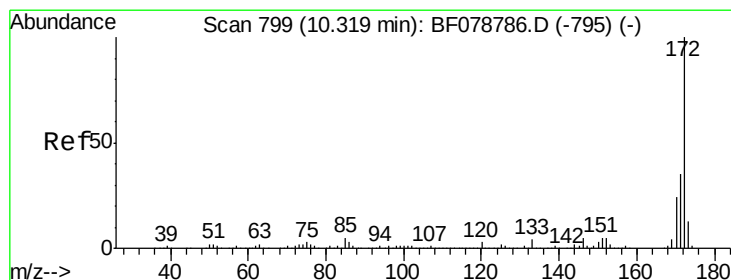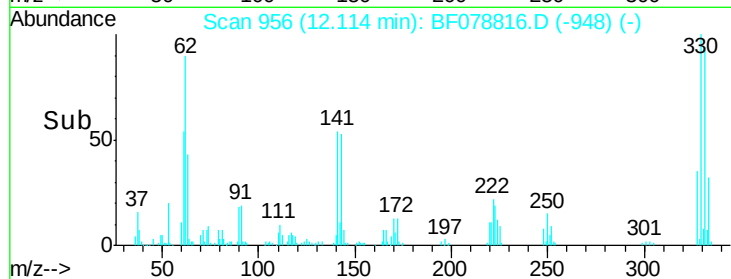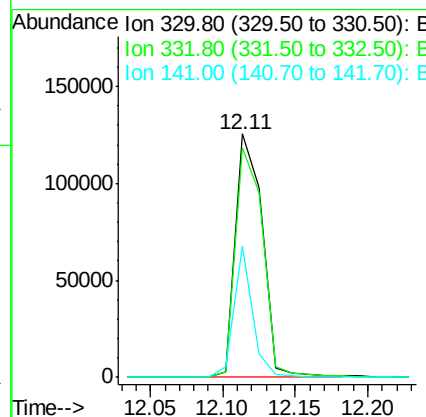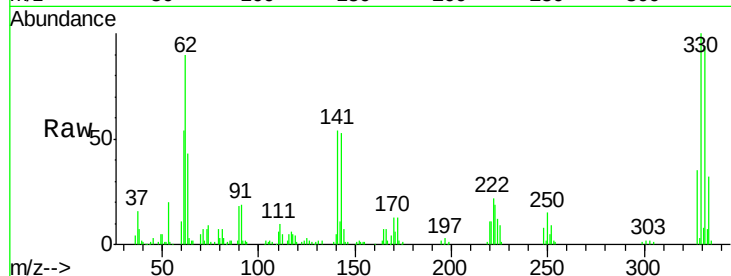

#44
 2-Fluorobiphenyl
 Concen: 79.58 ng
 RT: 10.31 min Scan# 798
 Delta R.T. -0.00 min
 Lab File: BF078816.D
 Acq: 29 Apr 2015 16:35

Tgt Ion:172 Resp: 805401
 Ion Ratio Lower Upper
 172 100
 171 35.7 27.9 41.9
 170 24.3 19.4 29.0

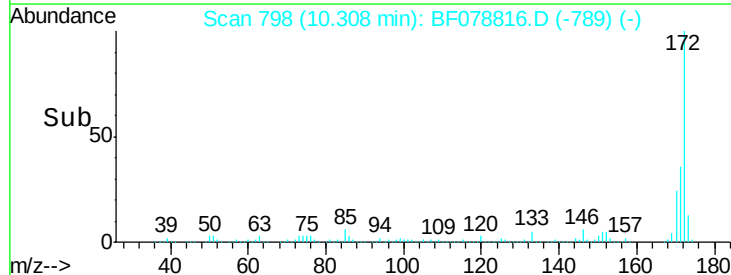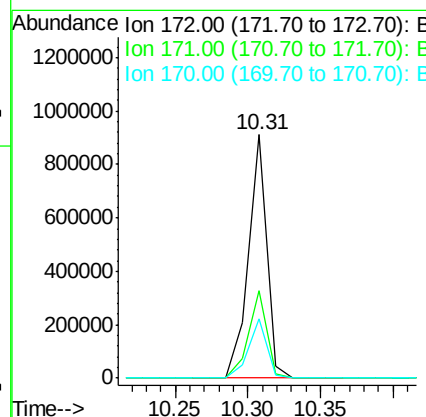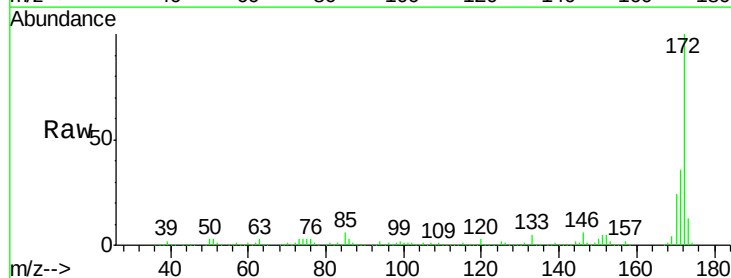


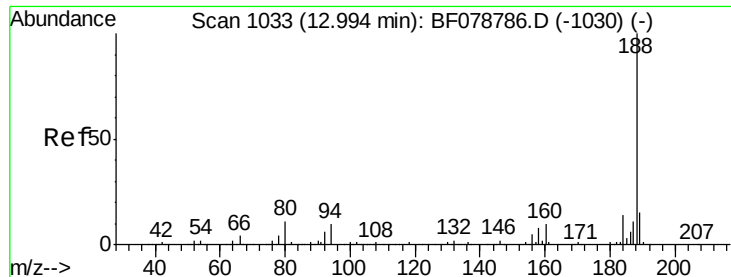




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 12.98 min Scan# 1032
Delta R.T. -0.00 min
Lab File: BF078816.D
Acq: 29 Apr 2015 16:35

Instrument :
BNA_F
ClientSampleId :
PB83015BL

Tgt Ion:188 Resp: 272894
Ion Ratio Lower Upper
188 100
94 12.0 8.2 12.2
80 12.8 8.9 13.3

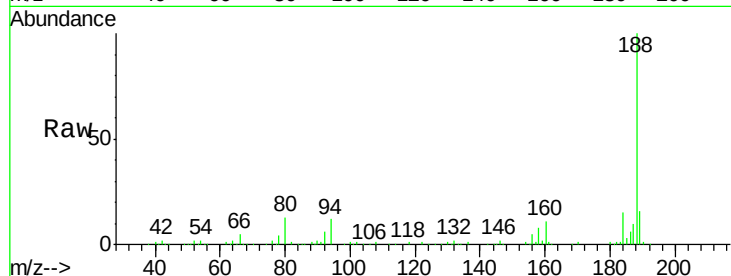


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

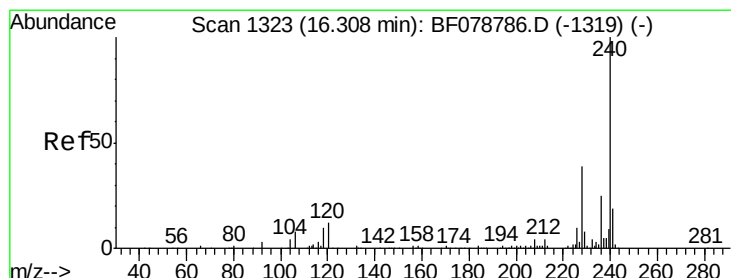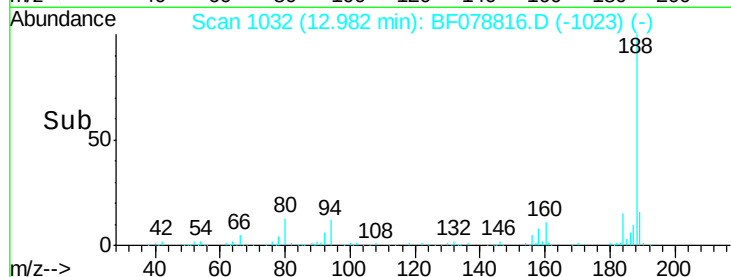
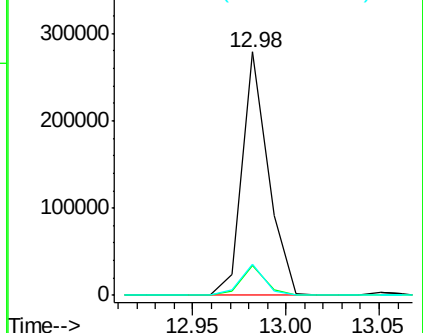



#75
Chrysene-d12
Concen: 20.00 ng
RT: 16.29 min Scan# 1321
Delta R.T. -0.01 min
Lab File: BF078816.D
Acq: 29 Apr 2015 16:35

Tgt Ion:240 Resp: 275821
Ion Ratio Lower Upper
240 100
120 12.3 9.7 14.5
236 25.8 20.2 30.4

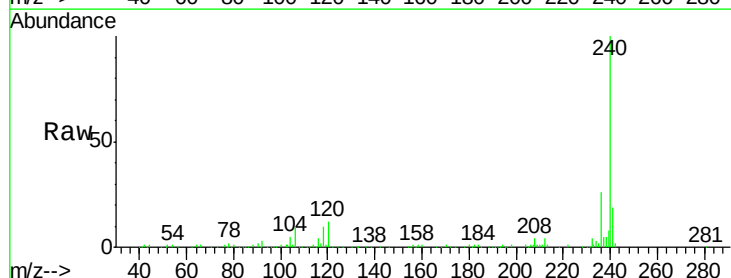

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E



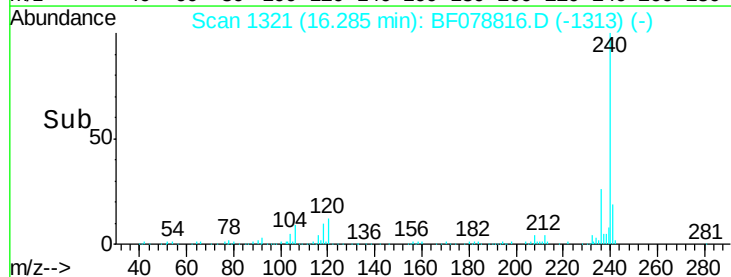
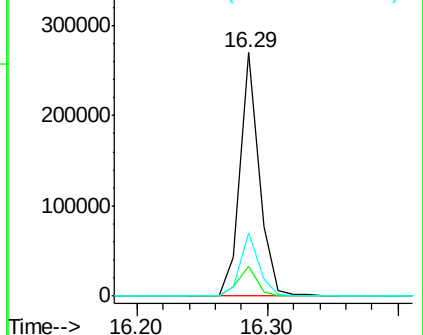


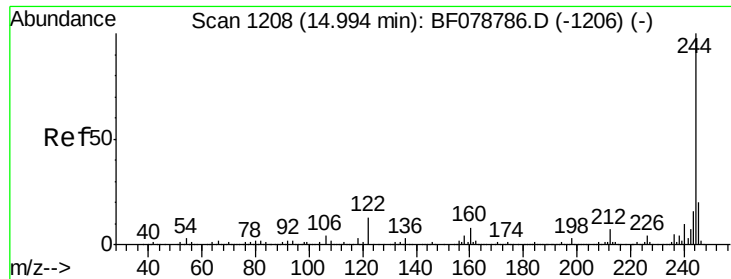

#78
 Terphenyl-d14
 Concen: 80.64 ng
 RT: 14.98 min Scan# 1207
 Delta R.T. -0.00 min
 Lab File: BF078816.D
 Acq: 29 Apr 2015 16:35

Instrument :
 BNA_F
 ClientSampleId :
 PB83015BL

Tgt Ion	Ratio	Lower	Upper
244	100		
212	7.0	5.6	8.4
122	12.9	10.3	15.5

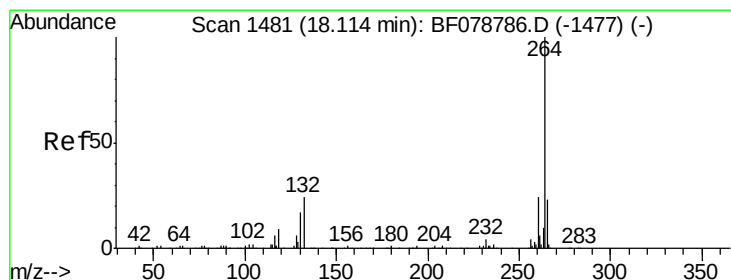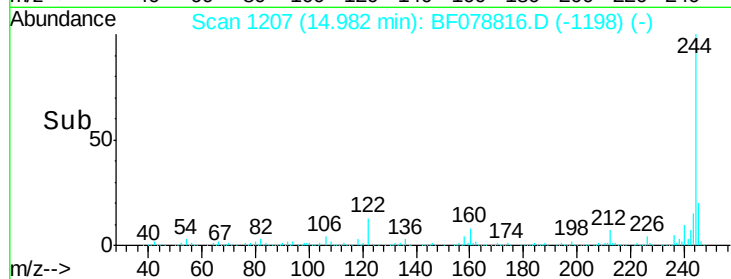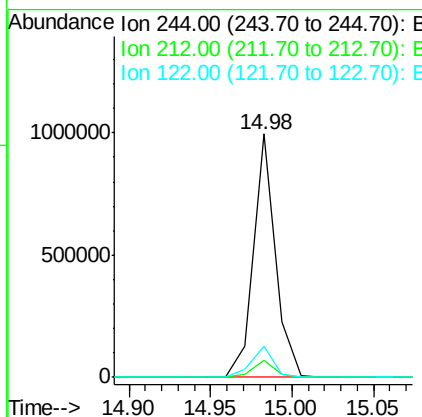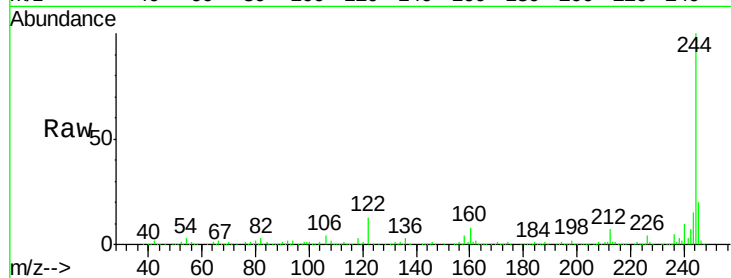

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 18.06 min Scan# 1476
 Delta R.T. -0.02 min
 Lab File: BF078816.D
 Acq: 29 Apr 2015 16:35

Tgt Ion	Ratio	Lower	Upper
264	100		
260	24.1	19.4	29.2
265	21.9	18.3	27.5

