
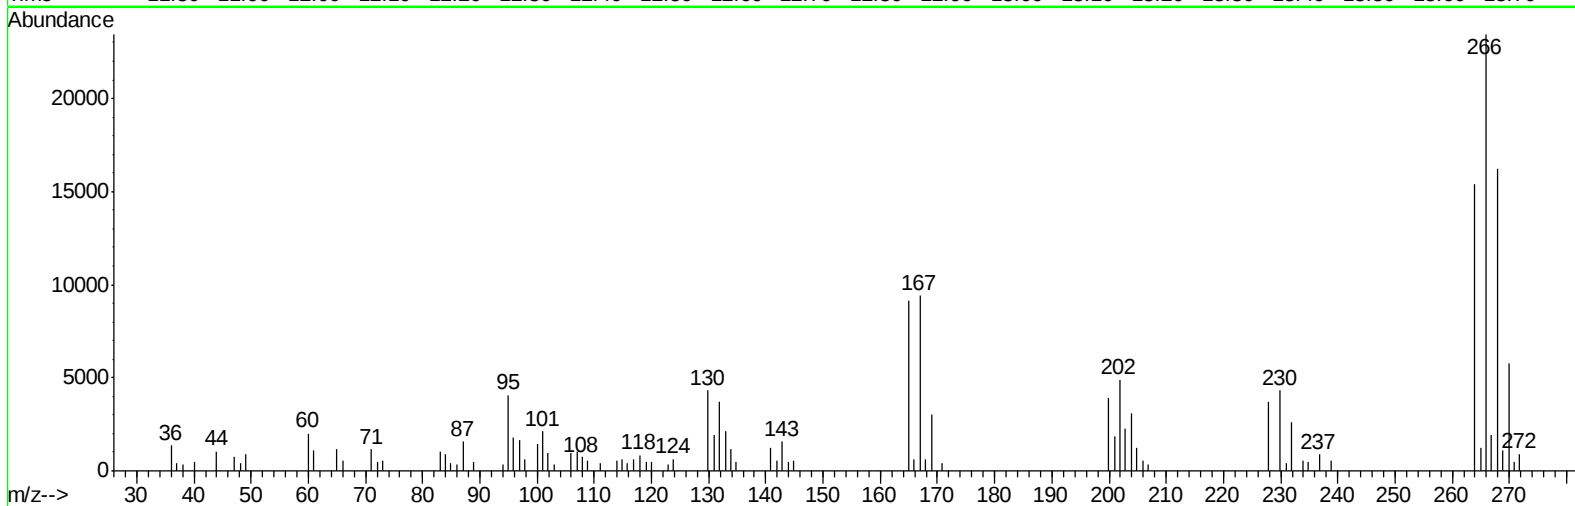


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF042915\
Data File : BF078828.D
Acq On : 29 Apr 2015 23:55
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 30 07:44:50 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 30 01:56:50 2015
Response via : Initial Calibration

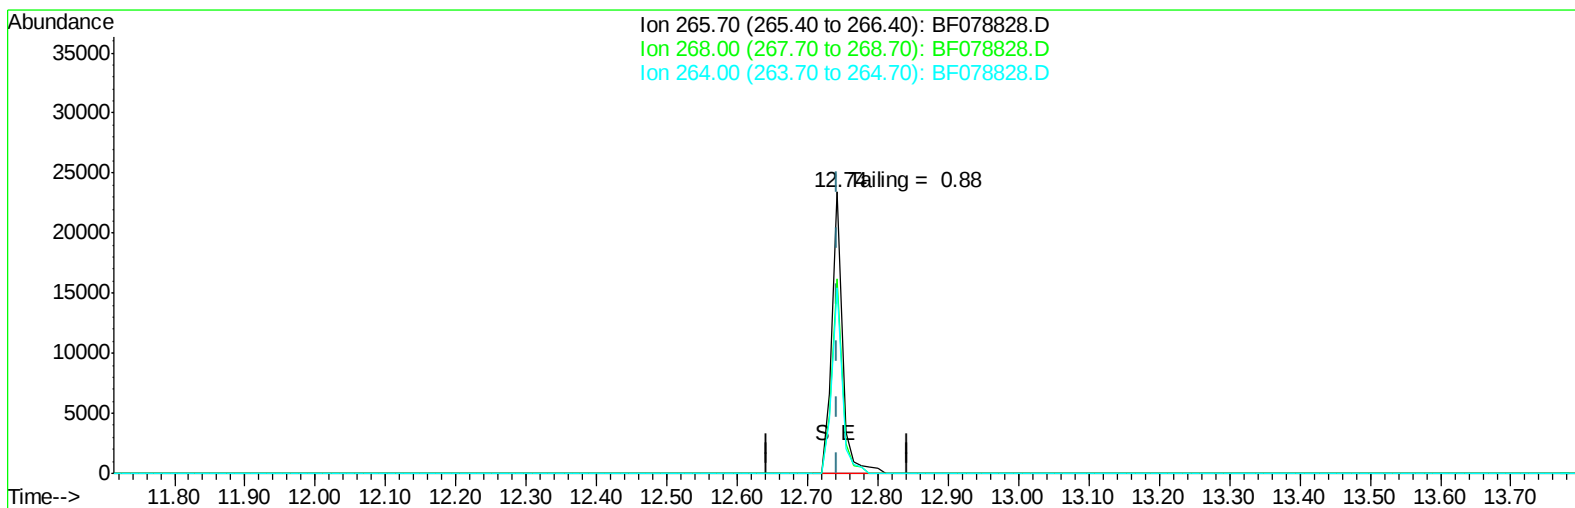

TIC: BF078828.D

(69) Pentachlorophenol (C)



12.742min (+0.000) 0.00ng

response 24736

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	69.26
264.00	60.20	65.73
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF042915\
Data File : BF078828.D
Acq On : 29 Apr 2015 23:55
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 30 07:44:50 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 30 01:56:50 2015
Response via : Initial Calibration

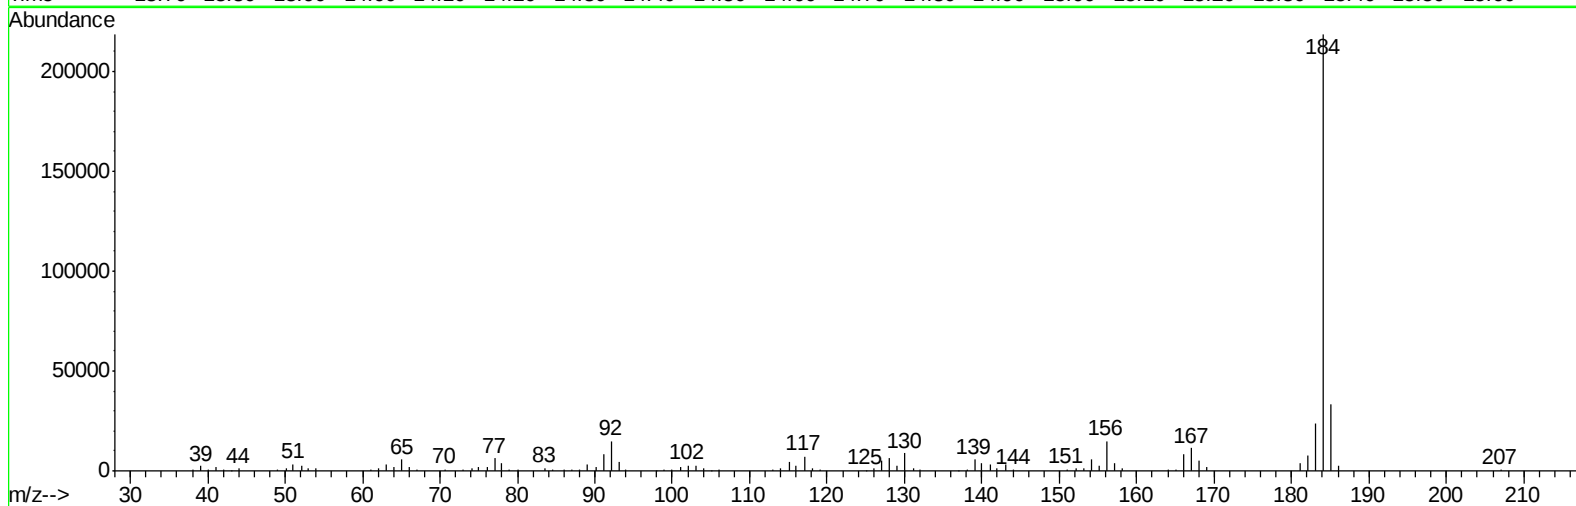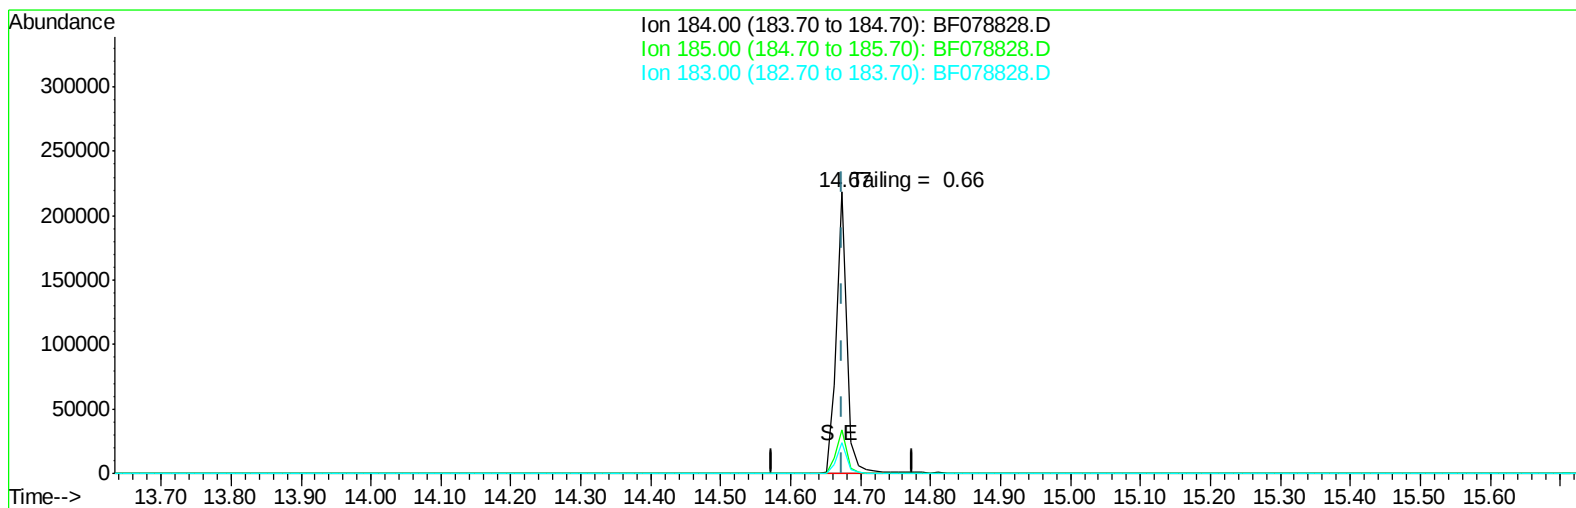

TIC: BF078828.D

(76) Benzidine

14.674min (+0.000) 0.00ng

response 223160

Ion	Exp%	Act%
184.00	100	100
185.00	15.40	15.30
183.00	10.50	10.80
0.00	0.00	0.00