


Data Path : Z:\HPCHEM1\BNA F\Data\BF042915\
Data File : BF078805.D
Acq On : 29 Apr 2015 10:20
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042815.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Apr 29 11:41:09 2015

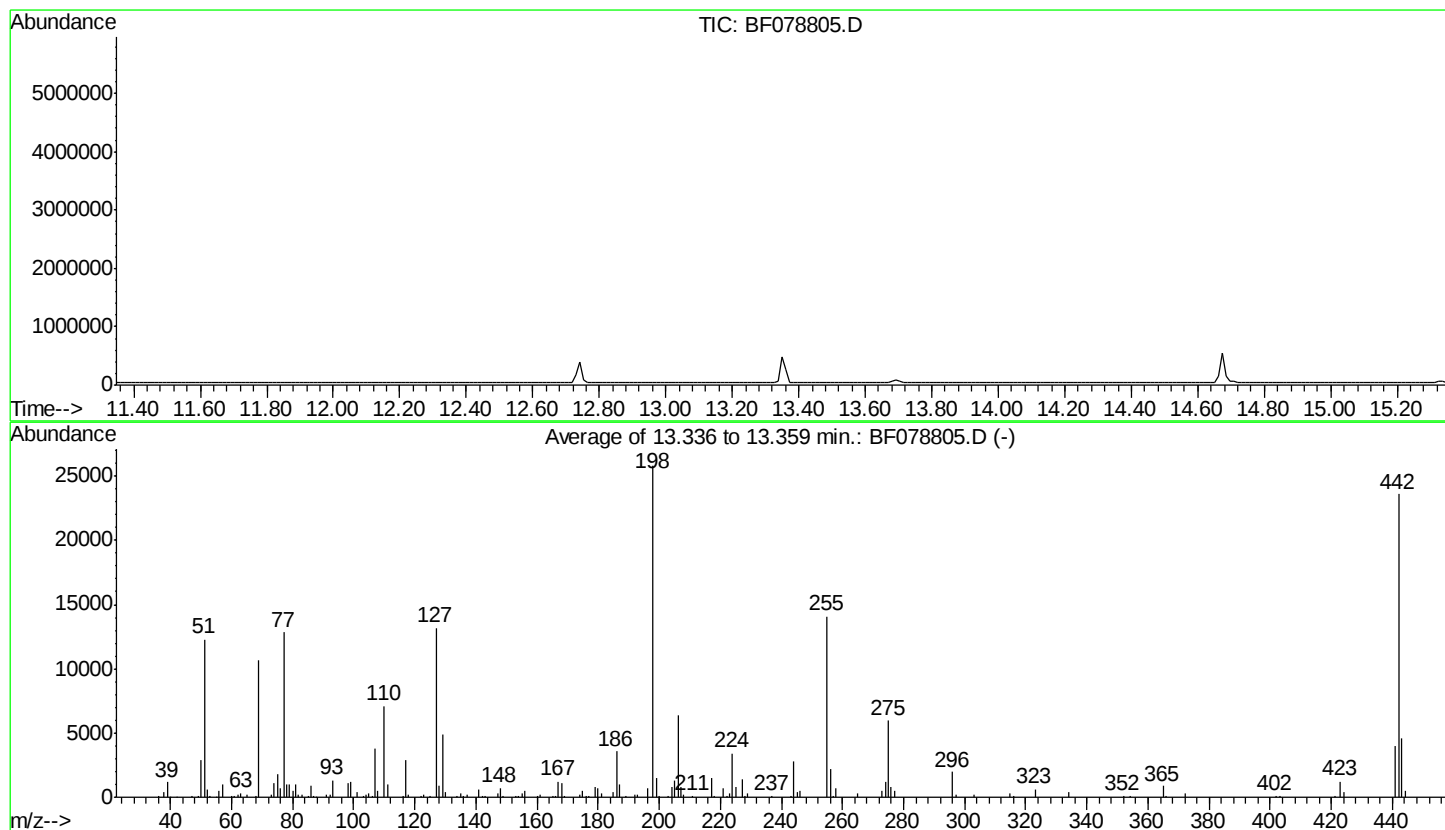

AutoFind: Scans 1063, 1064, 1065; Background Corrected with Scan 1060

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.7	12305	PASS
68	69	0.00	2	1.3	142	PASS
69	198	0.00	100	41.3	10664	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.0	13167	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	25814	PASS
199	198	5	9	5.8	1489	PASS
275	198	10	60	23.0	5937	PASS
365	198	1	100	3.3	861	PASS
441	442	0.01	24	16.8	3975	PASS
442	198	50	100	91.4	23600	PASS
443	442	15	24	19.5	4592	PASS