


Data Path : Z:\HPCHEM1\BNA F\Data\BF042915\
 Data File : BF078828.D
 Acq On : 29 Apr 2015 23:55
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042815.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 29 11:41:09 2015

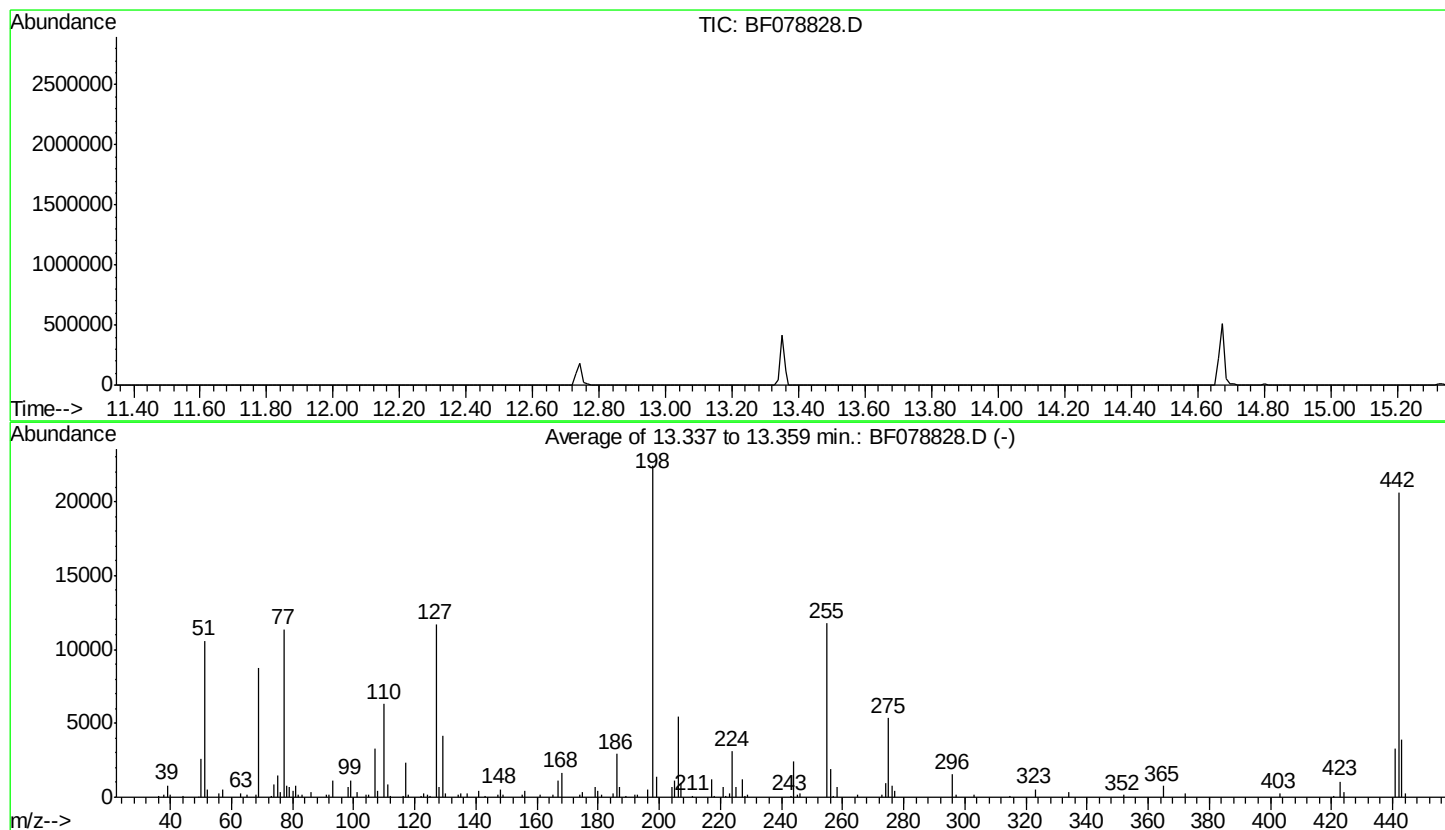

AutoFind: Scans 1063, 1064, 1065; Background Corrected with Scan 1060

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.3	10610	PASS
68	69	0.00	2	1.7	151	PASS
69	198	0.00	100	39.1	8767	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.1	11679	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	22433	PASS
199	198	5	9	6.1	1370	PASS
275	198	10	60	23.9	5355	PASS
365	198	1	100	3.5	775	PASS
441	442	0.01	24	16.0	3297	PASS
442	198	50	100	91.8	20584	PASS
443	442	15	24	19.0	3907	PASS