
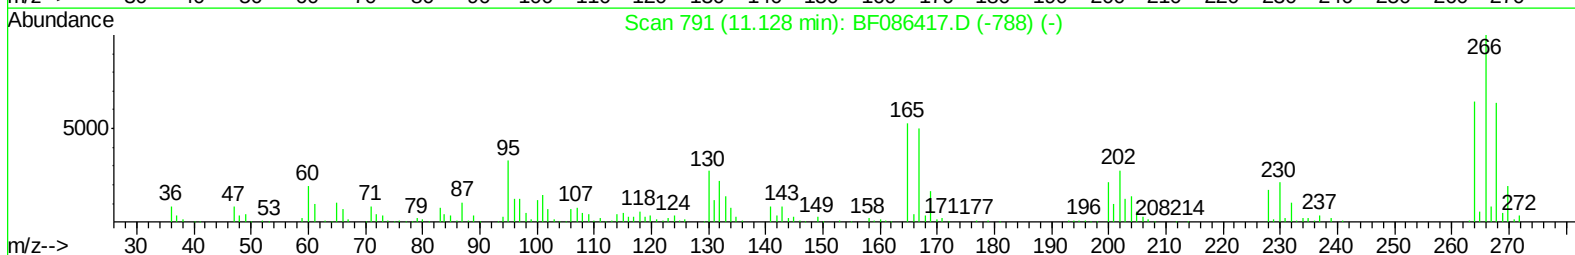
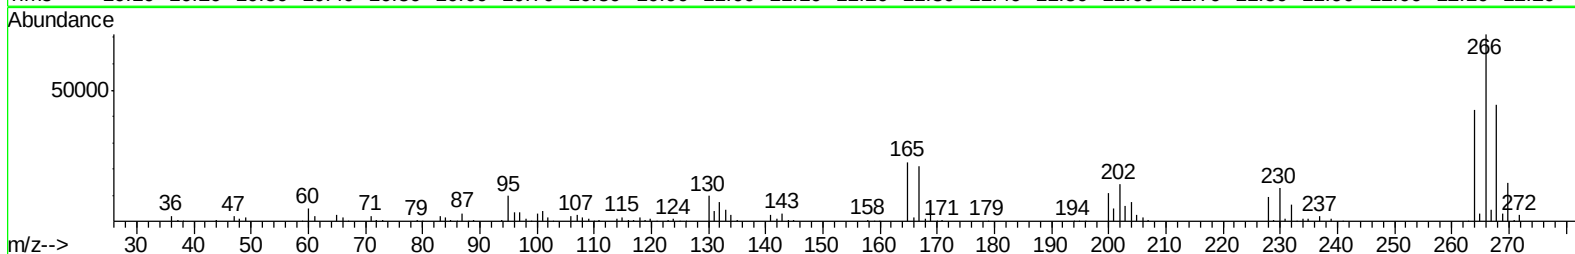


Data Path : Z:\HPCHEM1\BNA_F\Data\BF042916\
Data File : BF086487.D
Acq On : 29 Apr 2016 12:15
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 29 12:39:53 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 27 14:20:52 2016
Response via : Initial Calibration

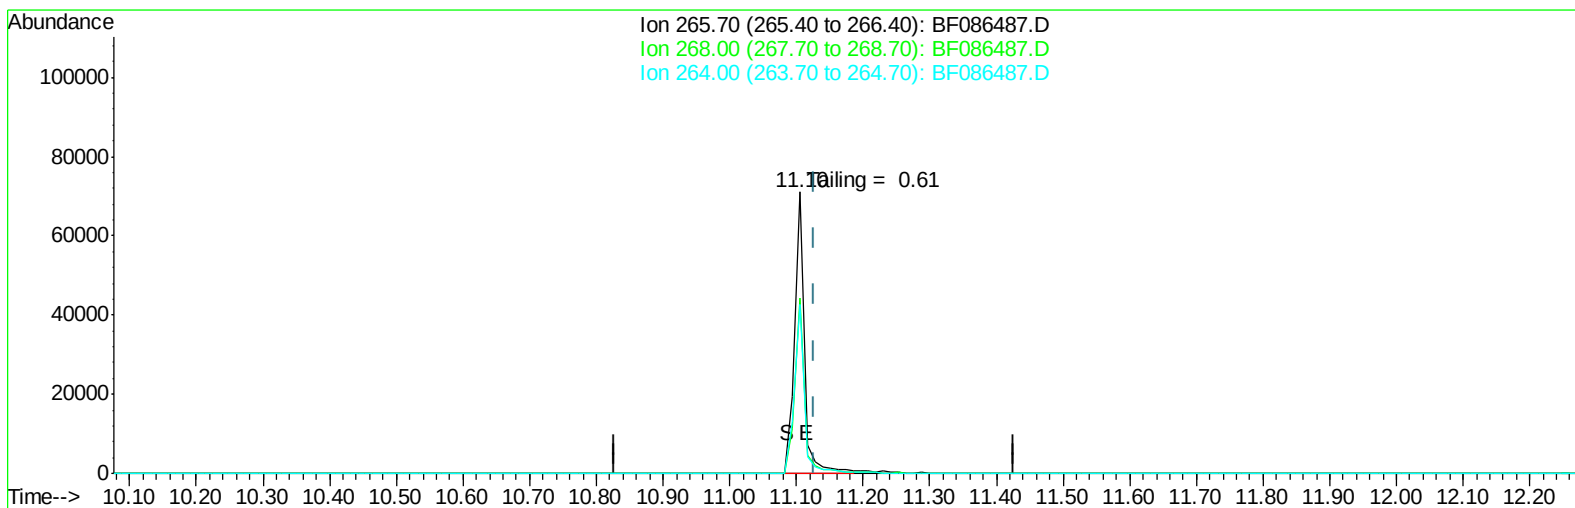

TIC: BF086487.D

(69) Pentachlorophenol (C)




11.105min (-0.023) 37698.42ng

response 74912

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	62.46
264.00	66.10	60.13
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF042916\
Data File : BF086487.D
Acq On : 29 Apr 2016 12:15
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 29 12:39:53 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 27 14:20:52 2016
Response via : Initial Calibration

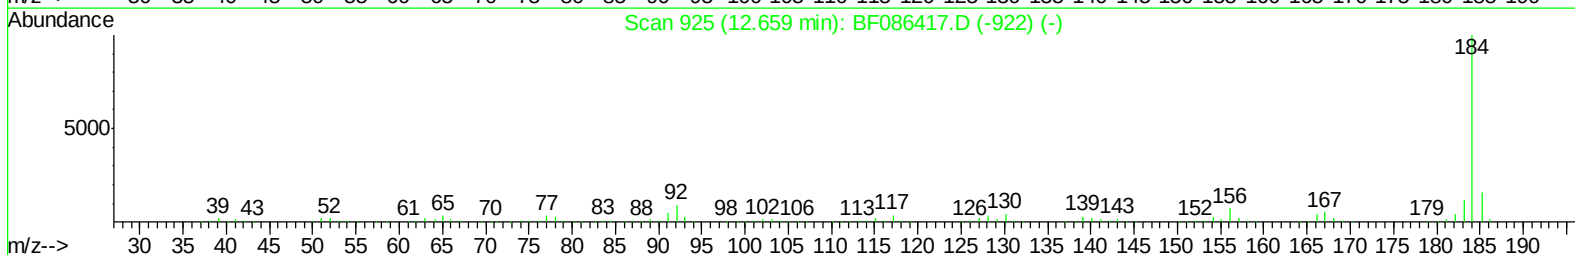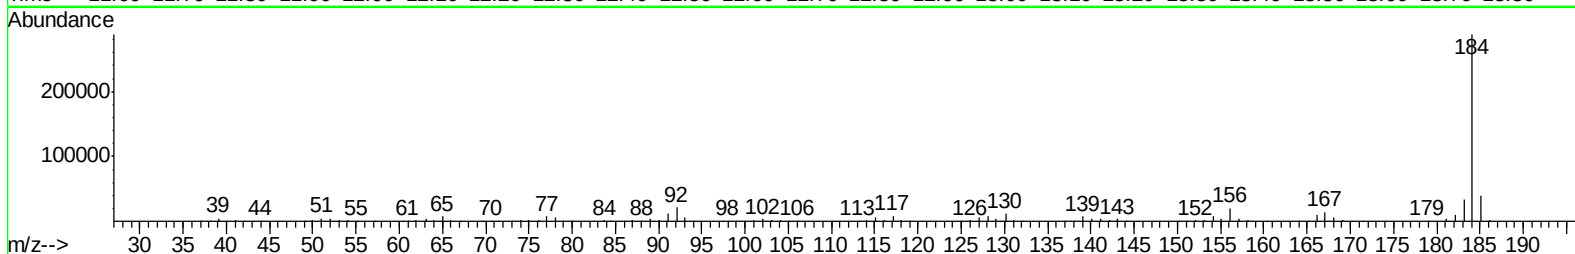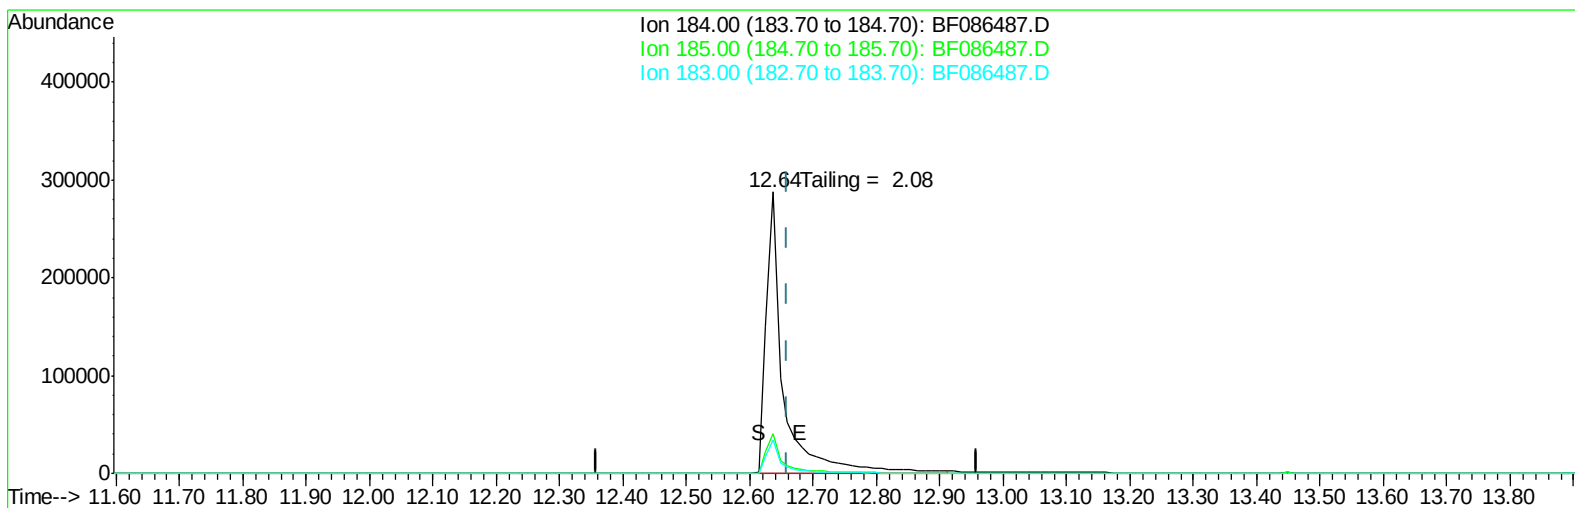

TIC: BF086487.D

(76) Benzidine

12.636min (-0.023) 0.00ng

response 543034

Ion	Exp%	Act%
184.00	100	100
185.00	17.00	14.12
183.00	12.20	11.79
0.00	0.00	0.00