

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF042916\
 Data File : BF086510.D
 Acq On : 29 Apr 2016 23:49
 Operator : UM/SJ
 Sample : H2685-10 8X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 26WARD-2B-CS-1(0-10FTBGS)

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.933	247	249	252	rBV	13937	17733	1.46%	0.201%
2	5.367	284	287	289	rBV	246054	346533	28.46%	3.935%
3	6.407	376	378	388	rBV	260692	397165	32.62%	4.510%
4	6.544	388	390	394	rBV	389007	416524	34.21%	4.730%
5	6.773	408	410	413	rBV	844825	914636	75.11%	10.386%
6	6.933	421	424	426	rBV	349660	331086	27.19%	3.760%
7	7.345	457	460	466	rBV	112627	219451	18.02%	2.492%
8	7.550	476	478	485	rVB	5538	13209	1.08%	0.150%
9	8.065	520	523	525	rBV	1374364	1217693	100.00%	13.827%
10	9.139	615	617	623	rBV	490458	438455	36.01%	4.979%
11	9.539	650	652	657	rVB	58774	60631	4.98%	0.688%
12	9.813	674	676	679	rBV	1174676	1184352	97.26%	13.449%
13	10.259	711	715	716	rBV	17284	21825	1.79%	0.248%
14	10.476	730	734	737	rBV	10300	19308	1.59%	0.219%
15	10.602	743	745	751	rBV	167421	178554	14.66%	2.028%
16	10.728	754	756	761	rVB	24393	32479	2.67%	0.369%
17	10.842	763	766	771	rVB4	10262	22409	1.84%	0.254%
18	11.299	804	806	808	rBV	930426	914030	75.06%	10.379%
19	11.676	837	839	844	rVB3	8865	19083	1.57%	0.217%
20	11.871	854	856	858	rBV3	8543	16244	1.33%	0.184%
21	12.499	909	911	913	rBV3	17271	25668	2.11%	0.291%
22	12.728	927	931	935	rBV2	22031	66590	5.47%	0.756%
23	12.877	942	944	948	rBV	275804	305059	25.05%	3.464%
24	13.779	1021	1023	1026	rBV	36505	55544	4.56%	0.631%
25	13.928	1033	1036	1041	rBV	766000	899208	73.85%	10.211%
26	15.322	1156	1158	1166	rVB	373752	673058	55.27%	7.643%


Sum of corrected areas: 8806527

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF042916\
Data File : BF086510.D
Acq On : 29 Apr 2016 23:49
Operator : UM/SJ
Sample : H2685-10 8X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
26WARD-2B-CS-1(0-10FTBGS)

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

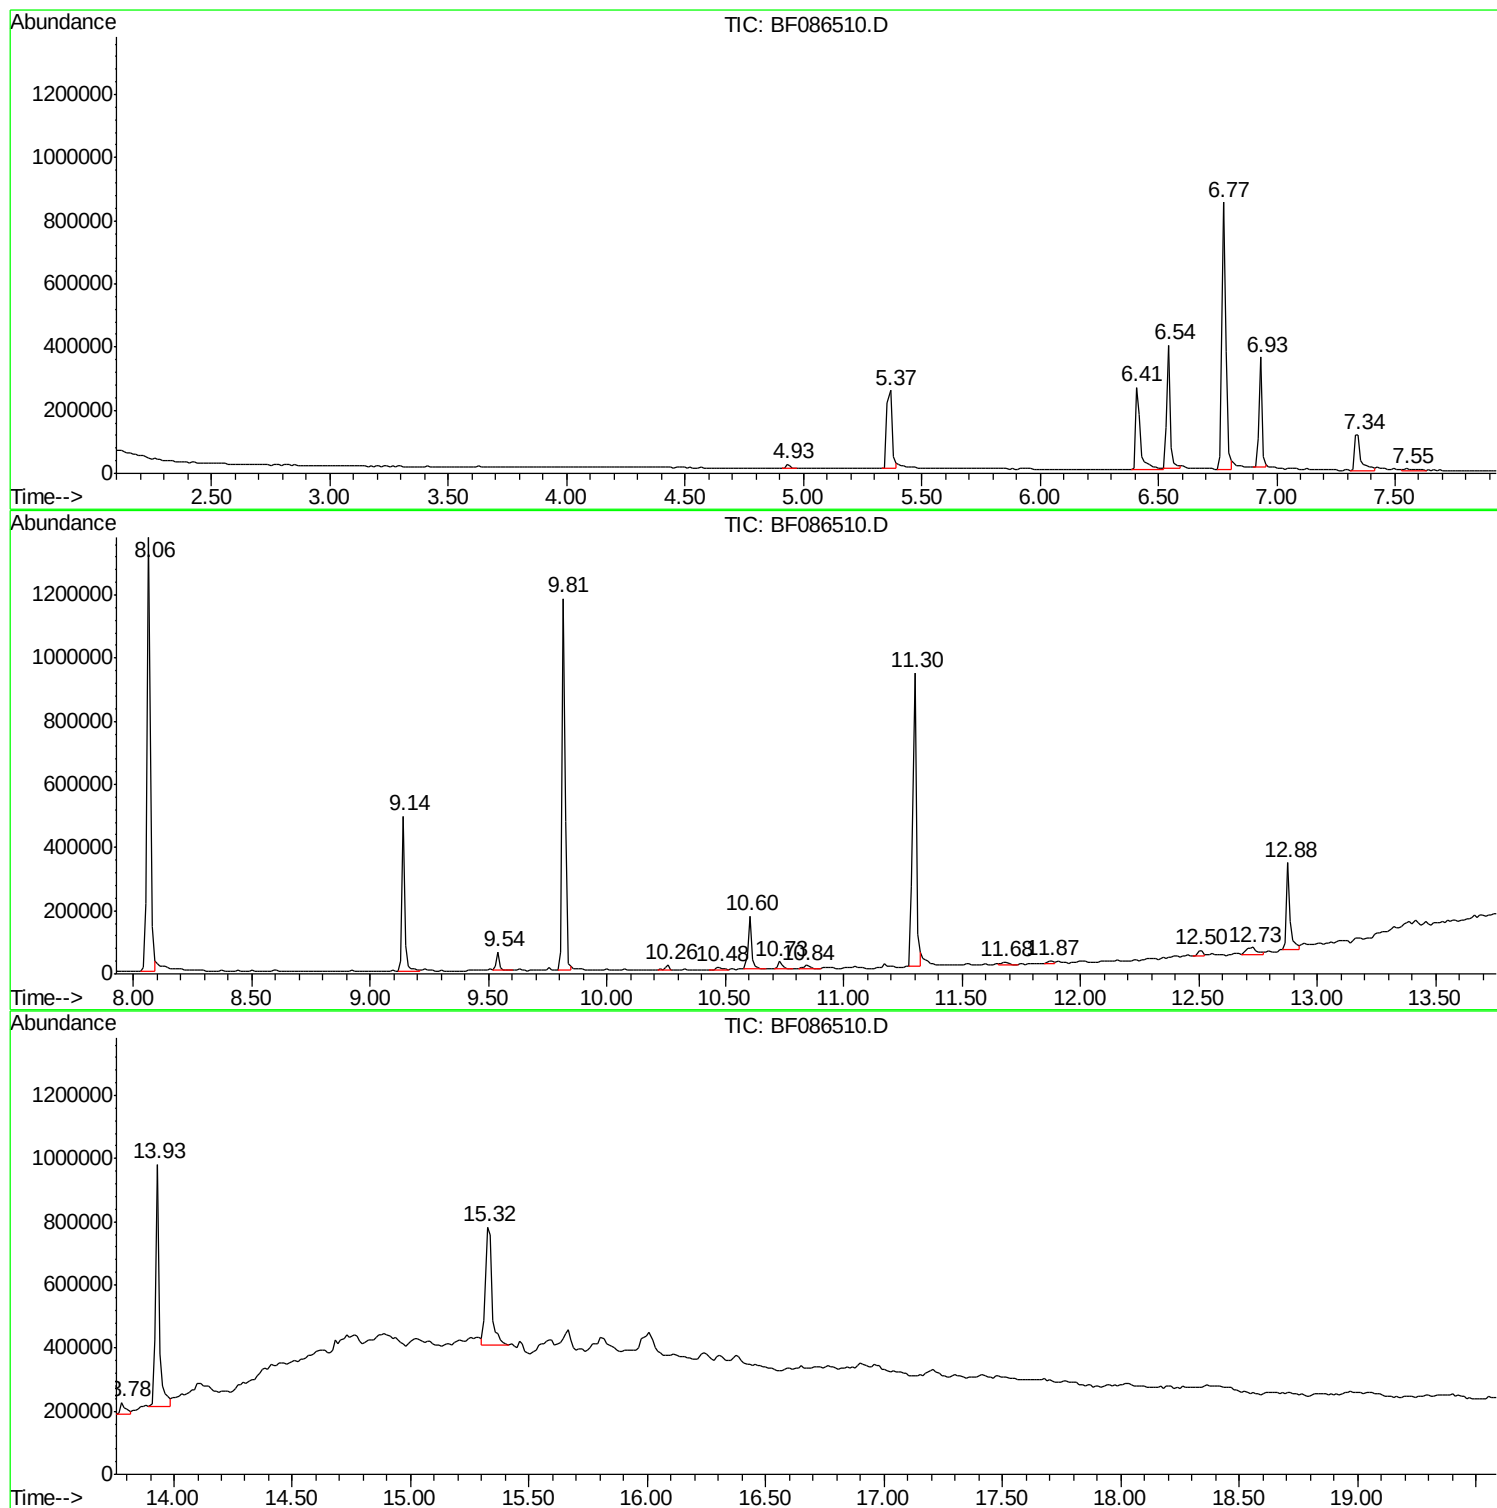

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF042916\
Data File : BF086510.D
Acq On : 29 Apr 2016 23:49
Operator : UM/SJ
Sample : H2685-10 8X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
26WARD-2B-CS-1(0-10FTBGS)










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.54 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.54	9.11 ng	416524	1,4-Dichlorobenzene-d4	6.77

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	16
3		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	12
4		Benzene, 1,3,5-trifluoro-	132	C6H3F3	000372-38-3	9
5		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9

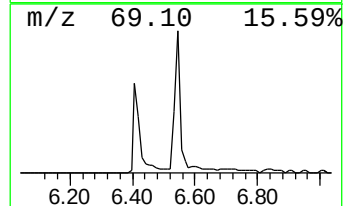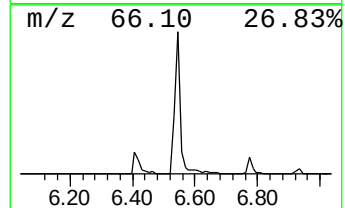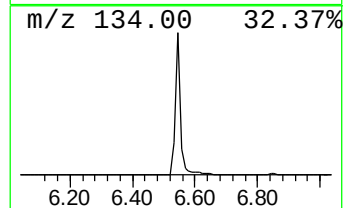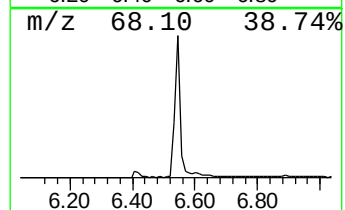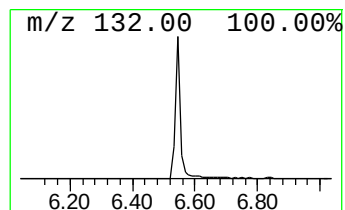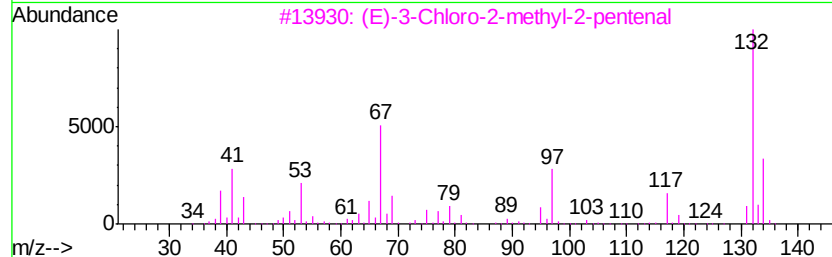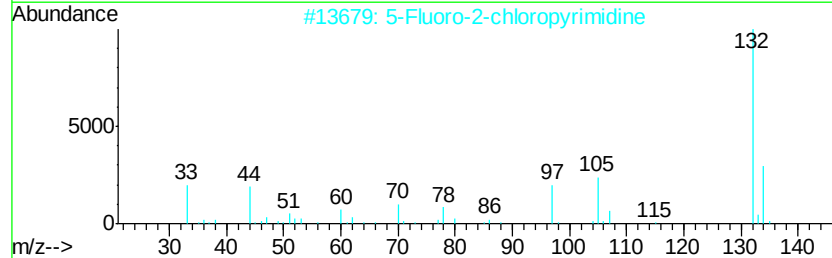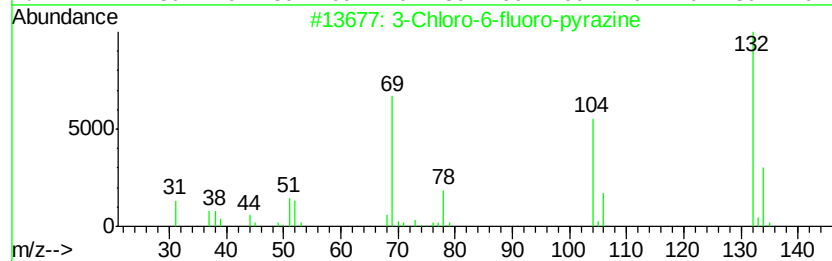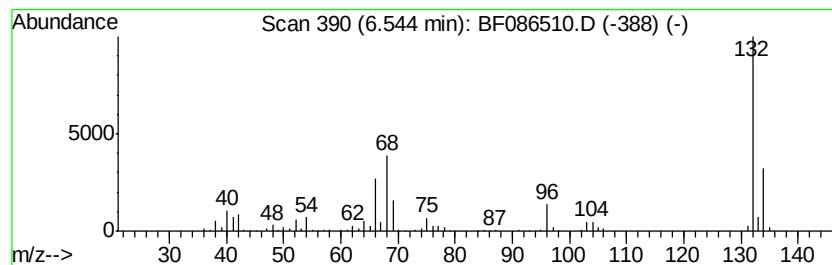

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF042916\
Data File : BF086510.D
Acq On : 29 Apr 2016 23:49
Operator : UM/SJ
Sample : H2685-10 8X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
26WARD-2B-CS-1(0-10FTBGS)

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.54	6.54	9.1	ng	416524	1	6.77	914636	20.0