


Data Path : Z:\HPCHEM1\BNA F\DATA\BF042916\
 Data File : BF086487.D
 Acq On : 29 Apr 2016 12:15
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 27 14:20:52 2016

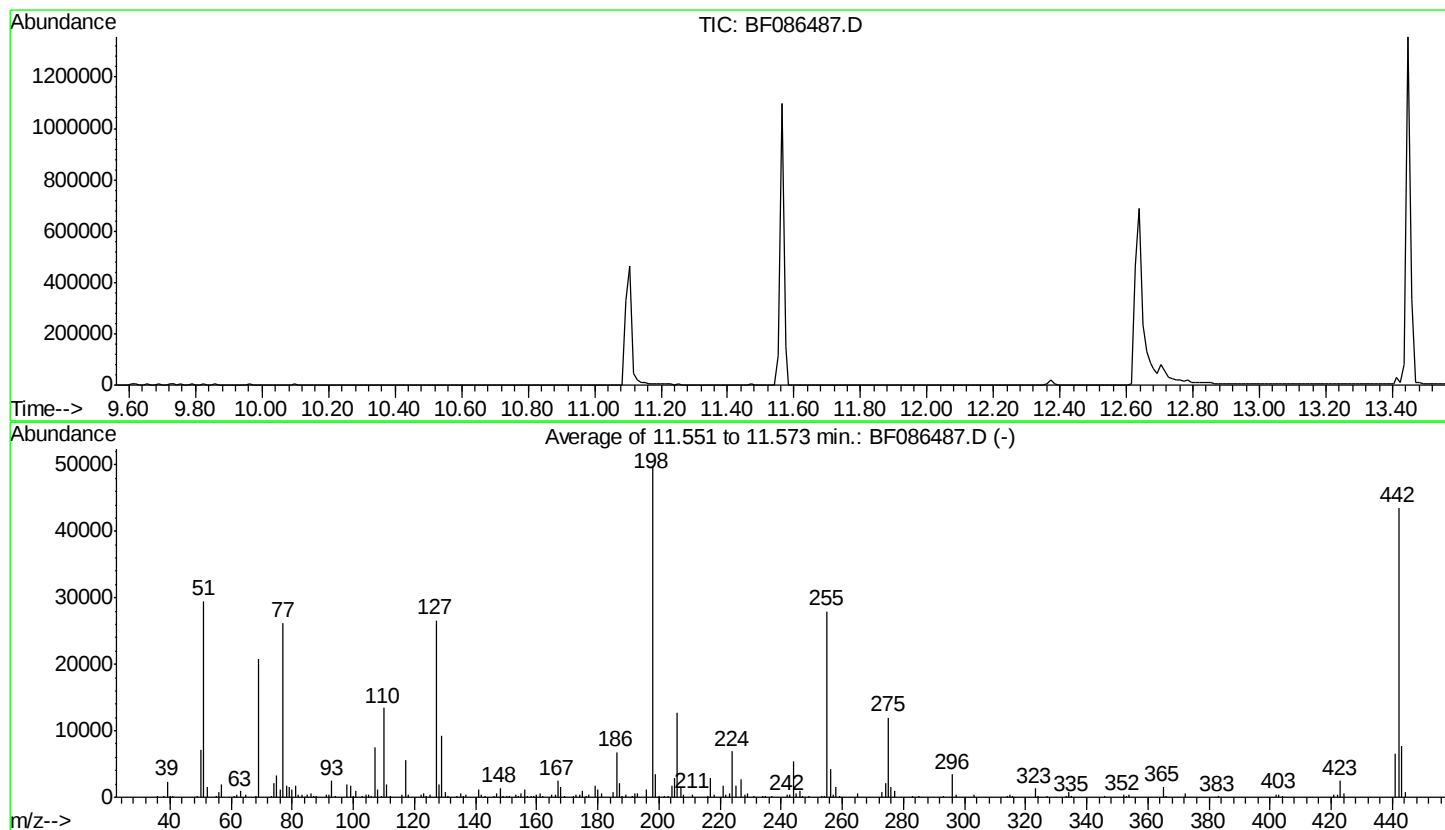

AutoFind: Scans 828, 829, 830; Background Corrected with Scan 825

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	59.2	29547	PASS
68	69	0.00	2	1.3	281	PASS
69	198	0.00	100	41.8	20846	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.4	26615	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	49876	PASS
199	198	5	9	6.9	3448	PASS
275	198	10	60	24.0	11979	PASS
365	198	1	100	3.2	1587	PASS
441	442	0.01	24	15.0	6531	PASS
442	198	50	100	87.4	43576	PASS
443	442	15	24	17.7	7707	PASS