


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042919\
 Data File : BF114016.D
 Acq On : 29 Apr 2019 11:19
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 23 03:32:35 2019

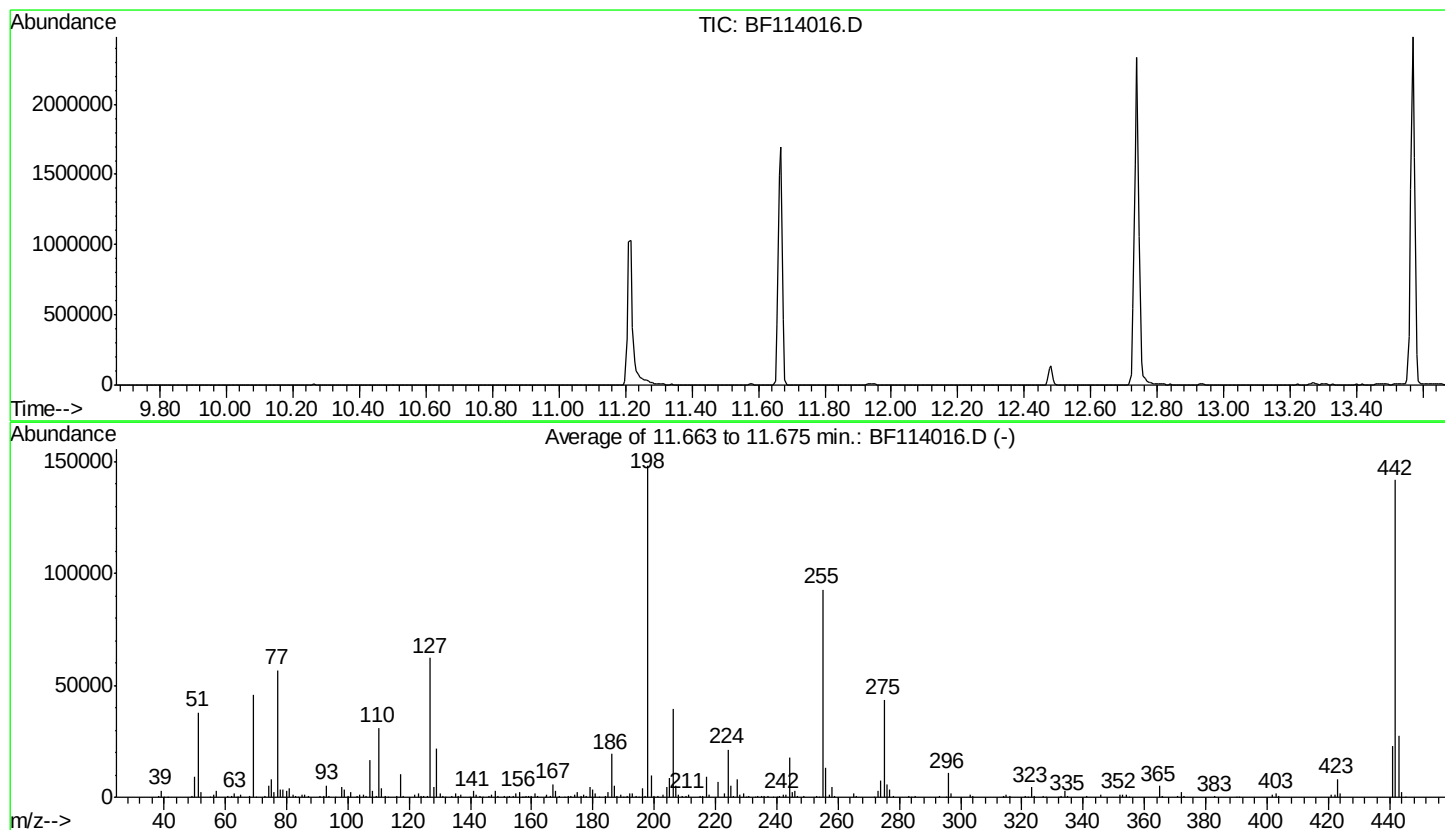

AutoFind: Scans 1628, 1629, 1630; Background Corrected with Scan 1623

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.6	37921	PASS
68	69	0.00	2	1.6	730	PASS
69	198	0.00	100	31.0	45906	PASS
70	69	0.00	2	0.3	157	PASS
127	198	10	80	41.9	62194	PASS
197	198	0.00	2	0.3	406	PASS
198	198	100	100	100.0	148280	PASS
199	198	5	9	6.8	10028	PASS
275	198	10	60	29.3	43506	PASS
365	198	1	100	3.4	5088	PASS
441	198	0.01	100	15.5	22962	PASS
442	198	50	100	95.7	141834	PASS
443	442	15	24	19.6	27778	PASS