
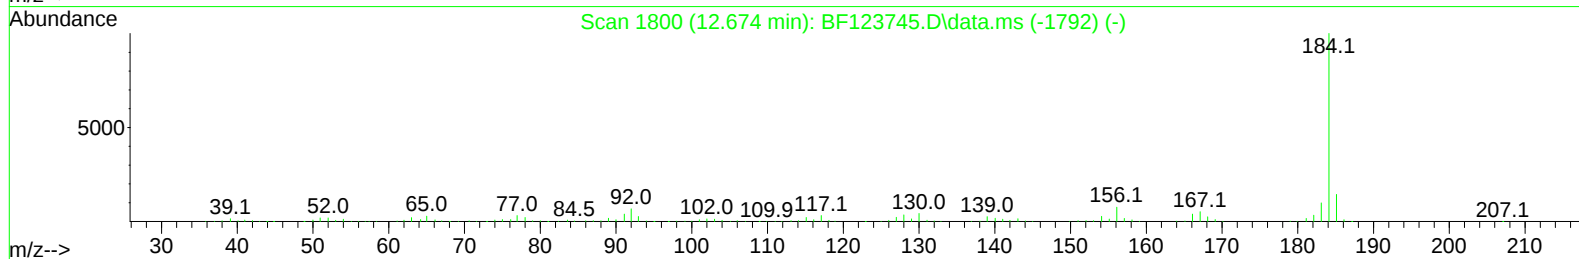
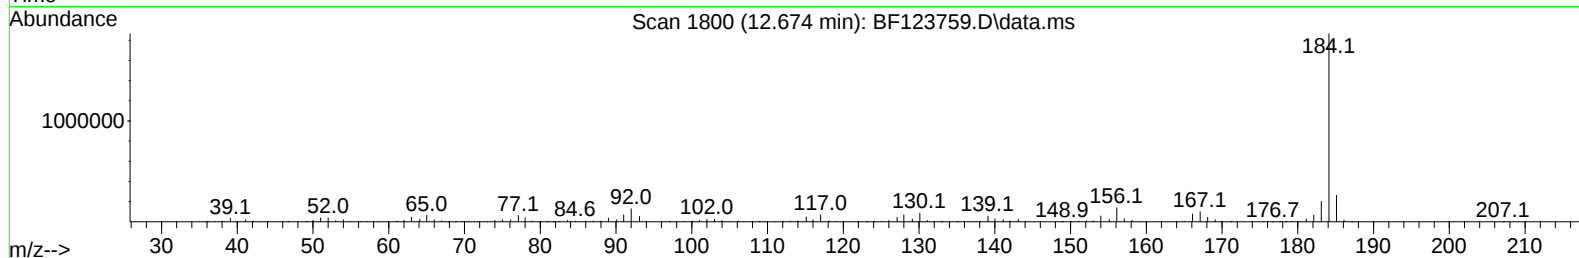


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042921\
Data File : BF123759.D
Acq On : 29 Apr 2021 9:20
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 29 11:05:21 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 27 16:30:39 2021
Response via : Initial Calibration

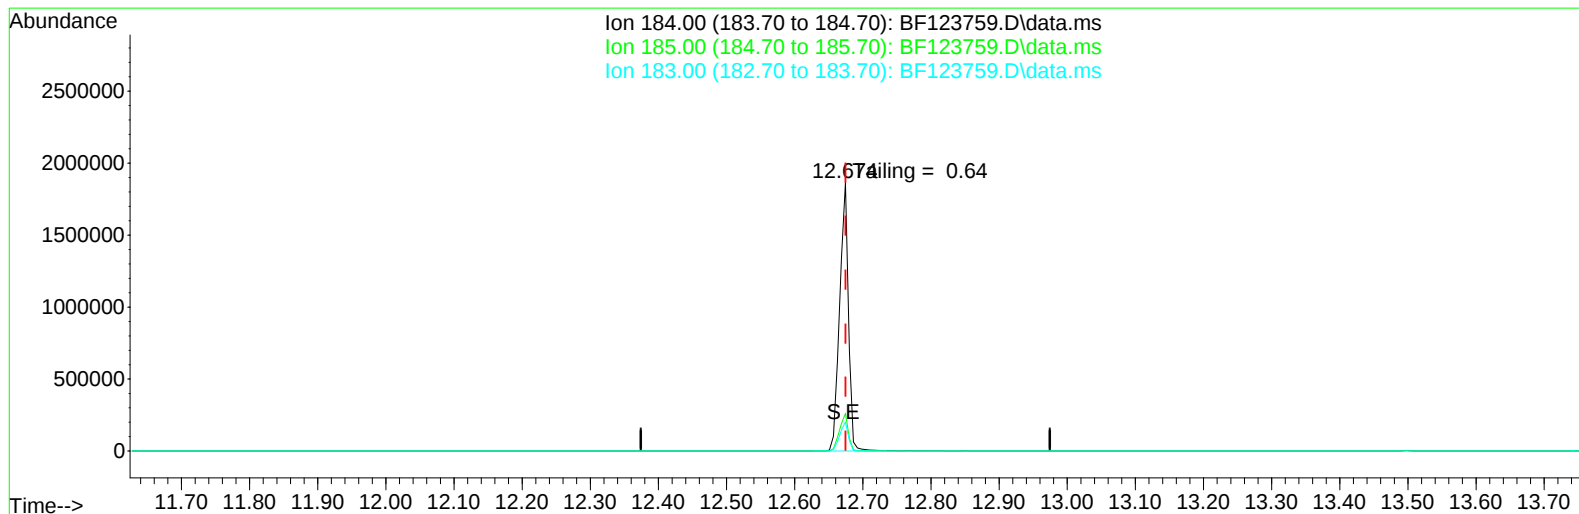

TIC: BF123759.D\data.ms

(77) Benzidine




12.674min (-0.000) 0.00 ng

response 1679893

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.06
183.00	9.80	10.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042921\
Data File : BF123759.D
Acq On : 29 Apr 2021 9:20
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 29 11:05:21 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 27 16:30:39 2021
Response via : Initial Calibration

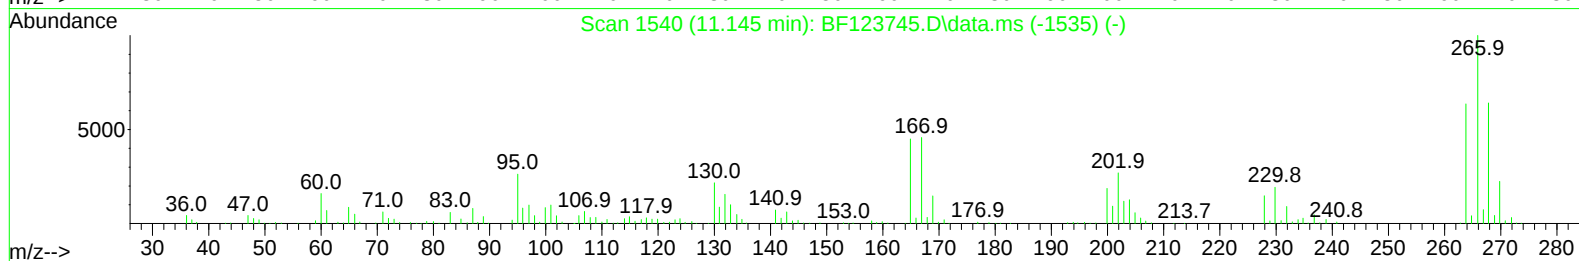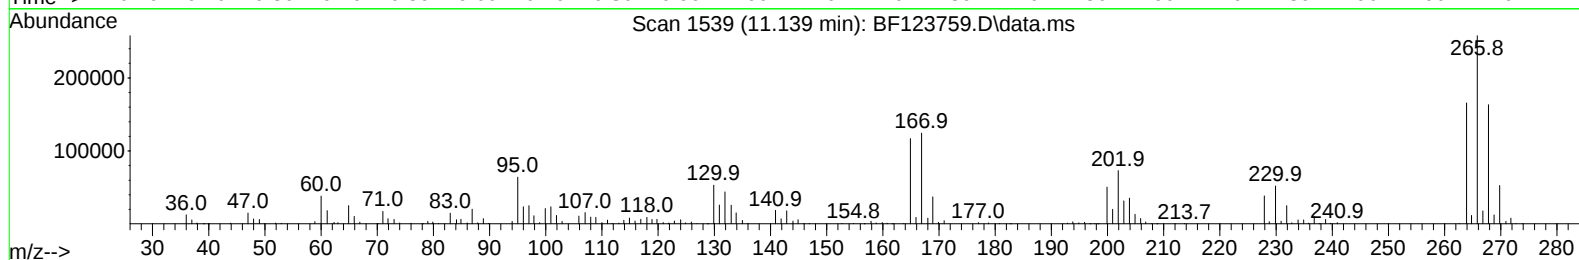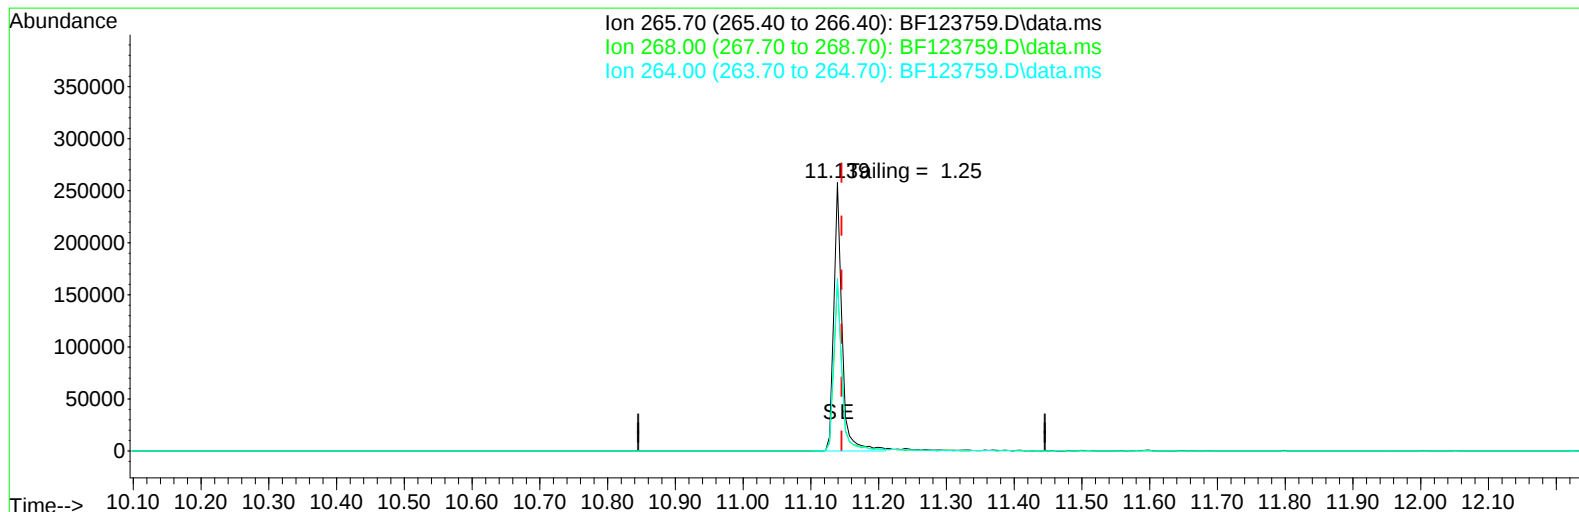

TIC: BF123759.D\data.ms

(70) Pentachlorophenol (C)

11.139min (-0.006) 28285.54 ng

response 222906

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.36
264.00	65.70	64.28
0.00	0.00	0.00