
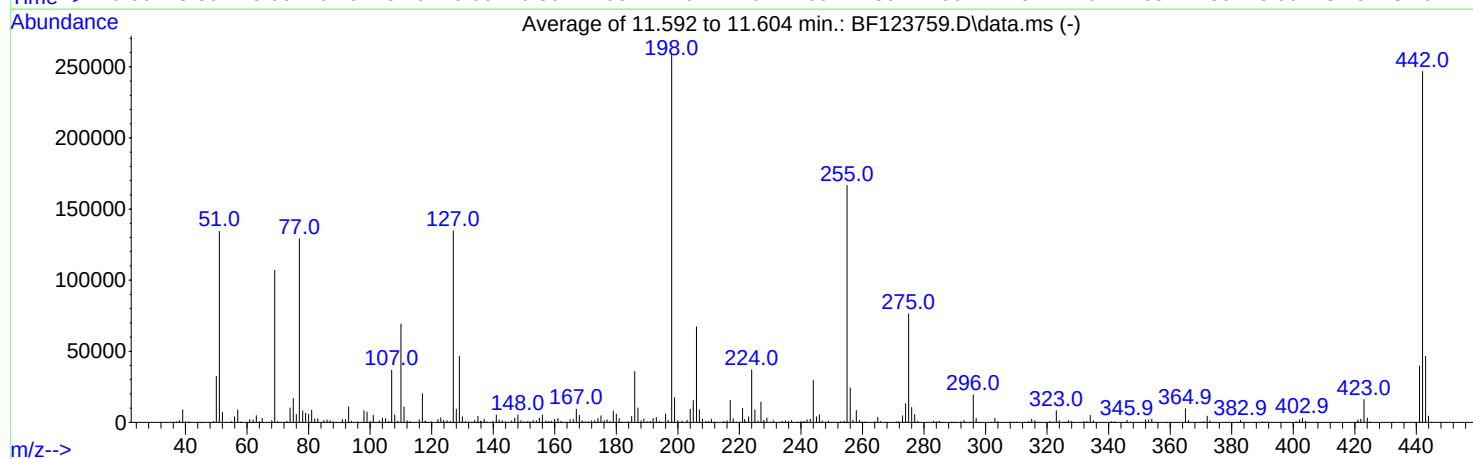


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042921\
 Data File : BF123759.D
 Acq On : 29 Apr 2021 9:20
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 27 16:30:39 2021

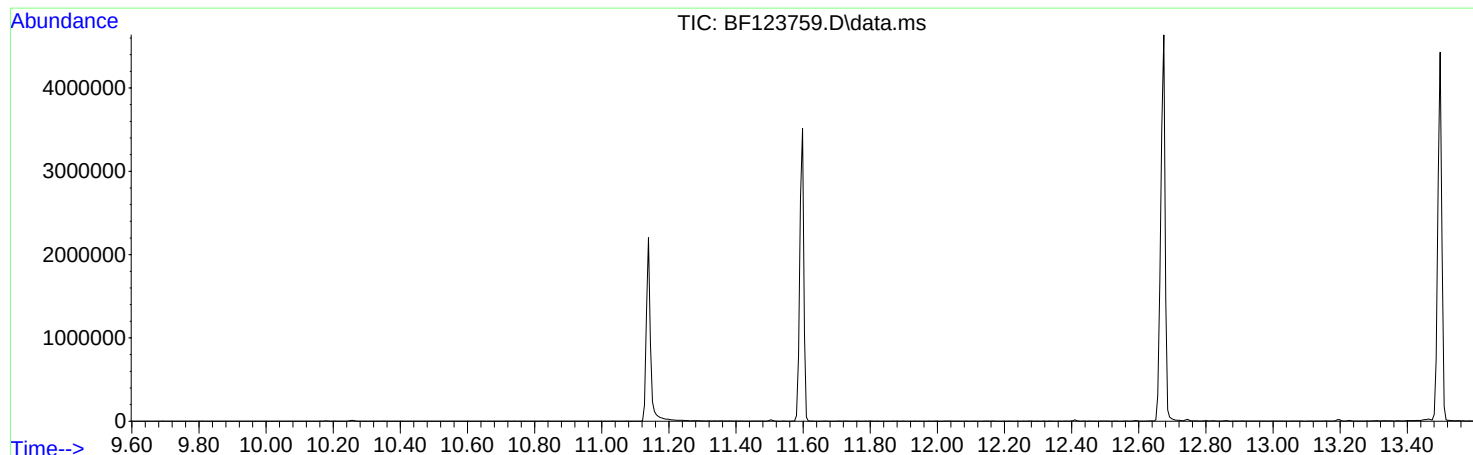




AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1611

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.9	134373	PASS
68	69	0.00	2	1.2	1239	PASS
69	198	0.00	100	41.4	107011	PASS
70	69	0.00	2	0.5	545	PASS
127	198	10	80	52.0	134637	PASS
197	198	0.00	2	0.6	1479	PASS
198	198	100	100	100.0	258677	PASS
199	198	5	9	6.7	17410	PASS
275	198	10	60	29.5	76299	PASS
365	198	1	100	3.7	9539	PASS
441	198	0.01	100	15.3	39579	PASS
442	442	50	100	100.0	246699	PASS
443	442	15	24	18.8	46464	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042921\
Data File : BF123759.D
Acq On : 29 Apr 2021 9:20
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 29 11:05:21 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 27 16:30:39 2021
Response via : Initial Calibration

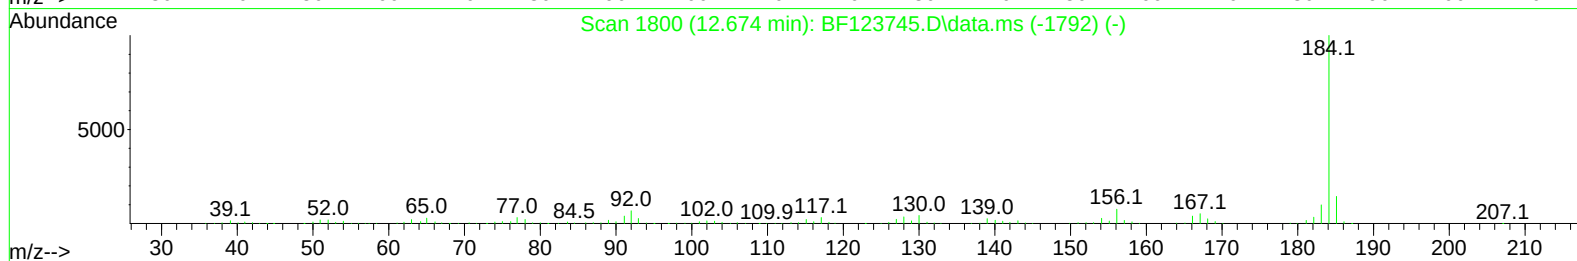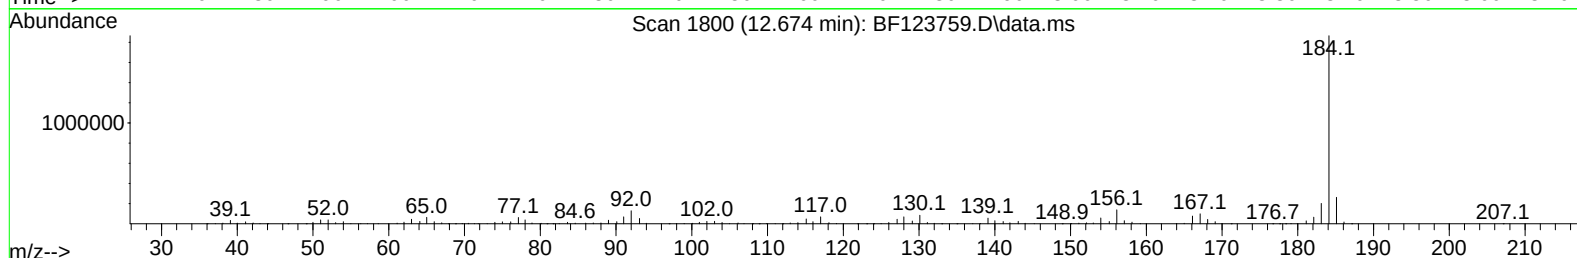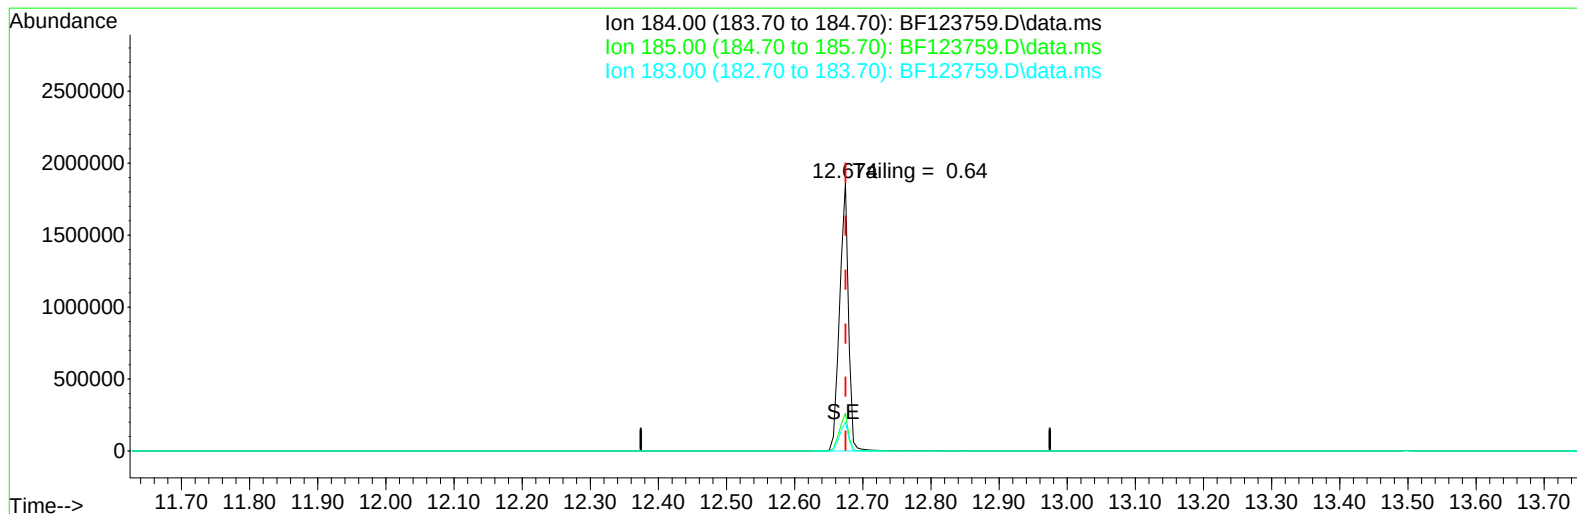

TIC: BF123759.D\data.ms

(77) Benzidine

12.674min (-0.000) 0.00 ng




response 1679893

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.06
183.00	9.80	10.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042921\
Data File : BF123759.D
Acq On : 29 Apr 2021 9:20
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 29 11:05:21 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 27 16:30:39 2021
Response via : Initial Calibration

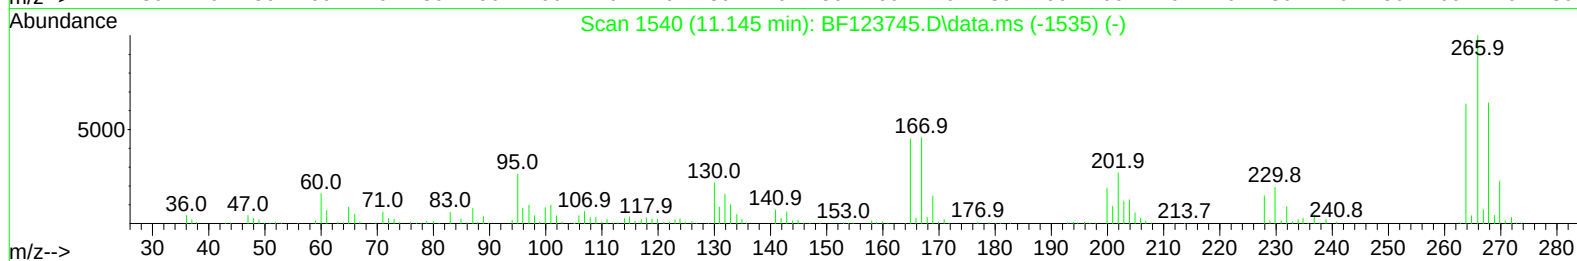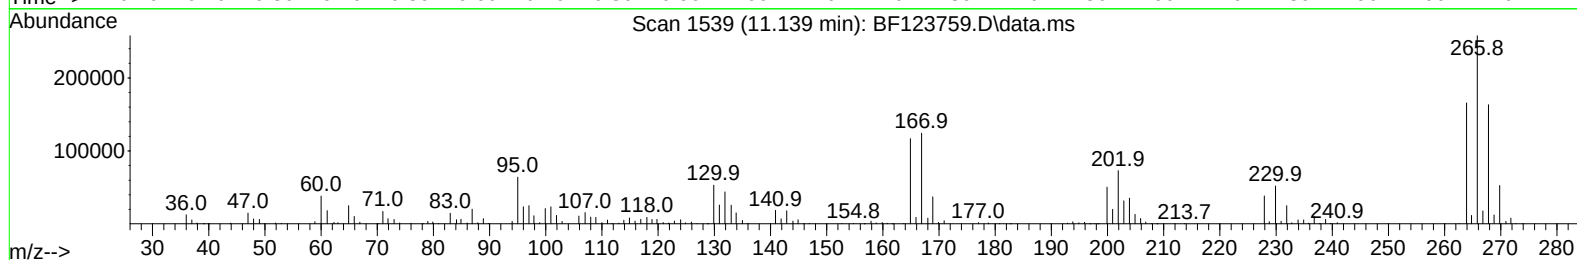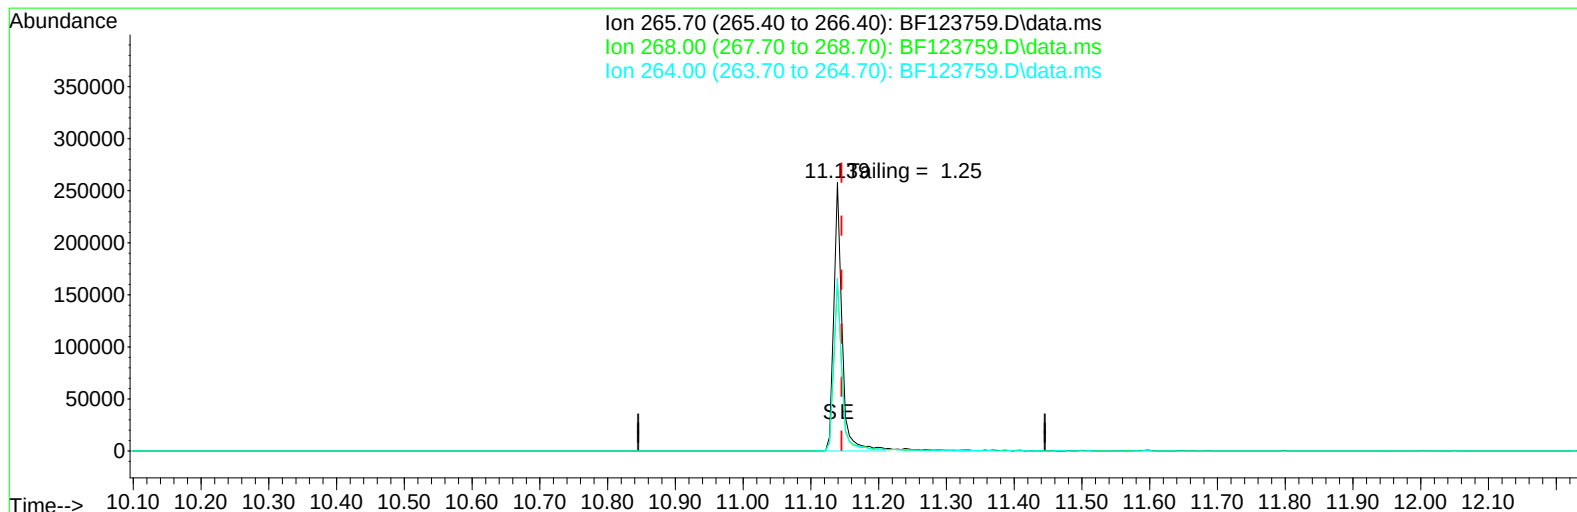

TIC: BF123759.D\data.ms

(70) Pentachlorophenol (C)

11.139min (-0.006) 28285.54 ng

response 222906

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.36
264.00	65.70	64.28
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/29/2021	BNA_F	<u>BF123759.D</u>
Compound Name	Response	Retention Time
DDT	693032	13.49
DDD	4114	13.19
DDE	1205	12.86
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5319	698351	0.76

Instrument :
BNA_F
ClientSampleId :
DFTPP