
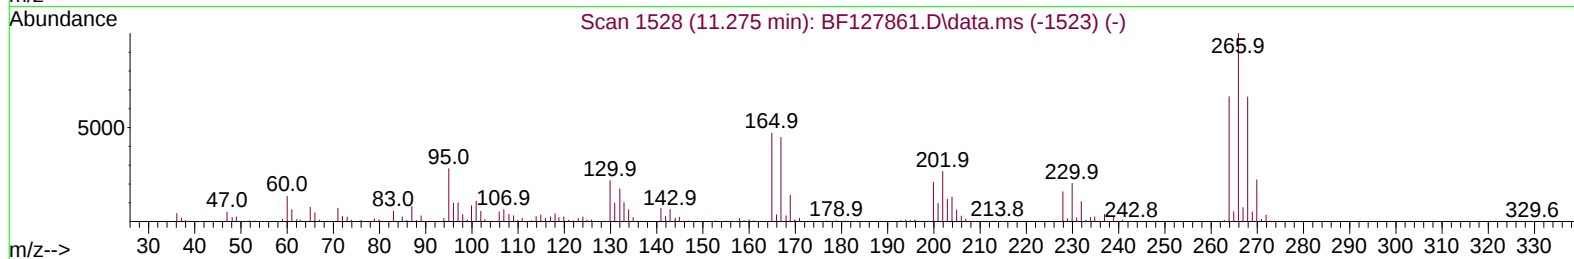
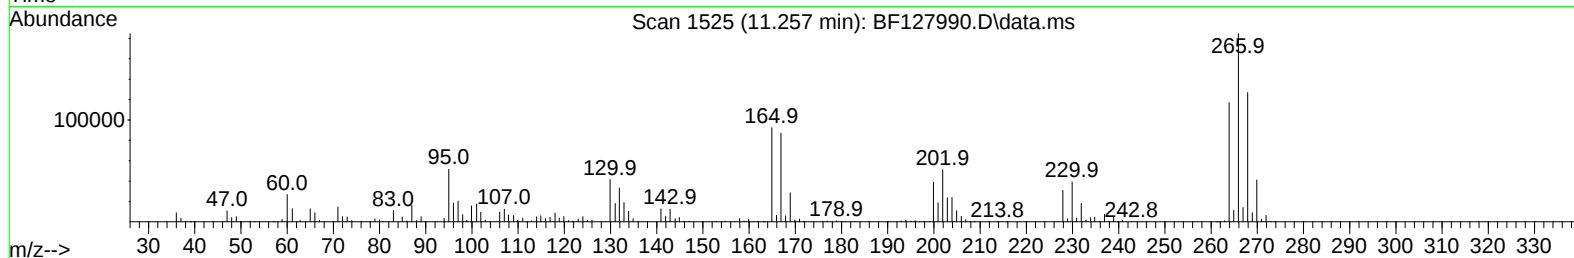


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042922\
Data File : BF127990.D
Acq On : 29 Apr 2022 12:43
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 29 17:53:38 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 28 05:13:03 2022
Response via : Initial Calibration

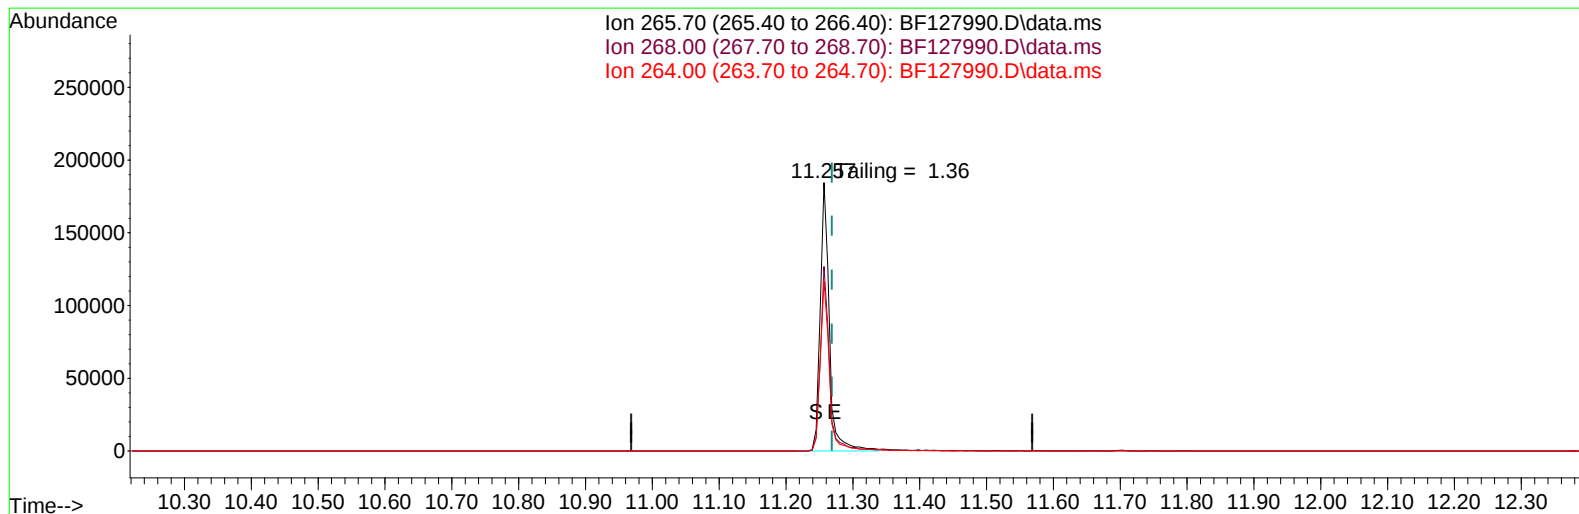

TIC: BF127990.D\data.ms

(70) Pentachlorophenol (C)




11.257min (-0.012) 44411.69 ng

response 177908

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.30	68.74
264.00	66.40	63.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042922\
 Data File : BF127990.D
 Acq On : 29 Apr 2022 12:43
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 29 17:53:38 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 28 05:13:03 2022
 Response via : Initial Calibration

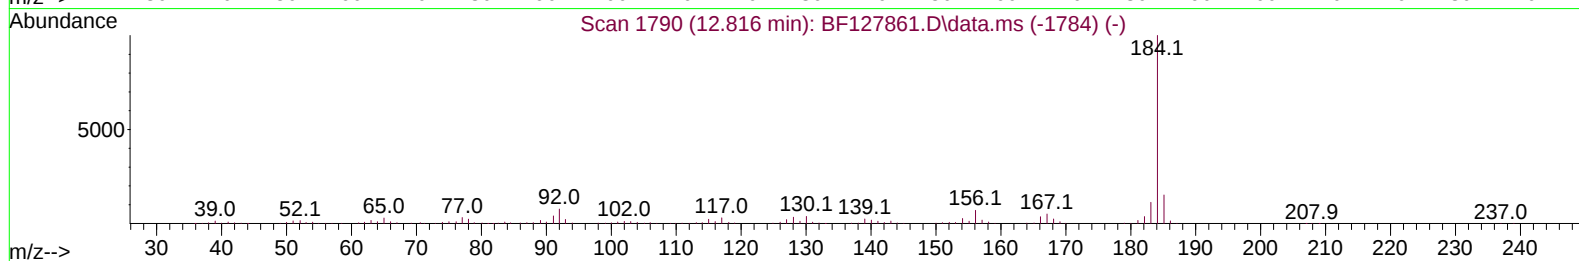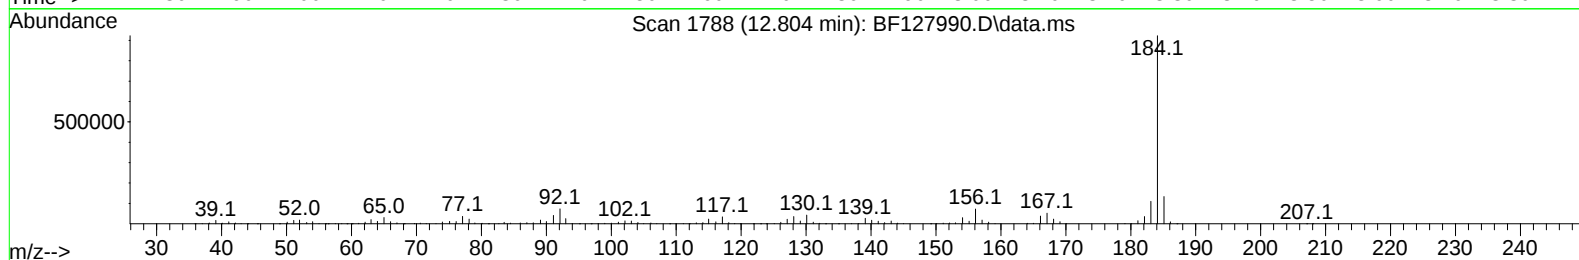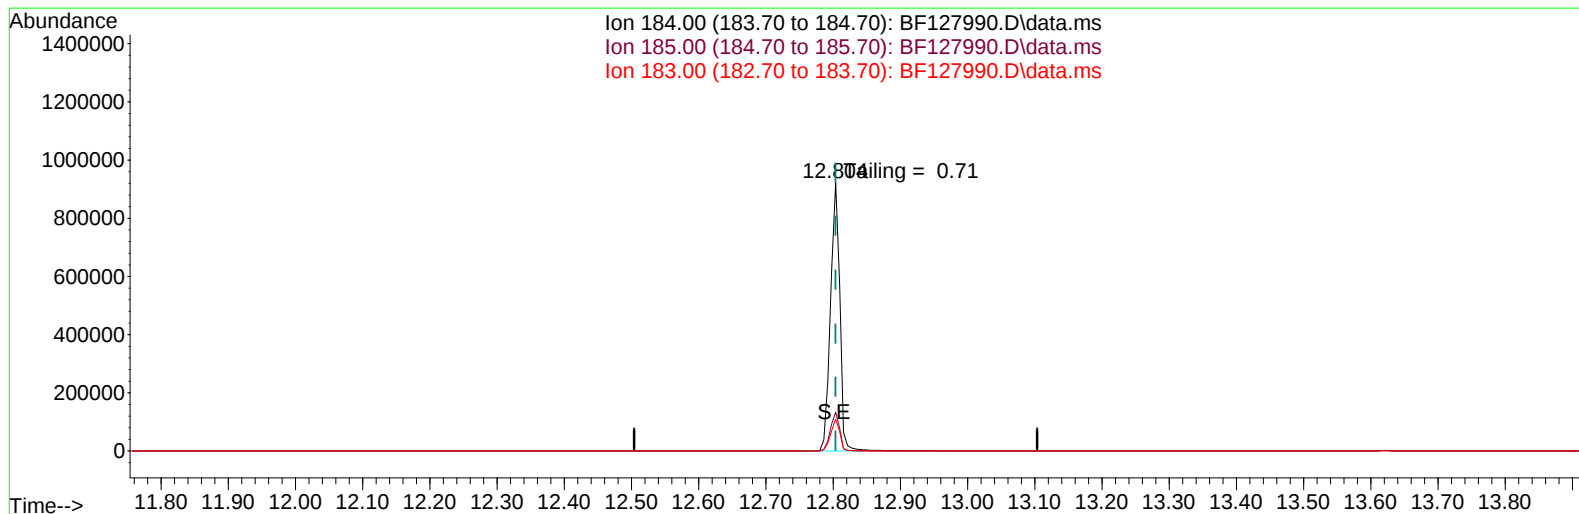

TIC: BF127990.D\data.ms

(77) Benzidine**12.804min (-0.000) 7583.47 ng****response 891505**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.48
183.00	11.20	11.93
0.00	0.00	0.00