

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042922\
 Data File : BF128011.D
 Acq On : 29 Apr 2022 22:58
 Operator : CG\JU
 Sample : N2605-05 2X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TR-06-042822

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128011.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.028	291	296	303	rVB	16053	19473	1.61%	0.176%
2	5.146	483	486	493	rVB	20564	22329	1.85%	0.202%
3	5.540	549	553	563	rVB	1165494	1153423	95.51%	10.425%
4	6.545	720	724	738	rBV	1201497	1168502	96.76%	10.562%
5	6.928	785	789	792	rBV	929729	737611	61.08%	6.667%
6	7.487	880	884	887	rBV	881211	727036	60.20%	6.571%
7	8.210	1003	1007	1010	rBV	1091566	846532	70.10%	7.652%
8	8.786	1102	1105	1109	rVB	26827	22431	1.86%	0.203%
9	9.286	1186	1190	1193	rBV	1411176	1207663	100.00%	10.916%
10	9.357	1199	1202	1205	rVB2	26909	24179	2.00%	0.219%
11	9.969	1303	1306	1309	rBV	1055609	816219	67.59%	7.378%
12	9.998	1309	1311	1315	rVB	38074	33970	2.81%	0.307%
13	10.175	1337	1341	1344	rVB	18565	17687	1.46%	0.160%
14	10.380	1370	1376	1379	rBV6	9837	16938	1.40%	0.153%
15	10.516	1396	1399	1405	rVB	34245	31372	2.60%	0.284%
16	10.757	1436	1440	1448	rBV	716281	631117	52.26%	5.704%
17	10.869	1455	1459	1465	rVB7	11292	20096	1.66%	0.182%
18	11.310	1529	1534	1537	rBV5	12371	17662	1.46%	0.160%
19	11.463	1556	1560	1562	rBV	1003162	804551	66.62%	7.272%
20	11.486	1562	1564	1568	rVV	89205	75776	6.27%	0.685%
21	11.539	1570	1573	1575	rVB	39560	36186	3.00%	0.327%
22	11.839	1621	1624	1627	rBV3	20863	17275	1.43%	0.156%
23	11.975	1643	1647	1649	rBV3	39663	47414	3.93%	0.429%
24	12.080	1662	1665	1671	rVB2	35349	40753	3.37%	0.368%
25	12.527	1739	1741	1743	rBV2	42822	39410	3.26%	0.356%
26	12.680	1763	1767	1770	rBV	189008	185174	15.33%	1.674%
27	12.910	1800	1806	1809	rBV	176486	184159	15.25%	1.665%
28	13.045	1826	1829	1833	rBV	1195946	1016287	84.15%	9.186%
29	14.110	2006	2010	2013	rBV	683611	603361	49.96%	5.454%
30	15.627	2264	2268	2276	rVB	364438	498990	41.32%	4.510%




Sum of corrected areas: 11063576

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042922\
Data File : BF128011.D
Acq On : 29 Apr 2022 22:58
Operator : CG\JU
Sample : N2605-05 2X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TR-06-042822

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

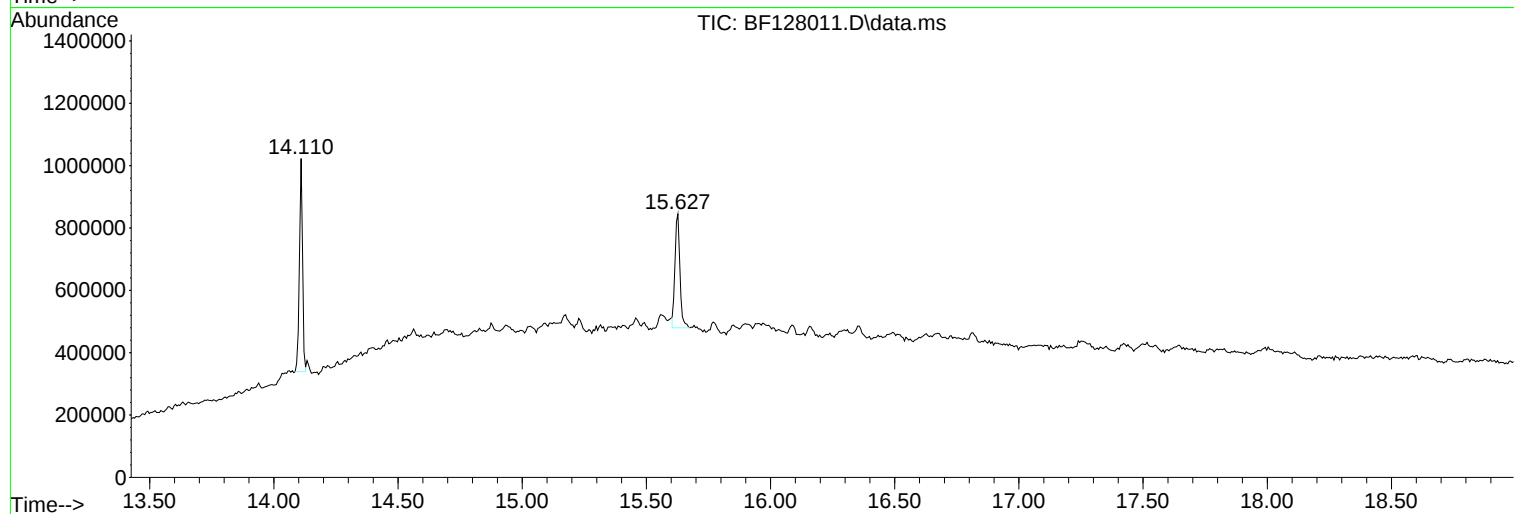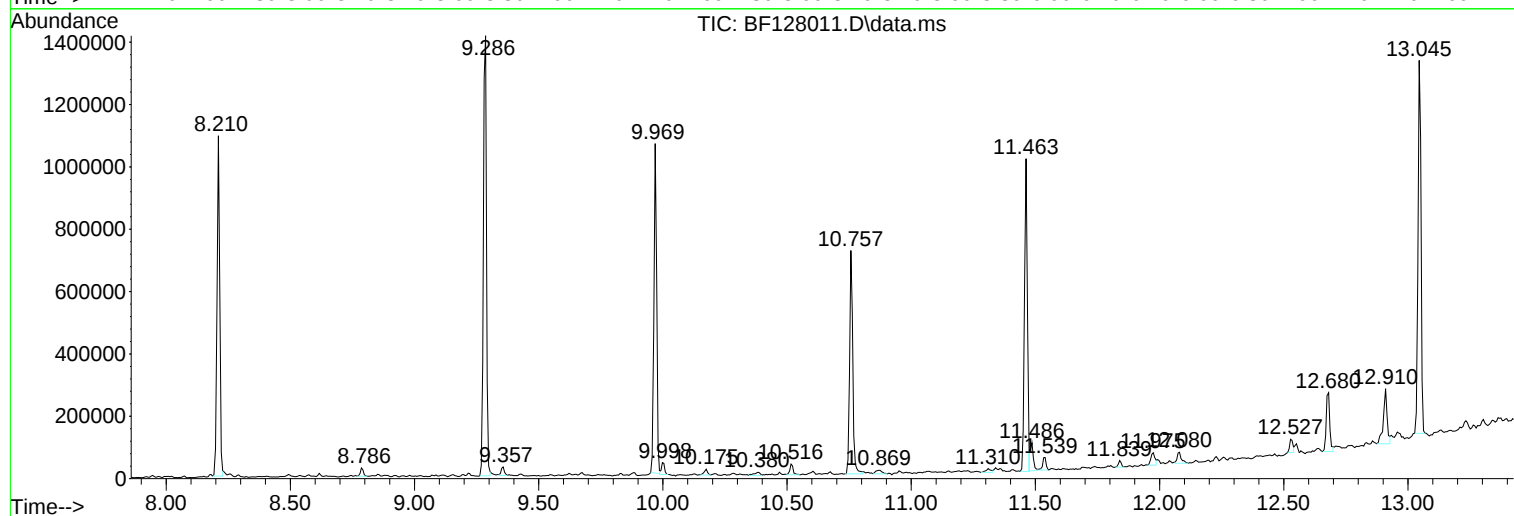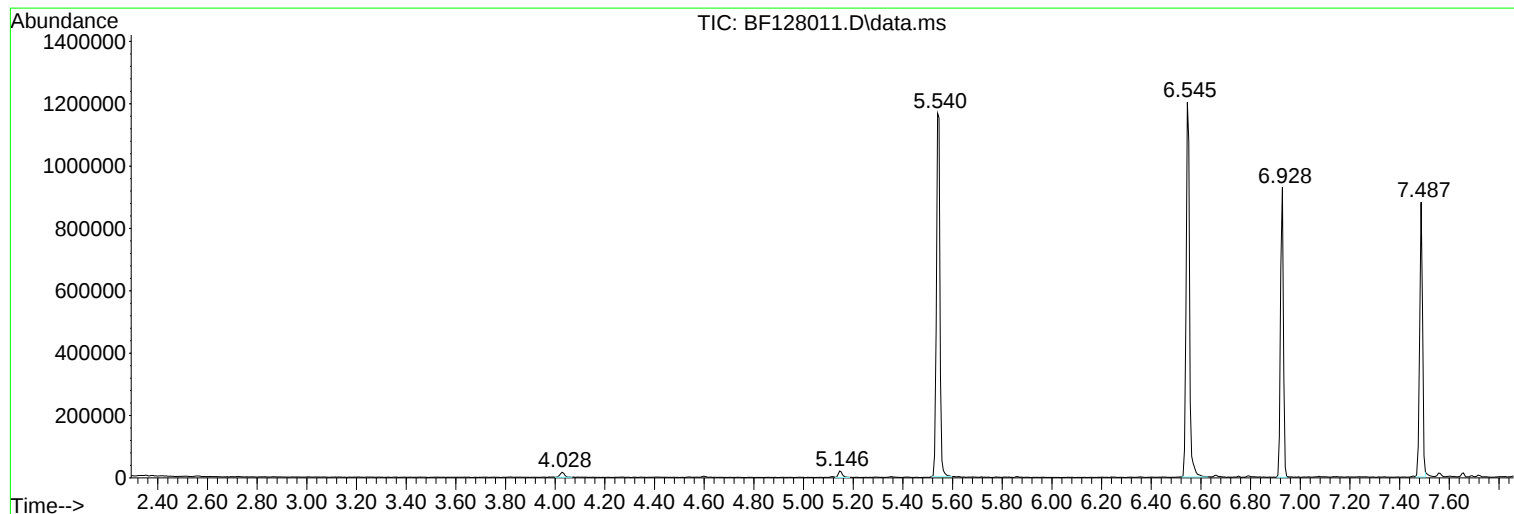

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042922\
Data File : BF128011.D
Acq On : 29 Apr 2022 22:58
Operator : CG\JU
Sample : N2605-05 2X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TR-06-042822

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042922\
Data File : BF128011.D
Acq On : 29 Apr 2022 22:58
Operator : CG\JU
Sample : N2605-05 2X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TR-06-042822

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------