
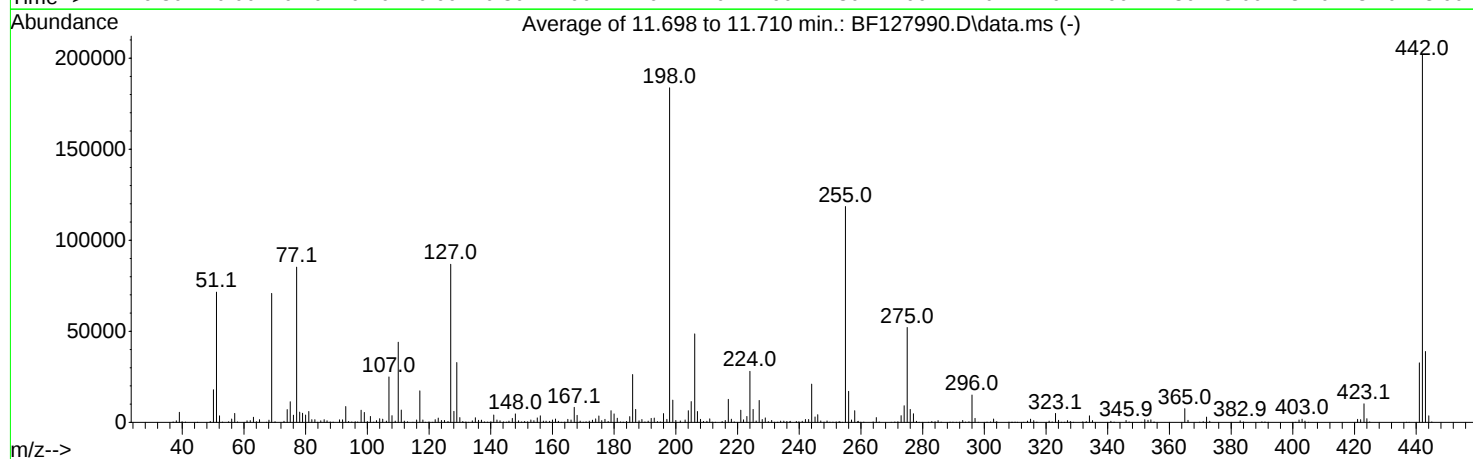


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042922\
 Data File : BF127990.D
 Acq On : 29 Apr 2022 12:43
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 28 05:13:03 2022

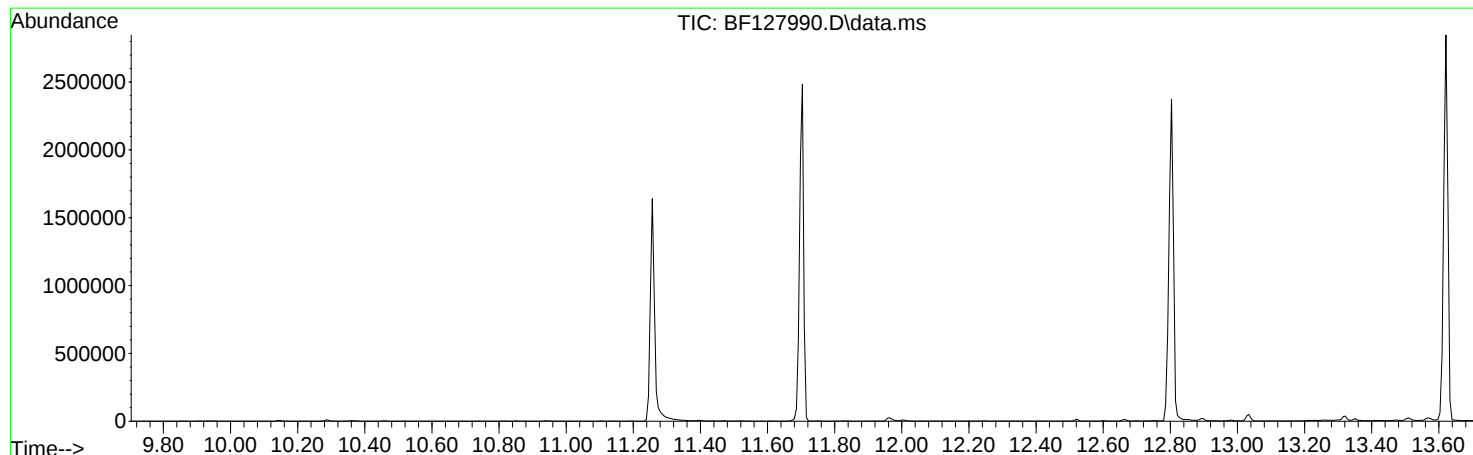

AutoFind: Scans 1600, 1601, 1602; Background Corrected with Scan 1594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.0	71561	PASS
68	69	0.00	2	1.8	1251	PASS
69	198	0.00	100	38.6	70854	PASS
70	69	0.00	2	0.5	353	PASS
127	198	10	80	47.3	86813	PASS
197	198	0.00	2	0.9	1673	PASS
198	198	100	100	100.0	183712	PASS
199	198	5	9	6.7	12243	PASS
275	198	10	60	28.4	52115	PASS
365	198	1	100	4.1	7526	PASS
441	198	0.01	100	17.8	32669	PASS
442	442	50	100	100.0	202005	PASS
443	442	15	24	19.3	38939	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/29/2022	BNA_F	<u>BF127990.D</u>
Compound Name	Response	Retention Time
DDT	474465	13.62
DDD	6231	13.32
DDE	800	12.98
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7031	481496	1.46

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042922\
Data File : BF127990.D
Acq On : 29 Apr 2022 12:43
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 29 17:53:38 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 28 05:13:03 2022
Response via : Initial Calibration

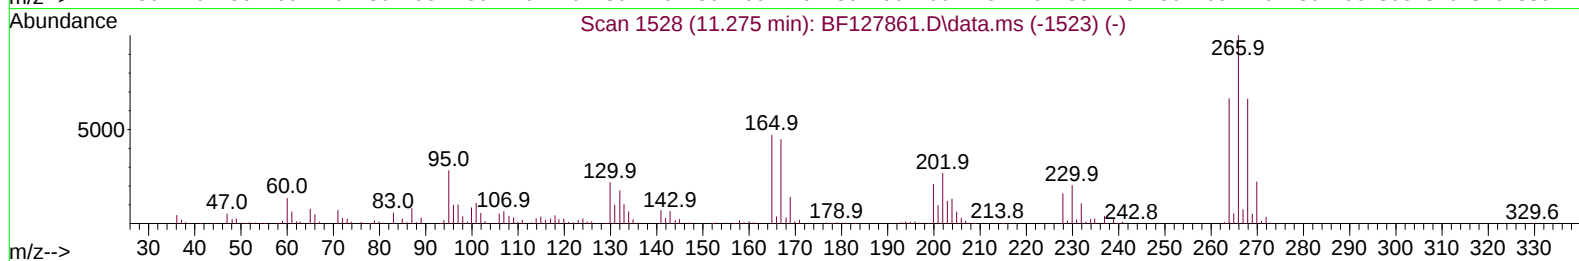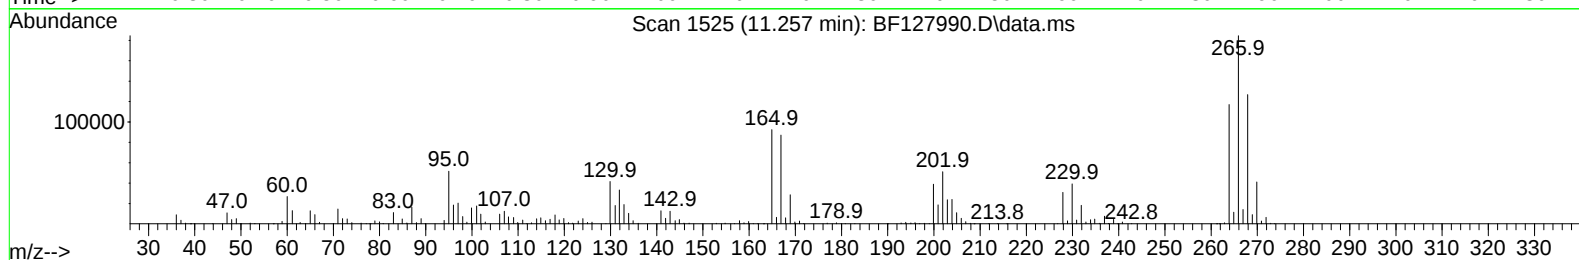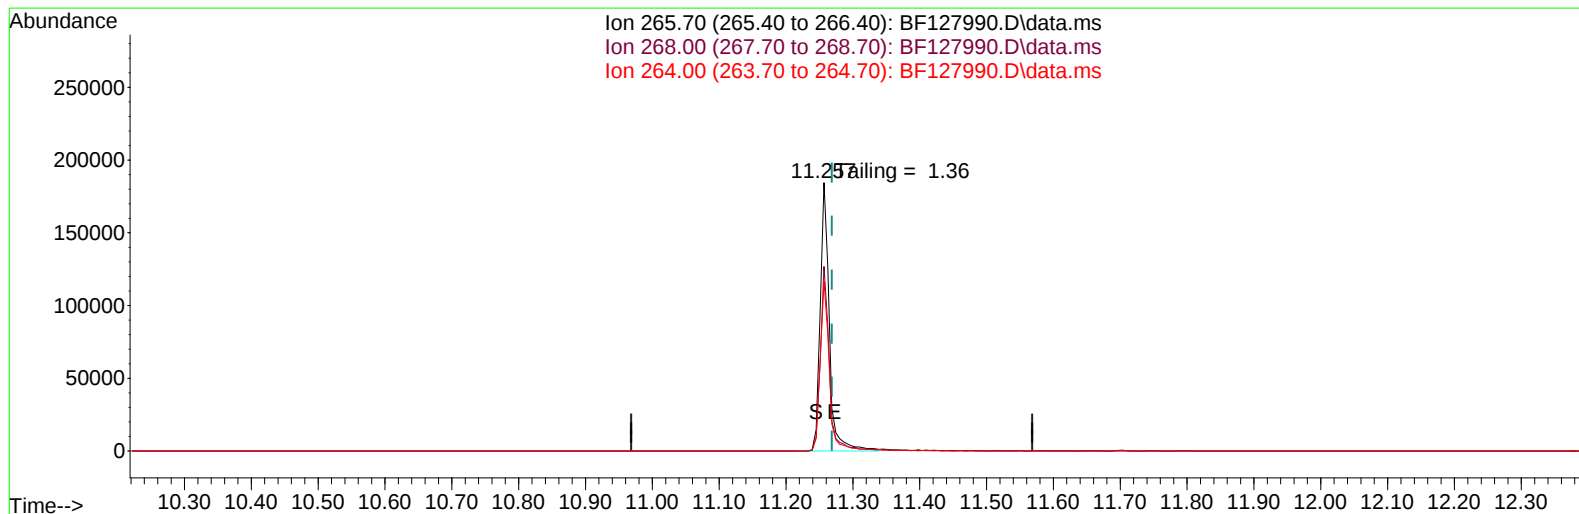

TIC: BF127990.D\data.ms

(70) Pentachlorophenol (C)

11.257min (-0.012) 44411.69 ng




response 177908

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.30	68.74
264.00	66.40	63.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042922\
Data File : BF127990.D
Acq On : 29 Apr 2022 12:43
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 29 17:53:38 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 28 05:13:03 2022
Response via : Initial Calibration

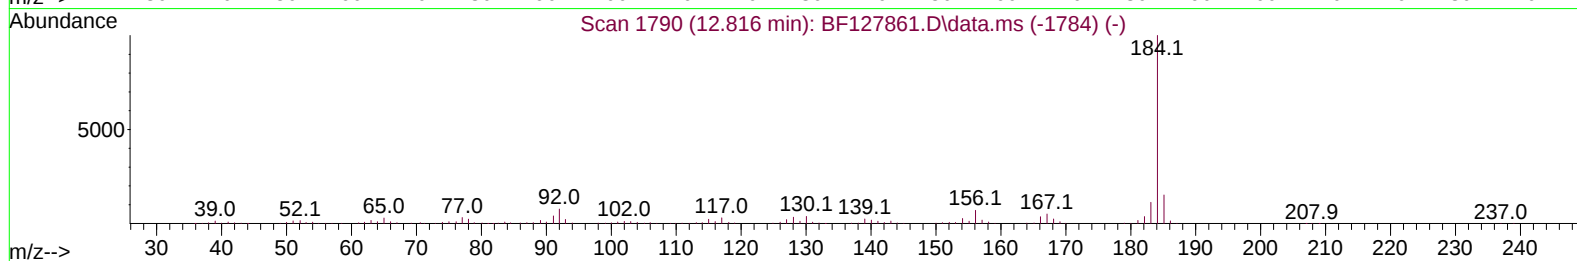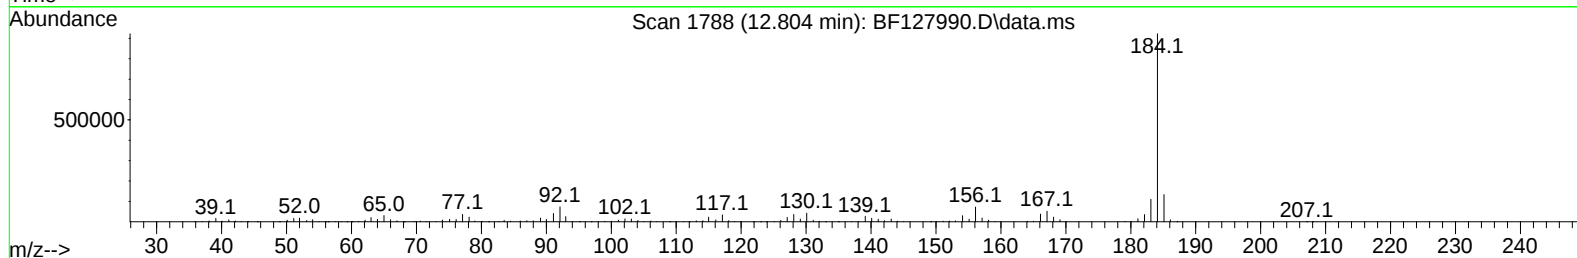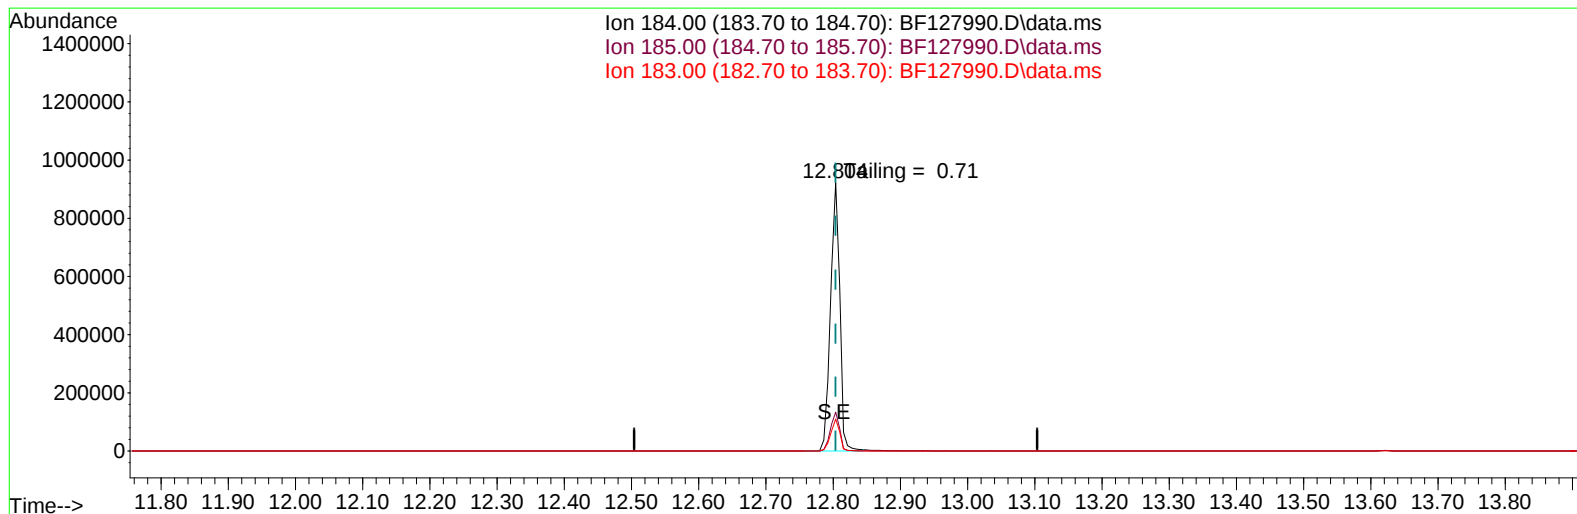

TIC: BF127990.D\data.ms

(77) Benzidine

12.804min (-0.000) 7583.47 ng

response 891505

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.48
183.00	11.20	11.93
0.00	0.00	0.00