


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042924\
Data File : BF137745.D
Acq On : 29 Apr 2024 09:35
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Apr 24 03:57:12 2024

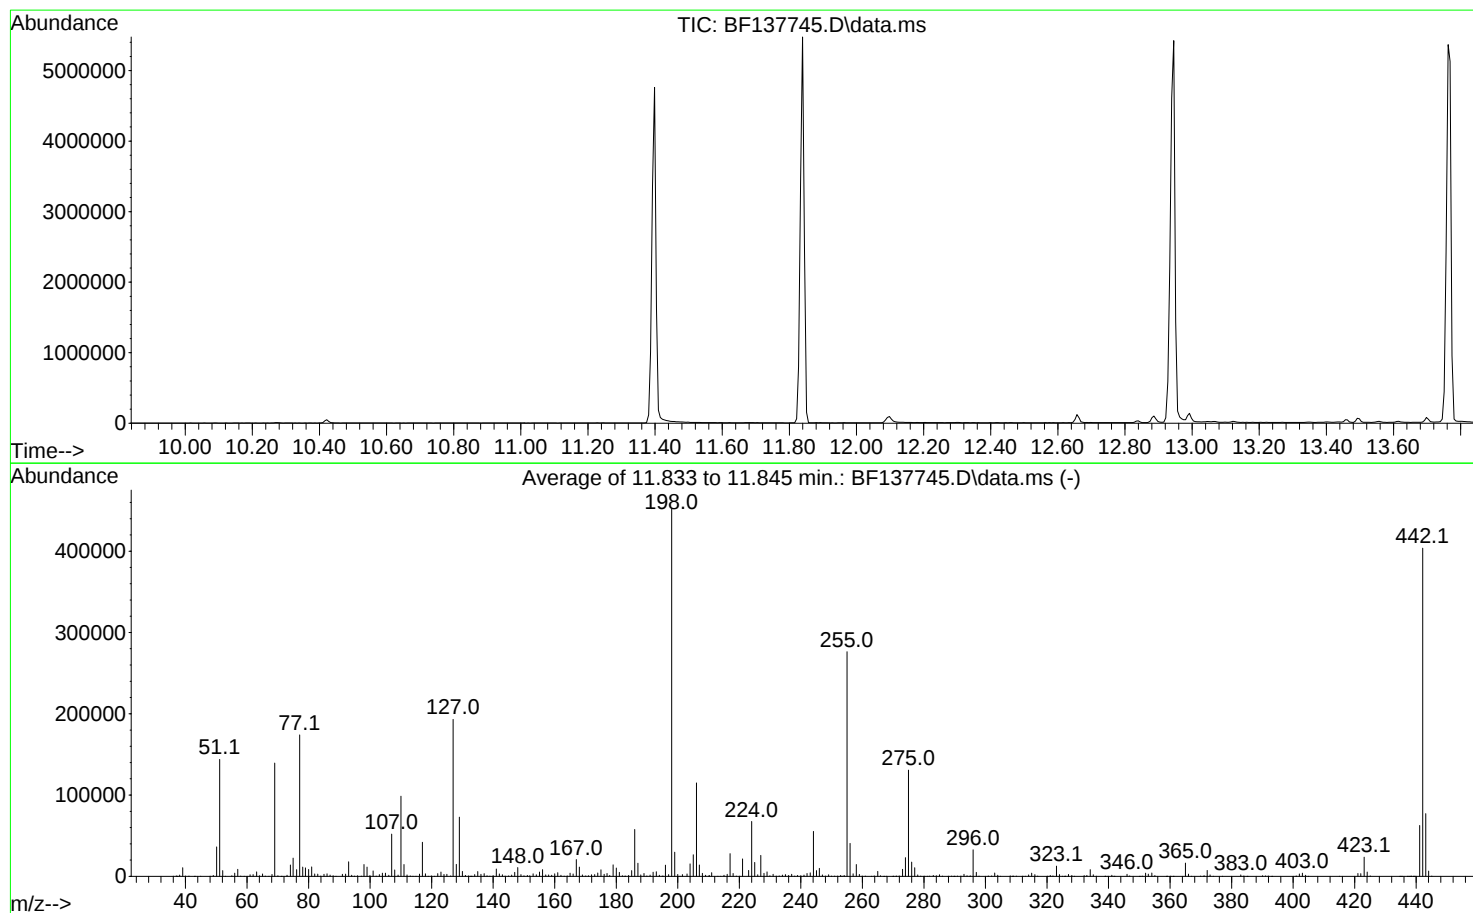




AutoFind: Scans 1657, 1658, 1659; Background Corrected with Scan 1652

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.8	143909	PASS
68	69	0.00	2	1.8	2455	PASS
69	198	0.00	100	30.8	139443	PASS
70	69	0.00	2	0.6	783	PASS
127	198	10	80	42.7	193091	PASS
197	198	0.00	2	0.5	2184	PASS
198	198	100	100	100.0	452523	PASS
199	198	5	9	6.6	29685	PASS
275	198	10	60	28.9	130613	PASS
365	198	1	100	3.6	16333	PASS
441	198	0.01	100	13.8	62552	PASS
442	442	50	100	100.0	403691	PASS
443	442	15	24	19.1	77245	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042924\
Data File : BF137745.D
Acq On : 29 Apr 2024 09:35
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 29 11:50:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 24 03:57:12 2024
Response via : Initial Calibration

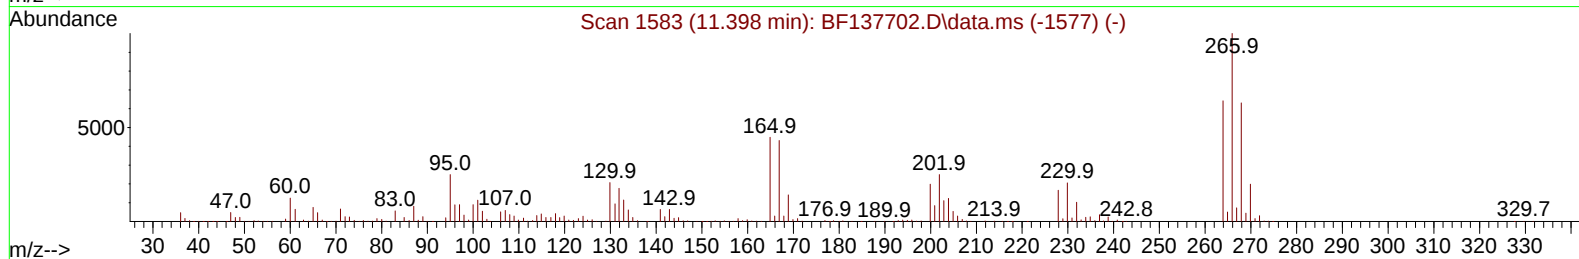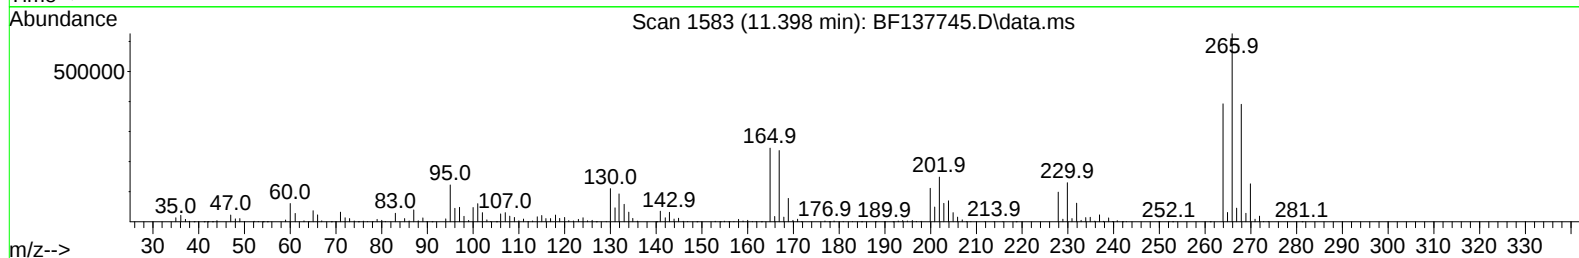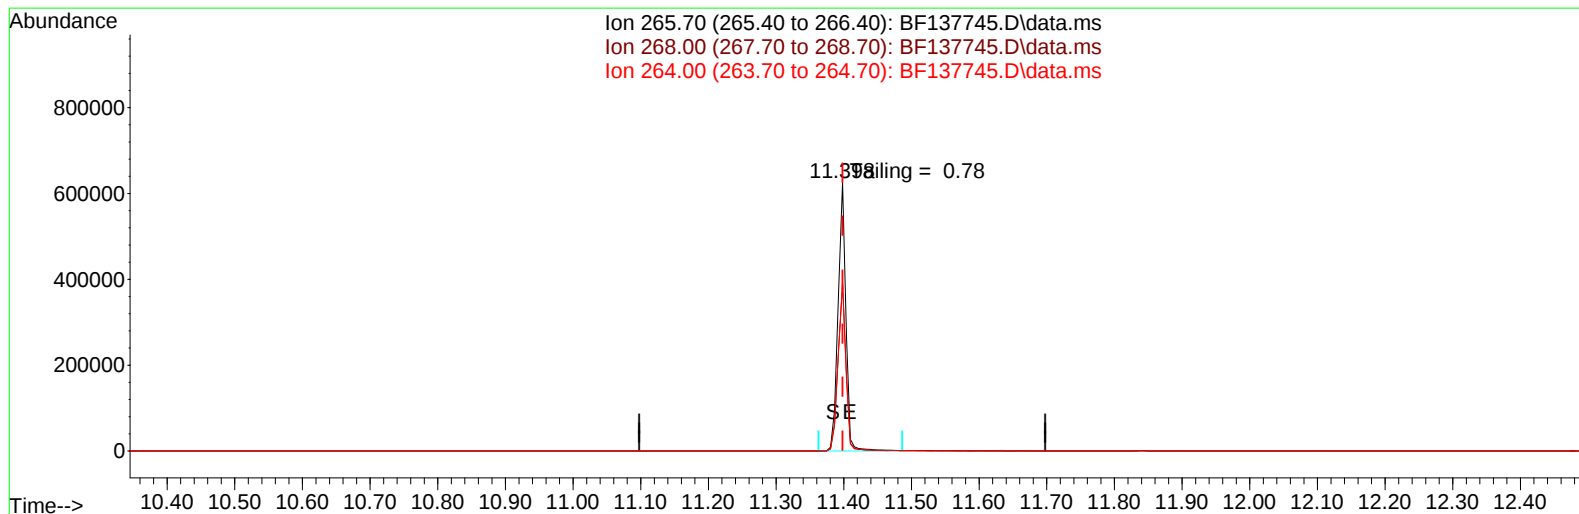

TIC: BF137745.D\data.ms

(70) Pentachlorophenol (C)

11.398min (+ 0.000) 334435.42 ng




response 505508

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	62.52
264.00	64.20	62.74
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042924\  
Data File : BF137745.D  
Acq On    : 29 Apr 2024  09:35  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 29 11:50:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 24 03:57:12 2024
Response via : Initial Calibration

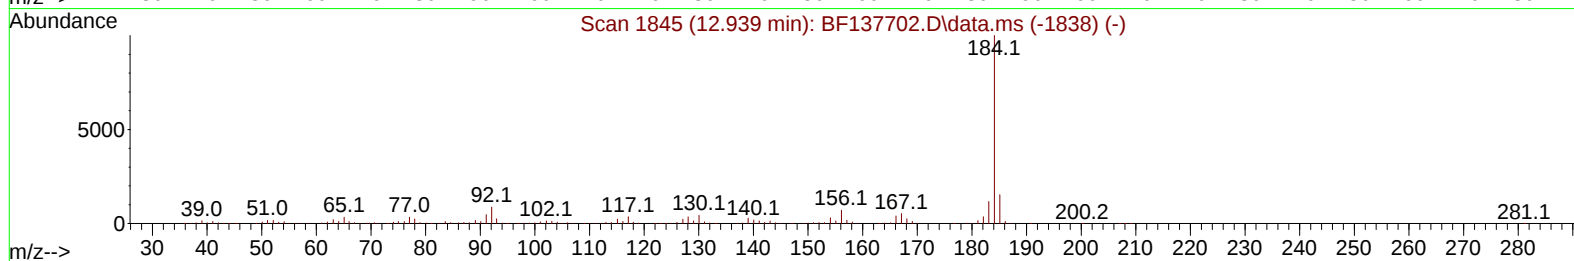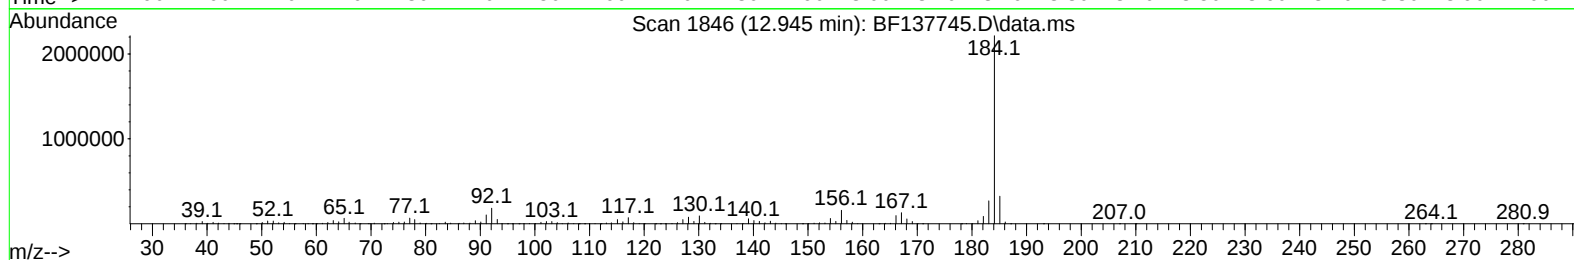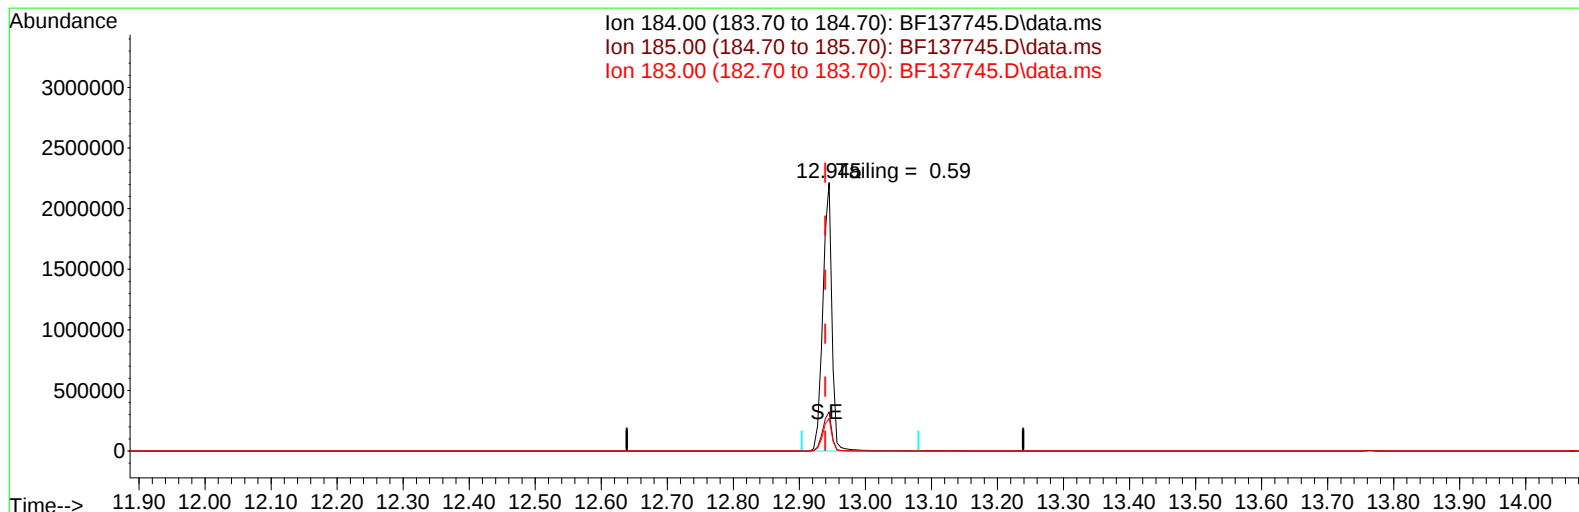

TIC: BF137745.D\data.ms

(77) Benzidine

12.945min (+ 0.006) 436241.71 ng m

response **2109158**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	14.62
183.00	11.70	12.18
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/29/2024	BNA_F	<u>BF137745.D</u>
Compound Name	Response	Retention Time
DDT	1019468	13.769
DDD	14725	13.492
DDE	1692	13.122
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16417	1035885	1.58

Instrument :
BNA_F
ClientSampleId :
DFTPP