
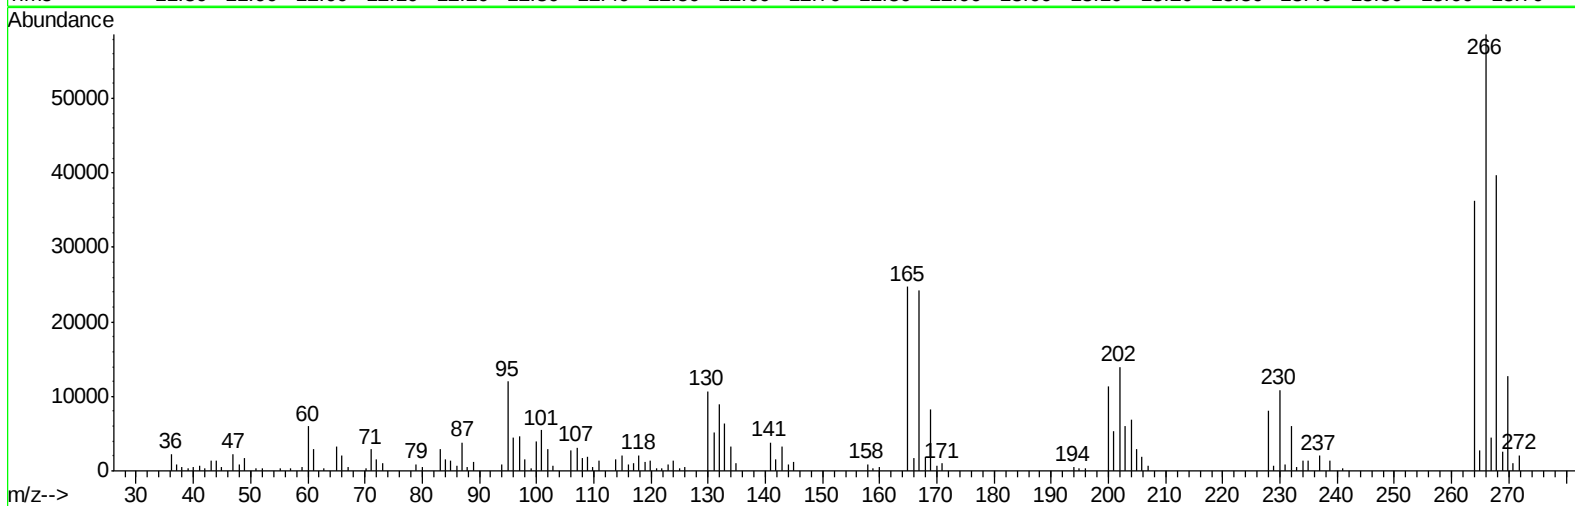


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF043015\
Data File : BF078849.D
Acq On : 30 Apr 2015 13:32
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 01 06:56:30 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 01 00:31:00 2015
Response via : Initial Calibration

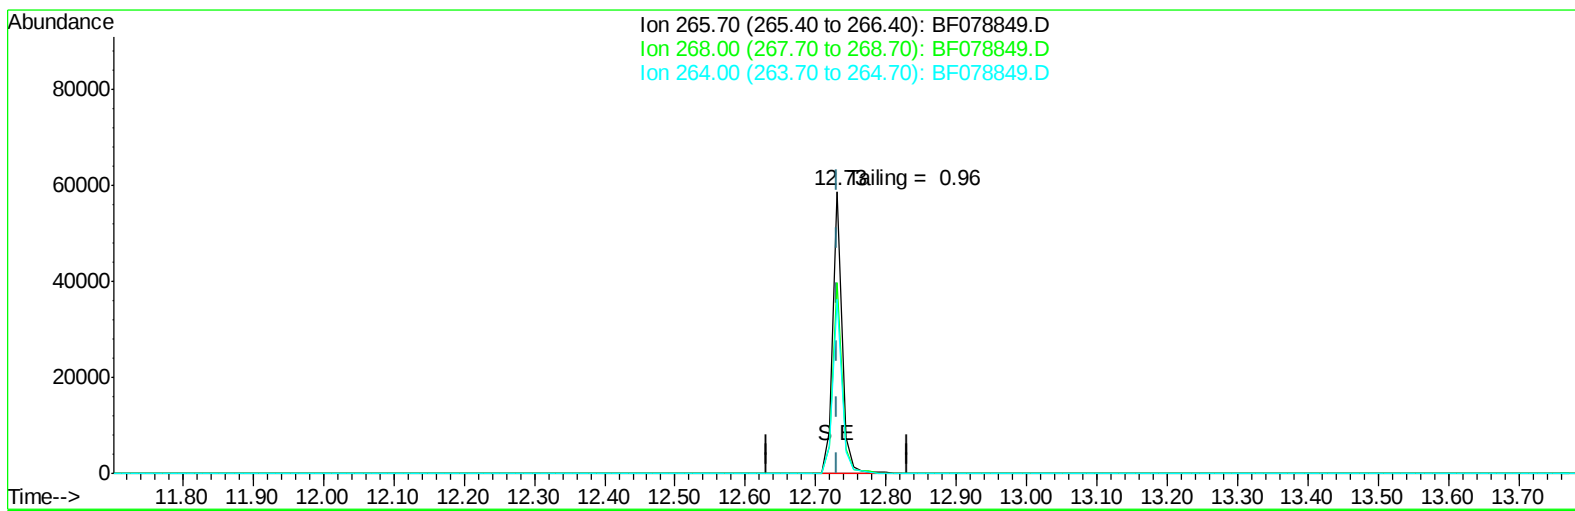

TIC: BF078849.D

(69) Pentachlorophenol (C)



12.731min (-0.000) 31356.15ng

response 53285

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	67.72
264.00	60.20	61.94
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF043015\
Data File : BF078849.D
Acq On : 30 Apr 2015 13:32
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 01 06:56:30 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 01 00:31:00 2015
Response via : Initial Calibration

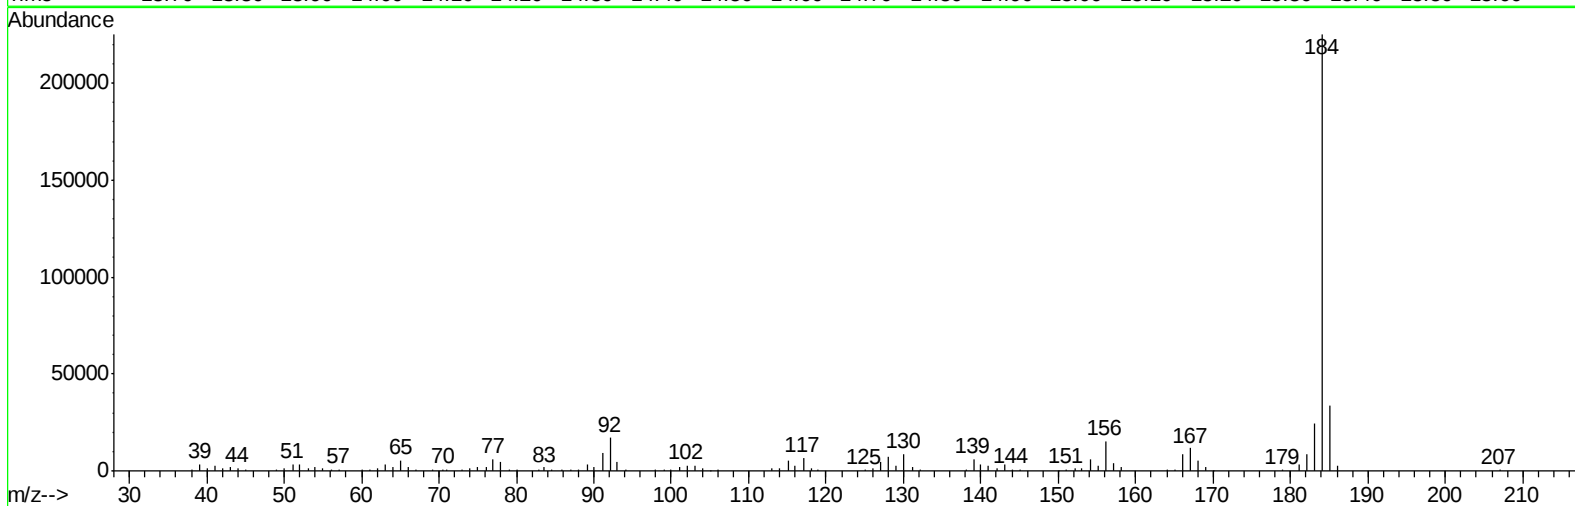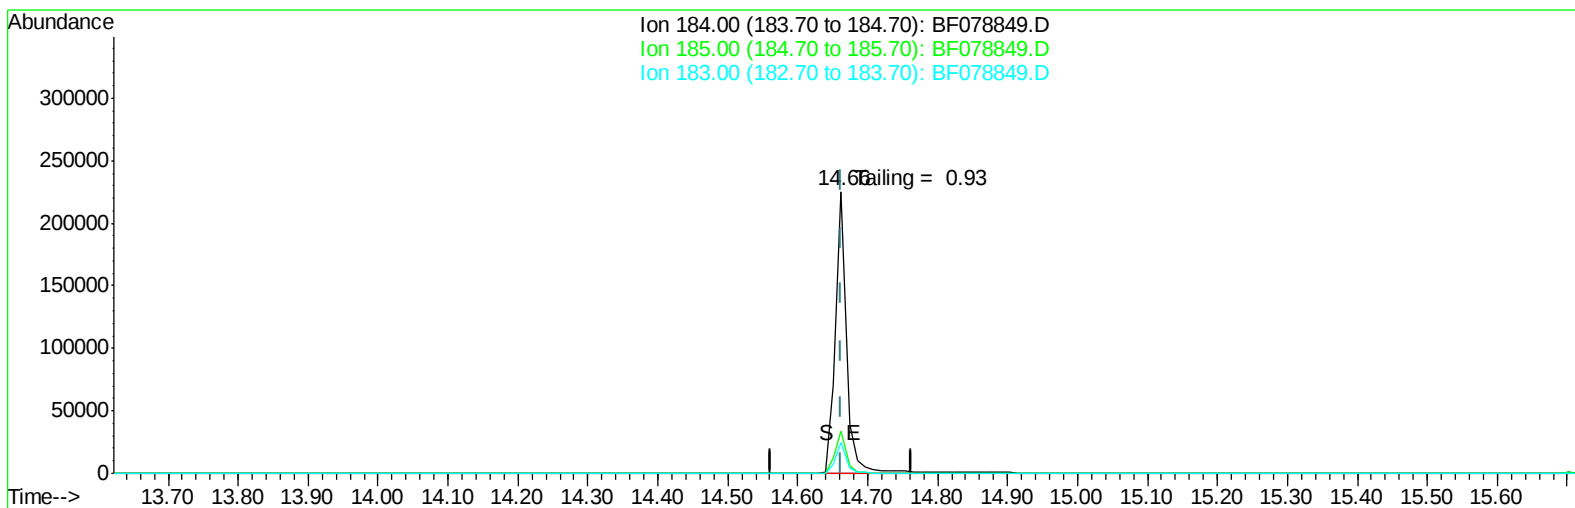

TIC: BF078849.D

(76) Benzidine

14.662min (-0.000) 0.00ng

response 244000

Ion	Exp%	Act%
184.00	100	100
185.00	15.40	14.93
183.00	10.50	10.87
0.00	0.00	0.00