
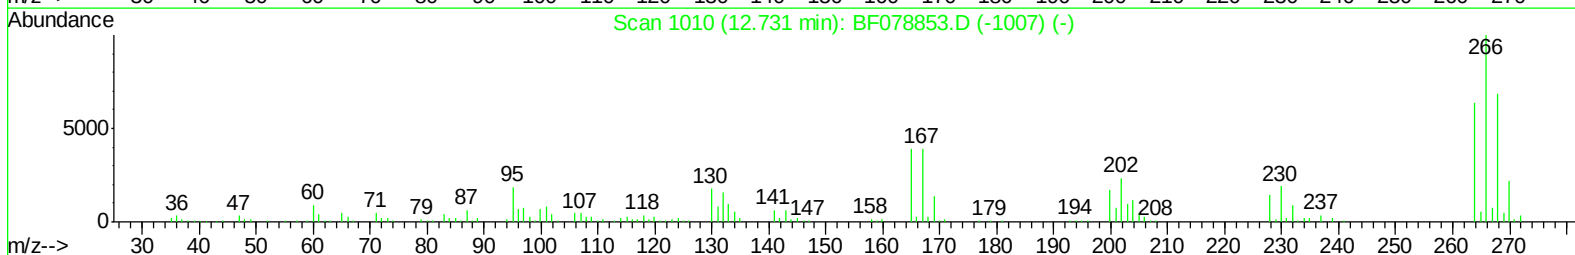
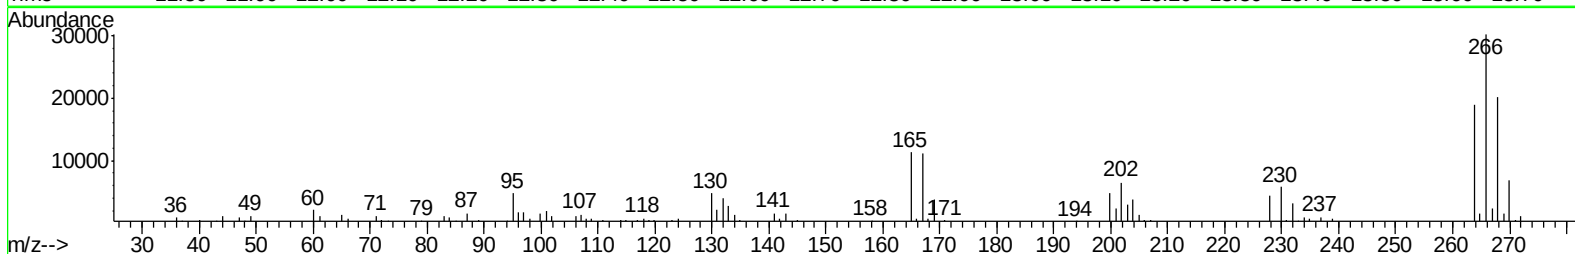


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF043015\
Data File : BF078858.D
Acq On : 30 Apr 2015 19:53
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 01 06:57:23 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 01 00:31:00 2015
Response via : Initial Calibration

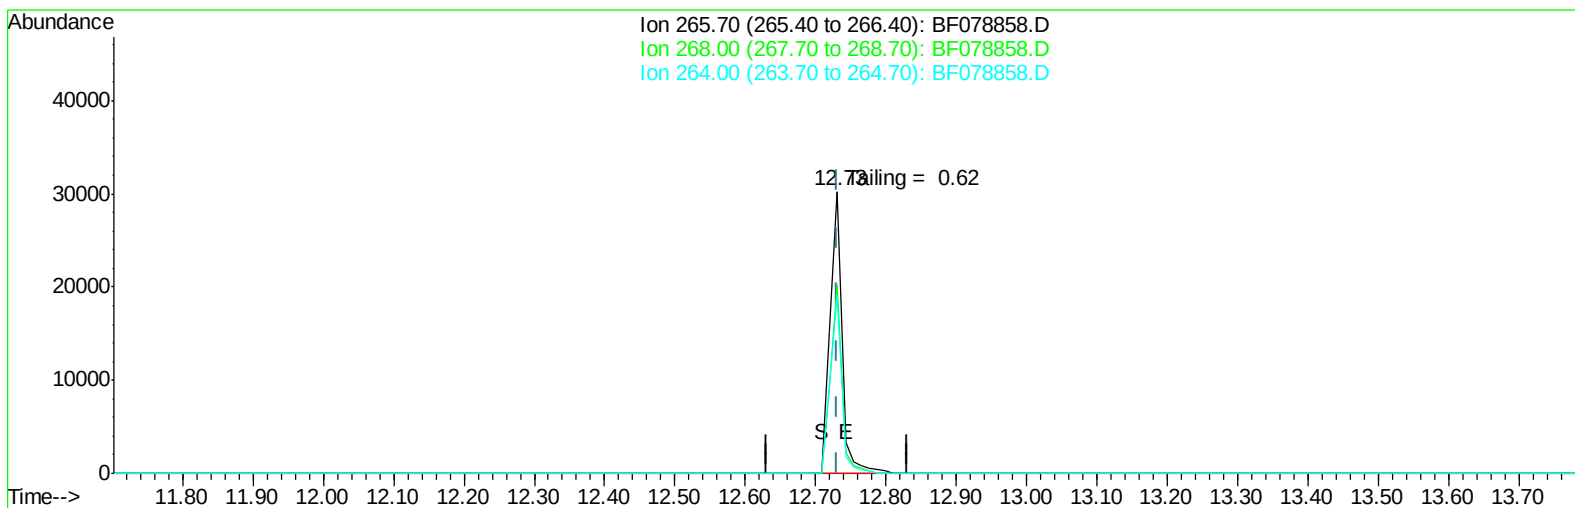

TIC: BF078858.D

(69) Pentachlorophenol (C)




12.731min (-0.000) 0.00ng

response 35494

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	66.98
264.00	60.20	63.01
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF043015\
Data File : BF078858.D
Acq On : 30 Apr 2015 19:53
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 01 06:57:23 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 01 00:31:00 2015
Response via : Initial Calibration

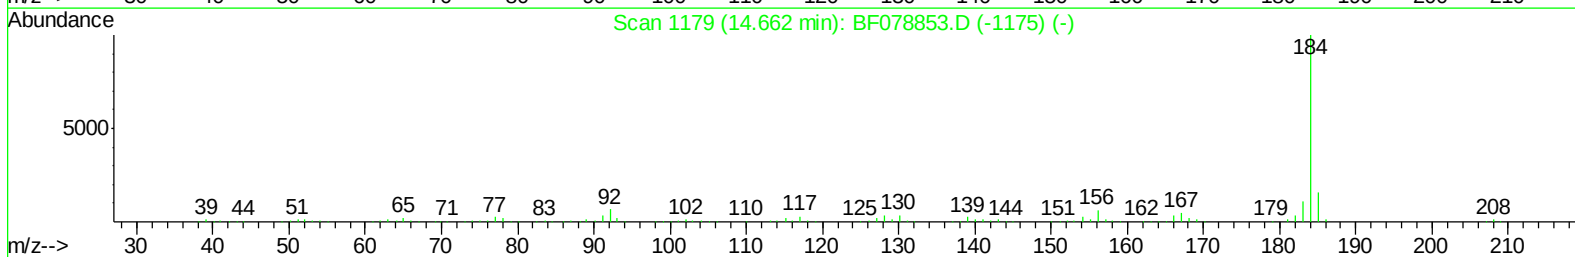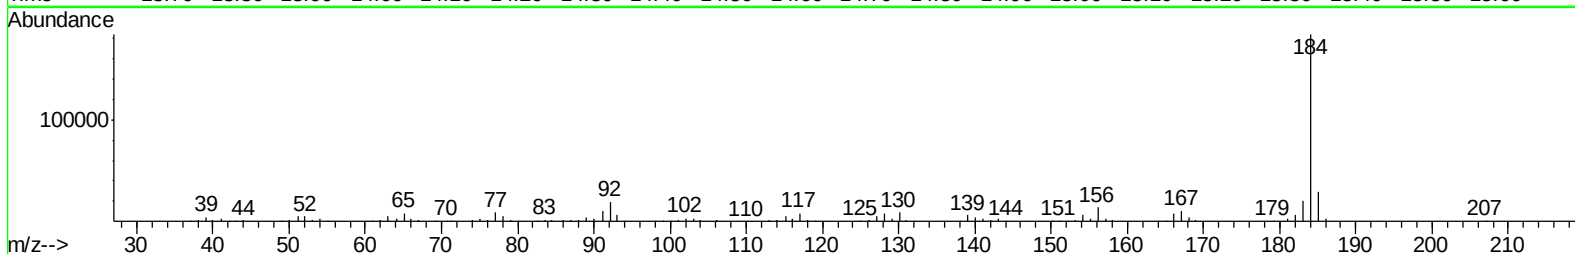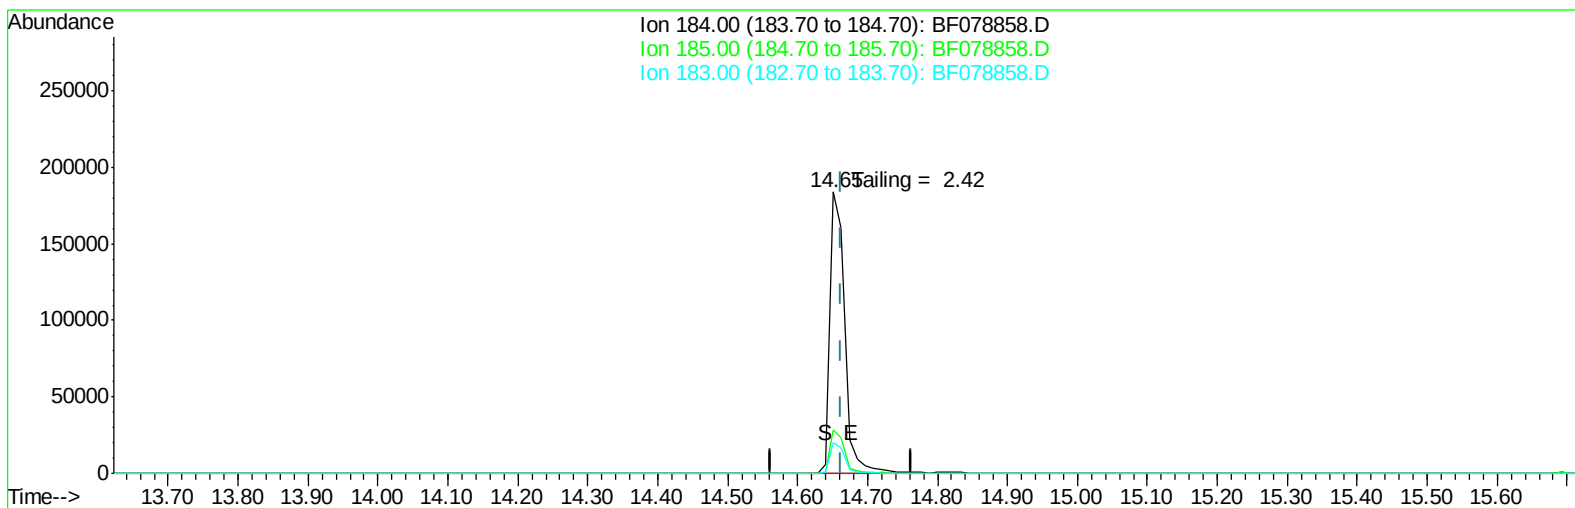

TIC: BF078858.D

(76) Benzidine

14.651min (-0.012) 0.00ng

response 268743

Ion	Exp%	Act%
184.00	100	100
185.00	15.40	15.67
183.00	10.50	11.04
0.00	0.00	0.00