


Data Path : Z:\HPCHEM1\BNA F\DATA\BF043015\
 Data File : BF078849.D
 Acq On : 30 Apr 2015 13:32
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 30 19:07:47 2015

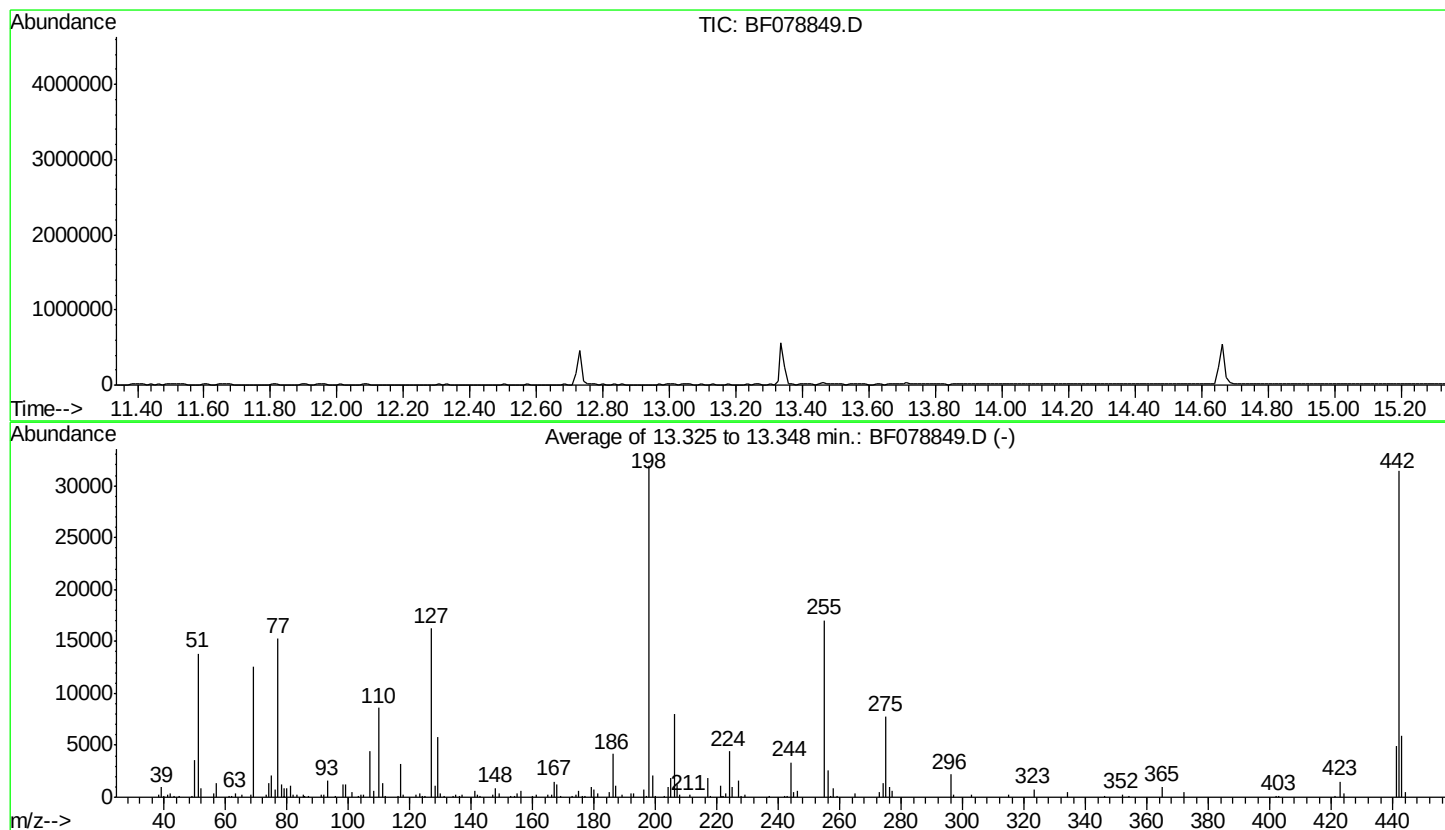

AutoFind: Scans 1062, 1063, 1064; Background Corrected with Scan 1059

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.3	13842	PASS
68	69	0.00	2	2.0	246	PASS
69	198	0.00	100	39.2	12521	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.8	16230	PASS
197	198	0.00	2	0.4	132	PASS
198	198	100	100	100.0	31937	PASS
199	198	5	9	6.6	2116	PASS
275	198	10	60	24.3	7767	PASS
365	198	1	100	3.2	1026	PASS
441	442	0.01	24	15.9	4992	PASS
442	198	50	100	98.3	31392	PASS
443	442	15	24	18.9	5931	PASS