


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF043015\
 Data File : BF078858.D
 Acq On : 30 Apr 2015 19:53
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 30 19:07:47 2015

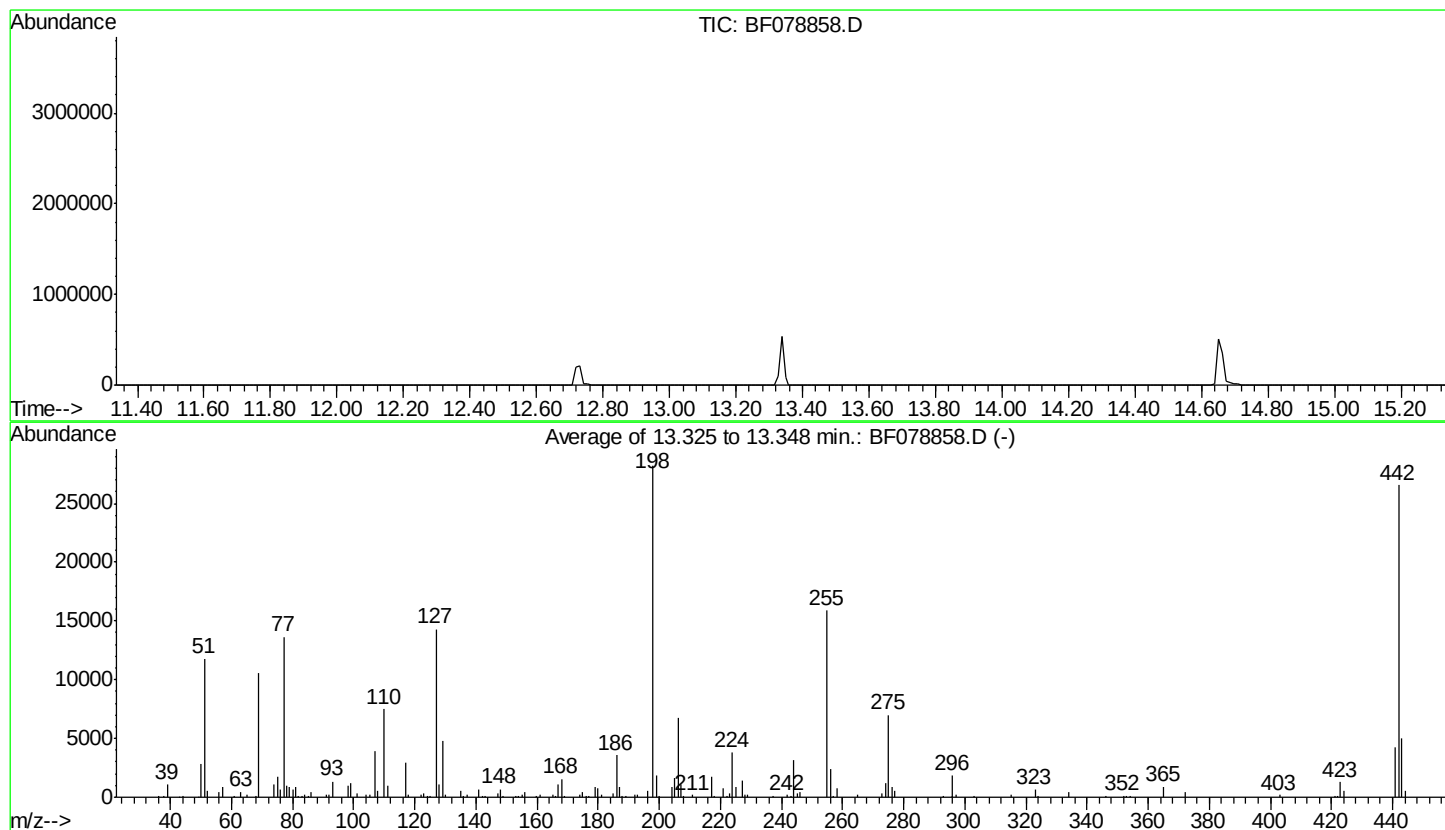

AutoFind: Scans 1062, 1063, 1064; Background Corrected with Scan 1059

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.8	11783	PASS
68	69	0.00	2	1.2	125	PASS
69	198	0.00	100	37.5	10574	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.6	14269	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	28216	PASS
199	198	5	9	6.5	1847	PASS
275	198	10	60	24.8	7010	PASS
365	198	1	100	3.3	922	PASS
441	442	0.01	24	15.9	4208	PASS
442	198	50	100	94.1	26541	PASS
443	442	15	24	18.7	4964	PASS