
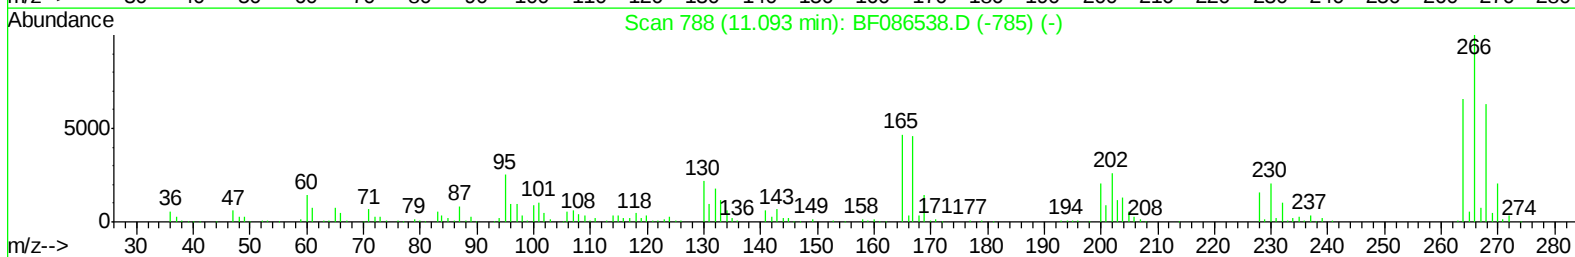
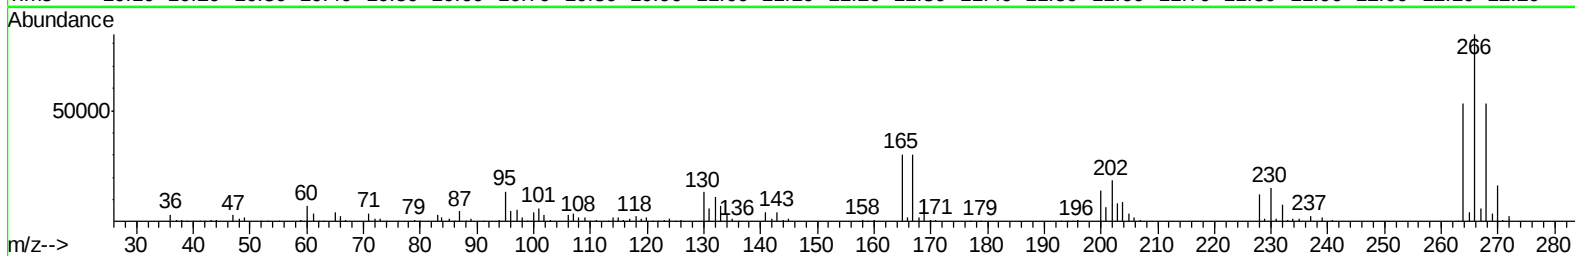


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF043016\
Data File : BF086512.D
Acq On : 30 Apr 2016 9:21
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 02 02:15:34 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 27 14:20:52 2016
Response via : Initial Calibration

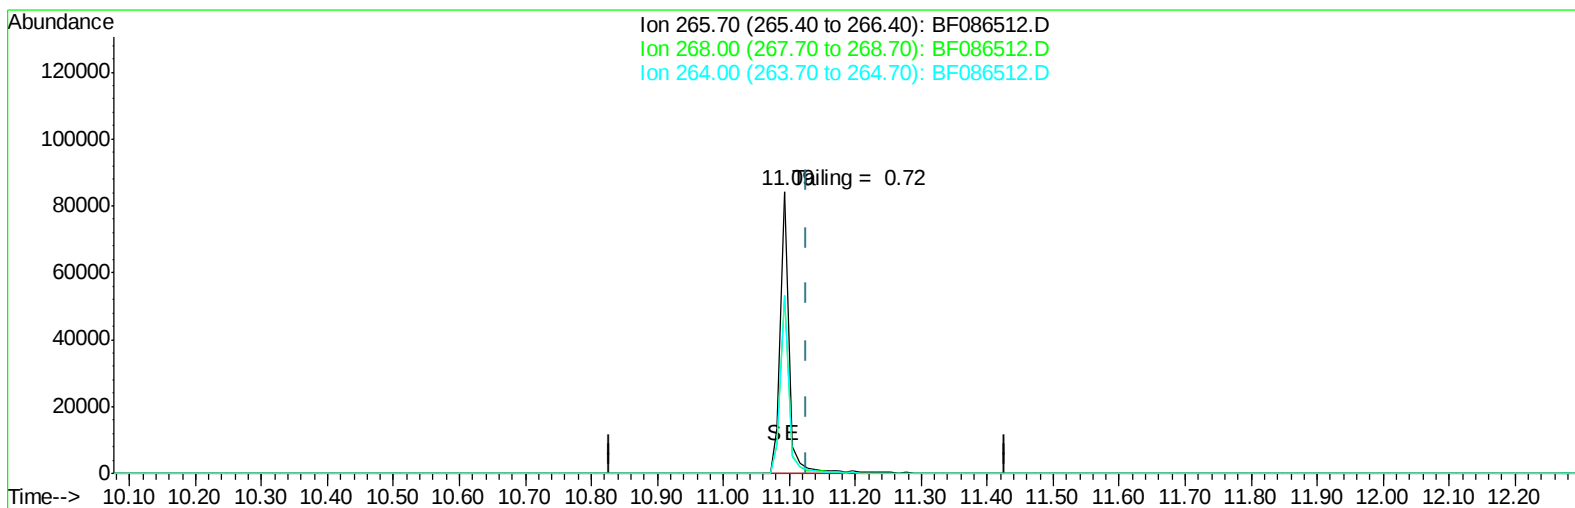

TIC: BF086512.D

(69) Pentachlorophenol (C)




11.094min (-0.034) 35951.17ng

response 80483

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	63.21
264.00	66.10	63.04
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF043016\
 Data File : BF086512.D
 Acq On : 30 Apr 2016 9:21
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 02 02:15:34 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 27 14:20:52 2016
 Response via : Initial Calibration

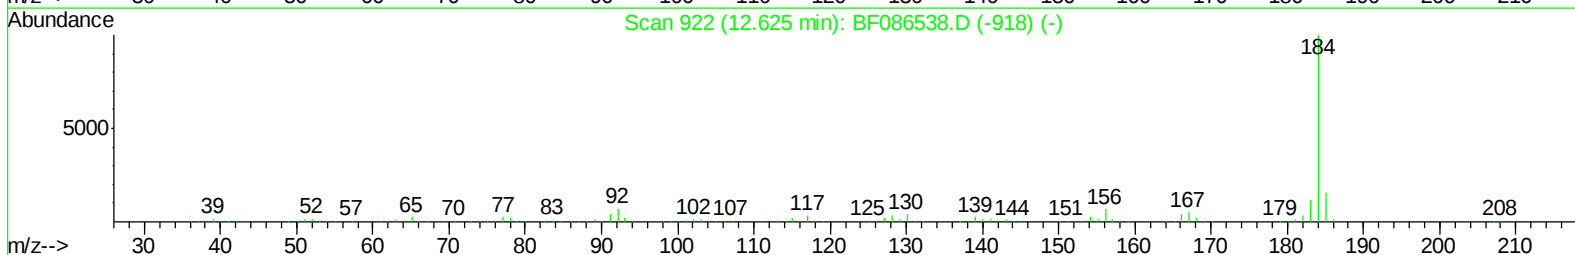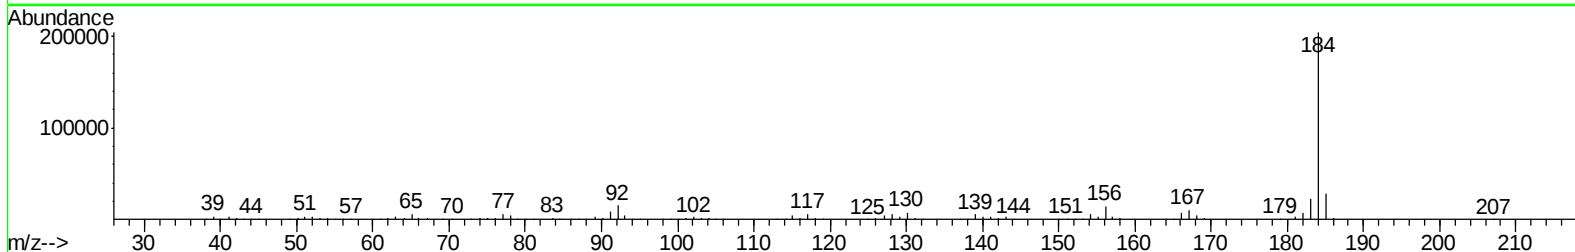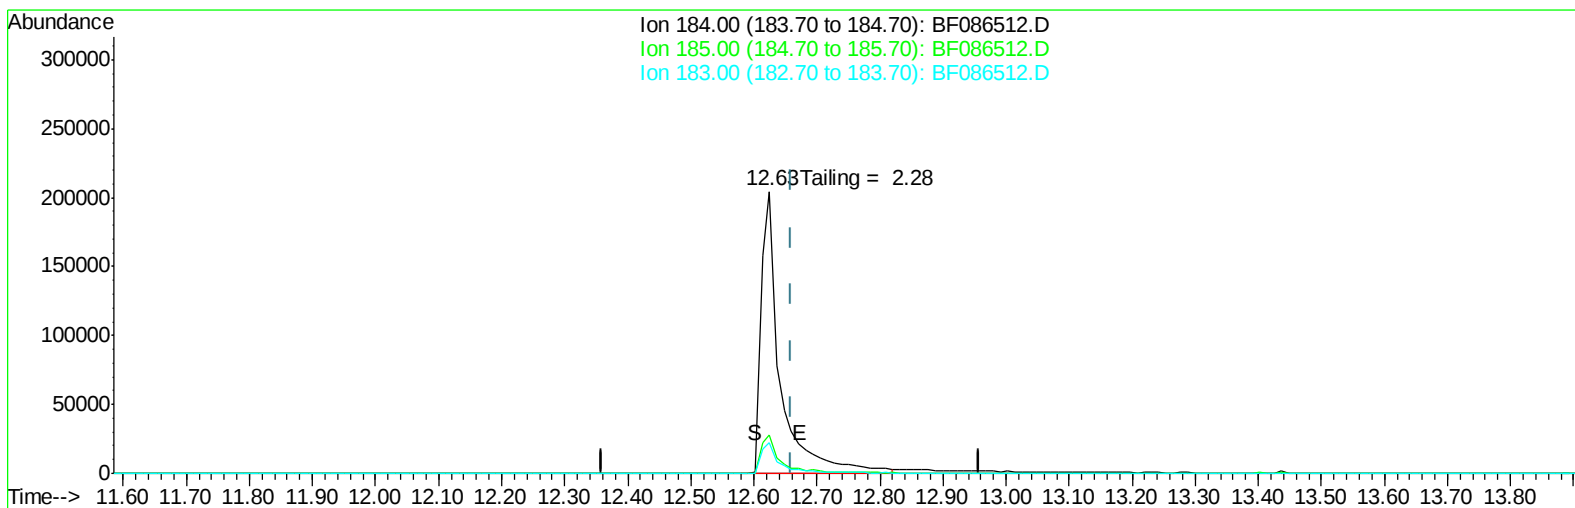

TIC: BF086512.D

(76) Benzidine

12.625min (-0.034) 0.00ng

response 449048

Ion	Exp%	Act%
184.00	100	100
185.00	17.00	13.65
183.00	12.20	11.07
0.00	0.00	0.00