
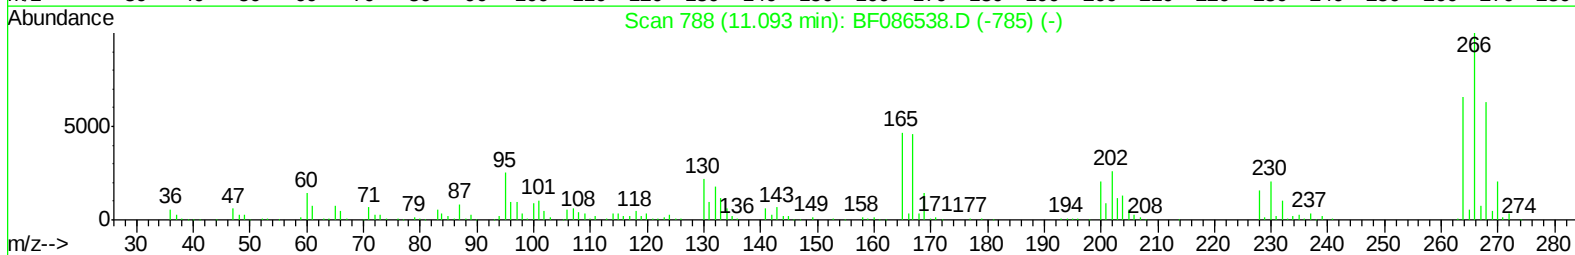
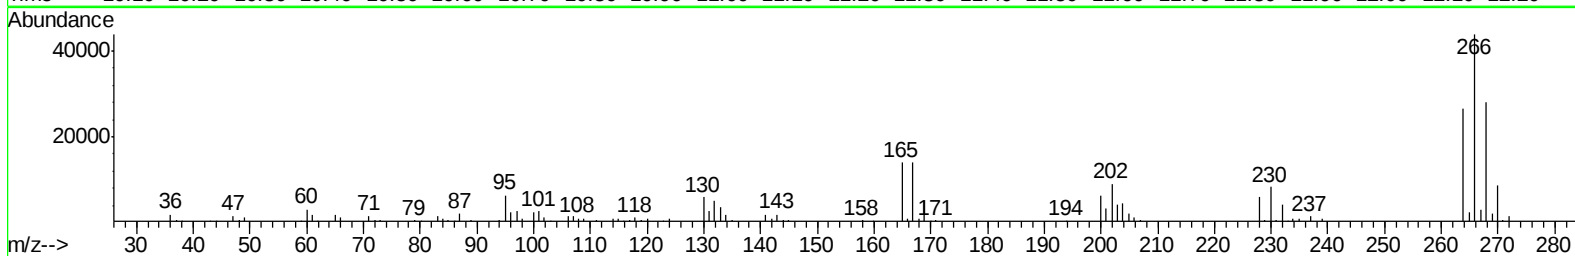


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF043016\
Data File : BF086537.D
Acq On : 30 Apr 2016 21:37
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 02 02:16:27 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 27 14:20:52 2016
Response via : Initial Calibration

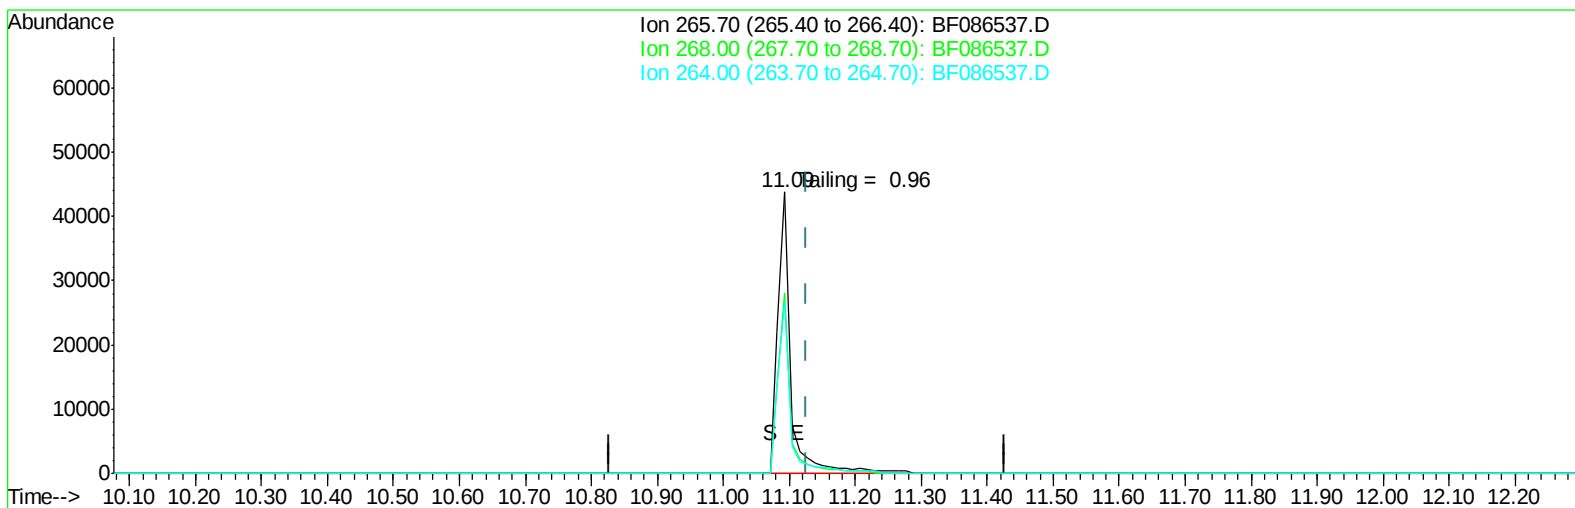

TIC: BF086537.D

(69) Pentachlorophenol (C)




11.093min (-0.034) 25164.08ng

response 60765

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	64.03
264.00	66.10	60.75
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF043016\
Data File : BF086537.D
Acq On : 30 Apr 2016 21:37
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 02 02:16:27 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 27 14:20:52 2016
Response via : Initial Calibration

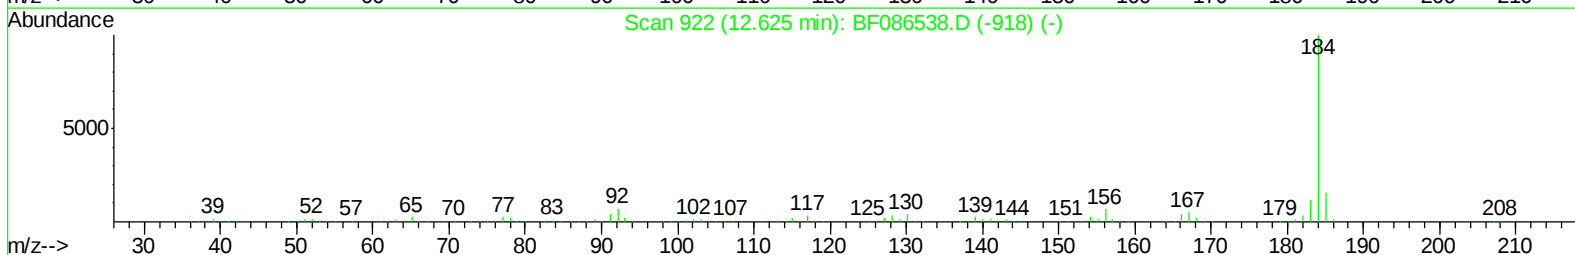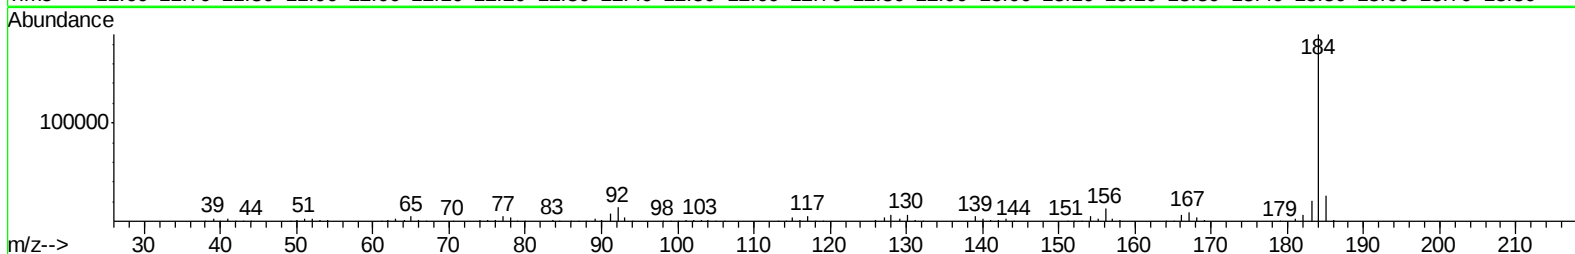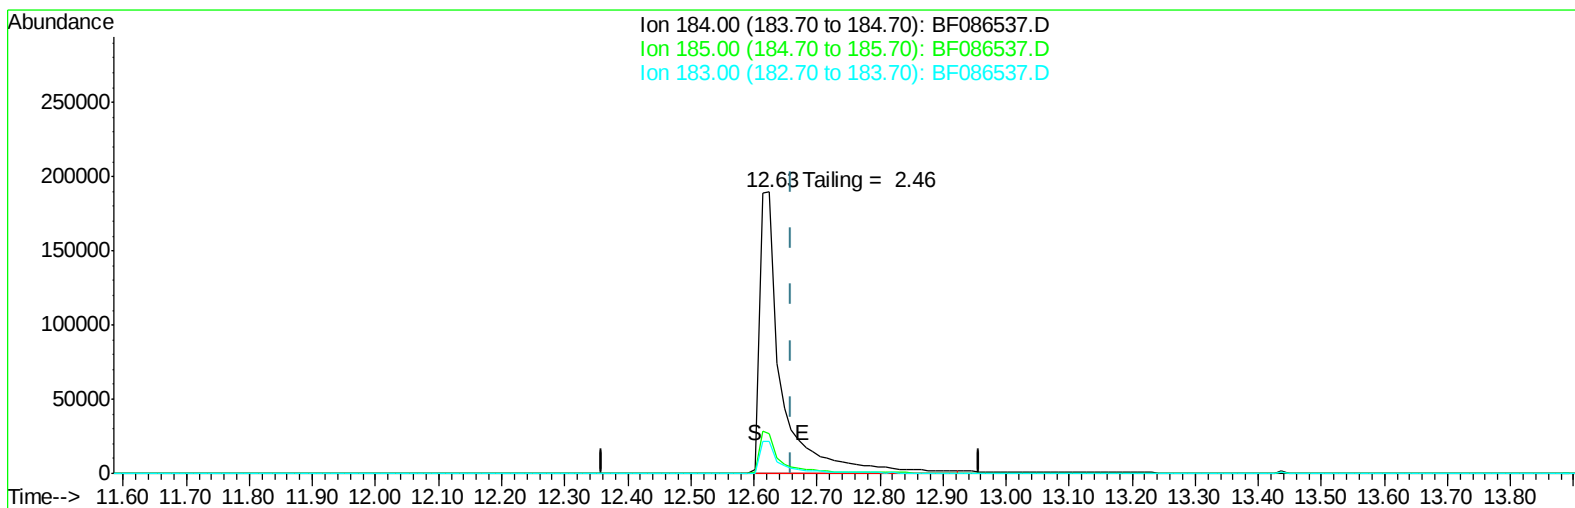

TIC: BF086537.D

(76) Benzidine

12.625min (-0.034) 0.00ng

response 461529

Ion	Exp%	Act%
184.00	100	100
185.00	17.00	14.20
183.00	12.20	11.17
0.00	0.00	0.00