

Data Path : Z:\HPCHEM1\BNA F\DATA\BF043016\
 Data File : BF086553.D
 Acq On : 1 May 2016 6:11
 Operator : UM/SJ
 Sample : H2737-07
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 HW-23-4-26-16

Quant Time: May 02 01:37:06 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF042716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 27 14:20:52 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.76	152	126528	20.00	ng	-0.05
21) Naphthalene-d8	8.05	136	557032	20.00	ng	-0.05
38) Acenaphthene-d10	9.80	164	274986	20.00	ng	-0.05
63) Phenanthrene-d10	11.28	188	483682	20.00	ng	-0.05
75) Chrysene-d12	13.91	240	340257	20.00	ng	-0.06
86) Perylene-d12	15.30	264	290388	20.00	ng	-0.06
System Monitoring Compounds						
5) 2-Fluorophenol	5.34	112	373479	50.91	ng	-0.04
7) Phenol-d6	6.40	99	345576	33.75	ng	-0.05
23) Nitrobenzene-d5	7.33	82	903942	87.47	ng	-0.05
41) 2,4,6-Tribromophenol	10.59	330	351931	121.36	ng	-0.05
44) 2-Fluorobiphenyl	9.13	172	1345652	85.82	ng	-0.05
78) Terphenyl-d14	12.86	244	1302968	84.37	ng	-0.05


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF043016\
Data File : BF086553.D
Acq On : 1 May 2016 6:11
Operator : UM/SJ
Sample : H2737-07
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HW-23-4-26-16

Quant Time: May 02 01:37:06 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF042716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 27 14:20:52 2016
Response via : Initial Calibration

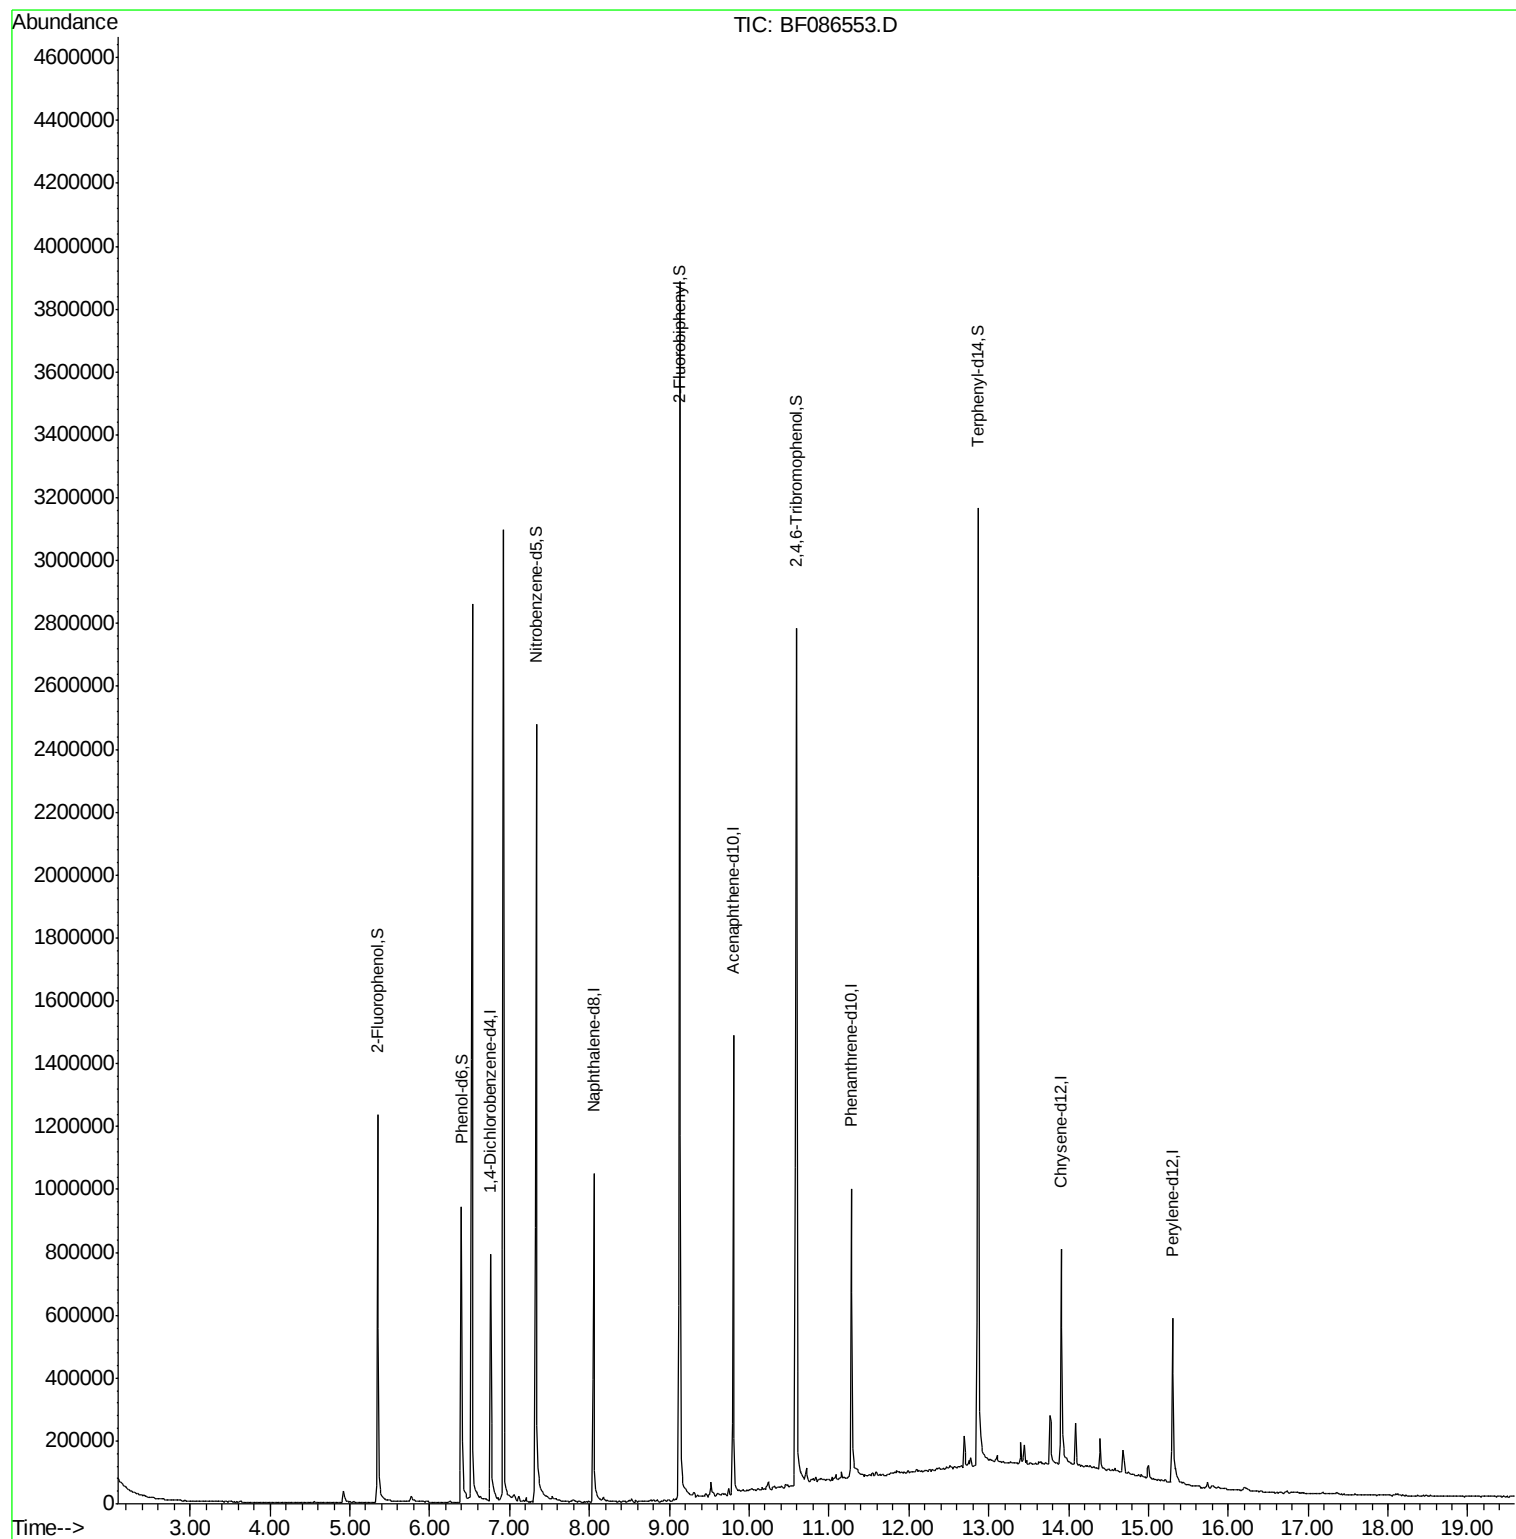

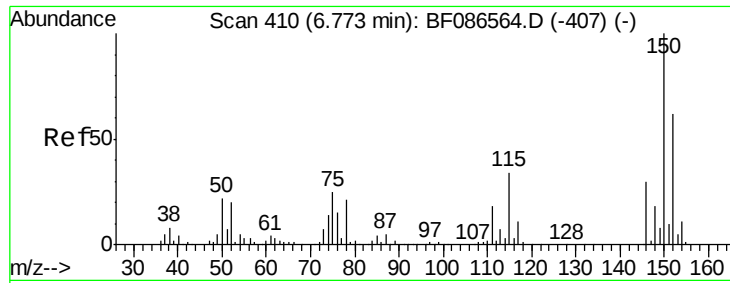

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.76 min Scan# 409

Delta R.T. -0.05 min

Lab File: BF086553.D

Acq: 1 May 2016 6:11

Instrument :

BNA_F

ClientSampleId :

HW-23-4-26-16


Tot Ion:152 Resp: 126528

Ion Ratio Lower Upper

152 100

150 159.9 125.8 188.6




115 69.8 51.5 77.3

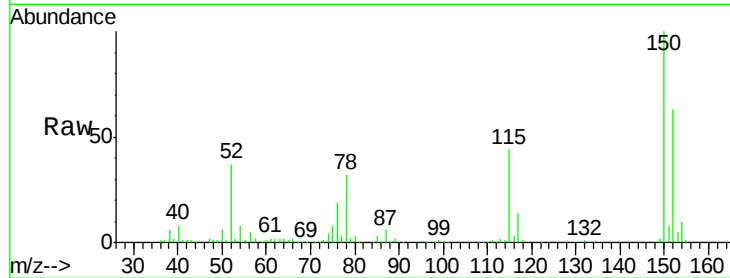

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

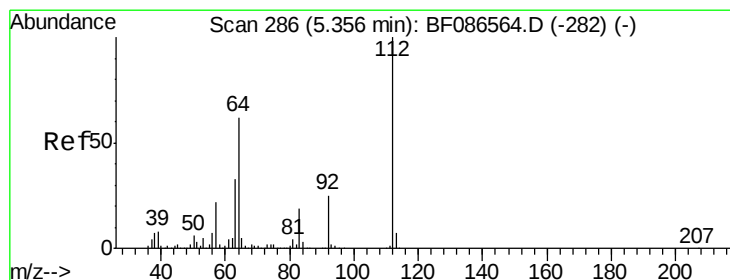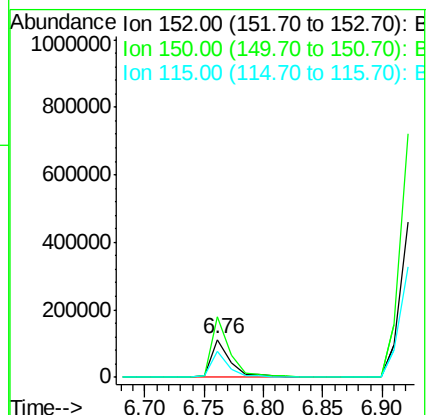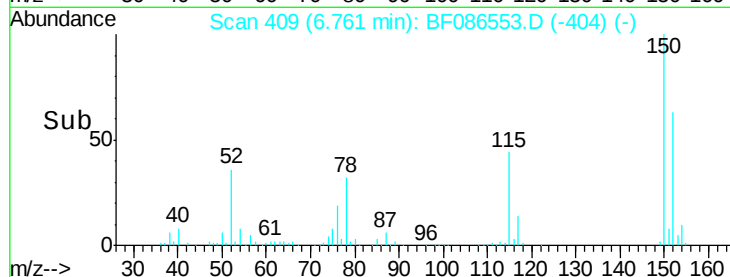

#5

2-Fluorophenol

Concen: 50.91 ng

RT: 5.34 min Scan# 285

Delta R.T. -0.04 min

Lab File: BF086553.D

Acq: 1 May 2016 6:11


Tgt Ion:112 Resp: 373479

Ion Ratio Lower Upper

112 100

64 75.1 52.1 78.1



63 40.0 25.7 38.5#

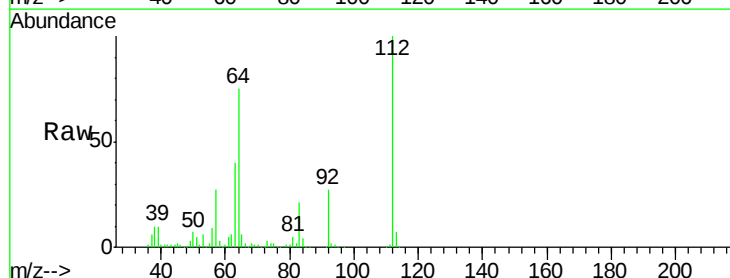


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

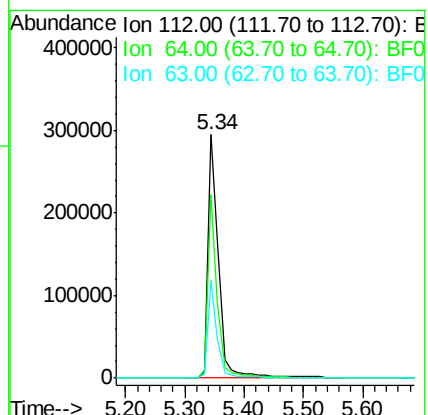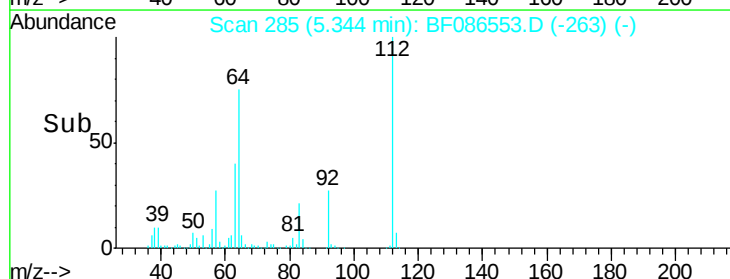

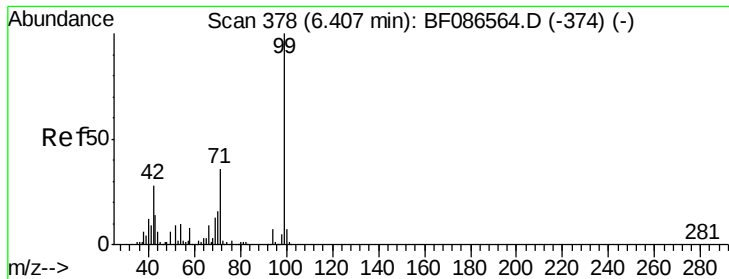

#7

Phenol-d6

Concen: 33.75 ng

RT: 6.40 min Scan# 377

Delta R.T. -0.05 min

Lab File: BF086553.D

Acq: 1 May 2016 6:11

Instrument :

BNA_F

ClientSampleId :

HW-23-4-26-16





Tot Ion: 99 Resp: 345576

Ion Ratio Lower Upper

99 100

42 25.4 13.6 20.4#

71 34.0 24.6 36.8

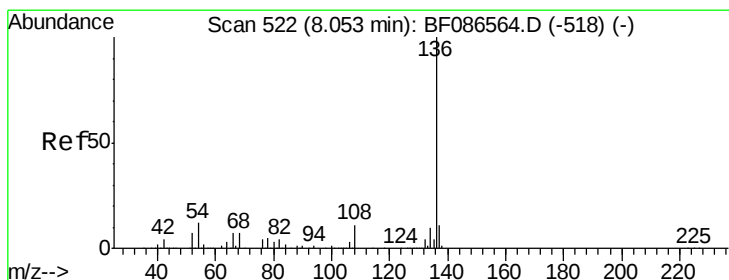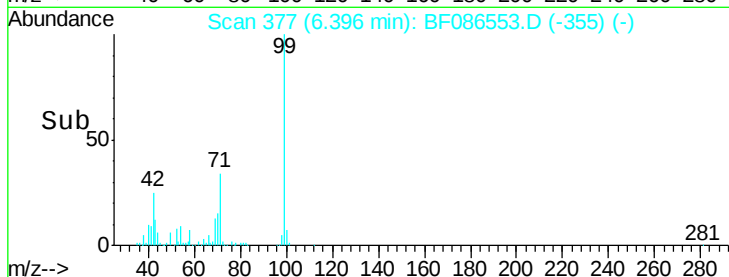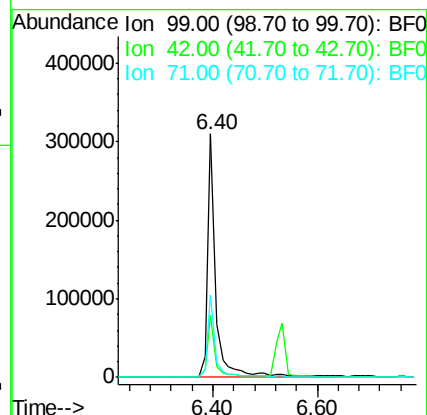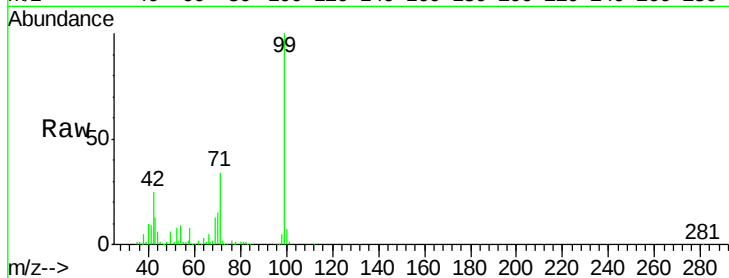

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.05 min Scan# 522

Delta R.T. -0.05 min

Lab File: BF086553.D

Acq: 1 May 2016 6:11

Tgt Ion: 136 Resp: 557032




Ion Ratio Lower Upper


136 100

137 10.7 8.8 13.2

54 9.3 5.0 7.4#

68 5.9 4.4 6.6


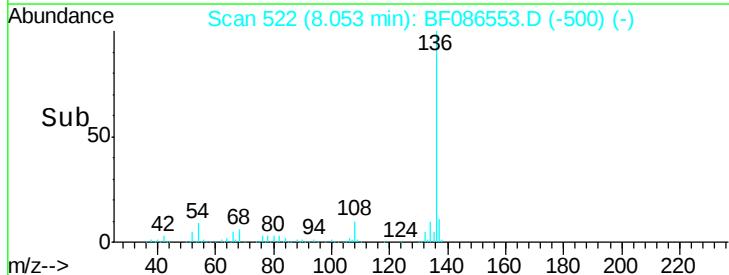
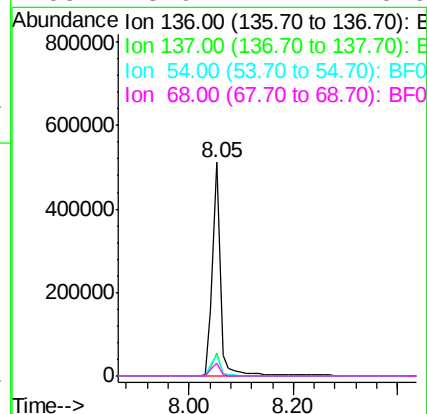
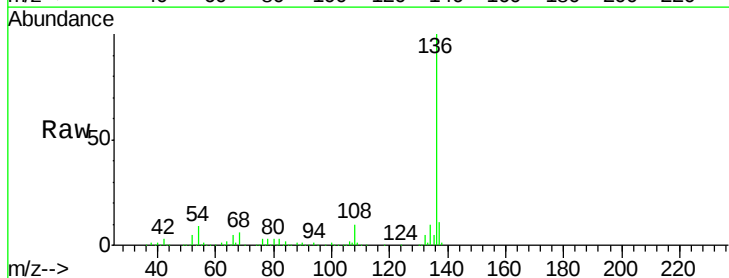


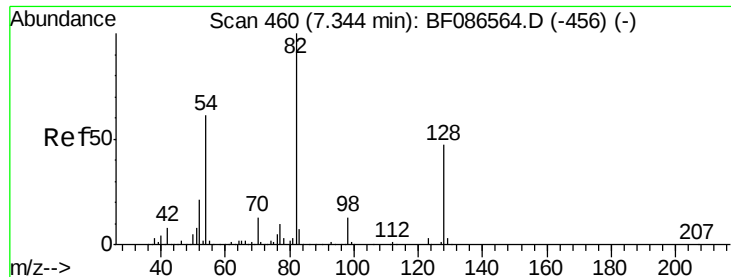

#23
 Nitrobenzene-d5
 Concen: 87.47 ng
 RT: 7.33 min Scan# 459
 Delta R.T. -0.05 min
 Lab File: BF086553.D
 Acq: 1 May 2016 6:11




Instrument :
 BNA_F
 ClientSampleId :
 HW-23-4-26-16


Tot Ion: 82 Resp: 903942
 Ion Ratio Lower Upper
 82 100
 128 41.4 40.6 61.0
 54 65.8 38.1 57.1#

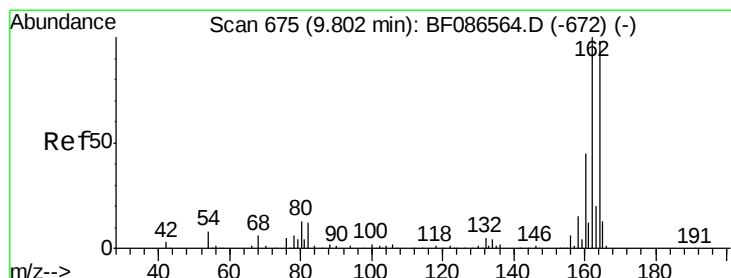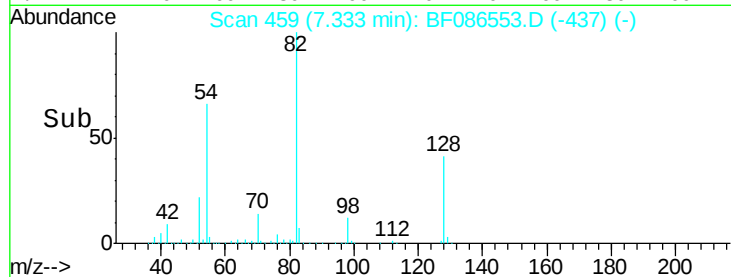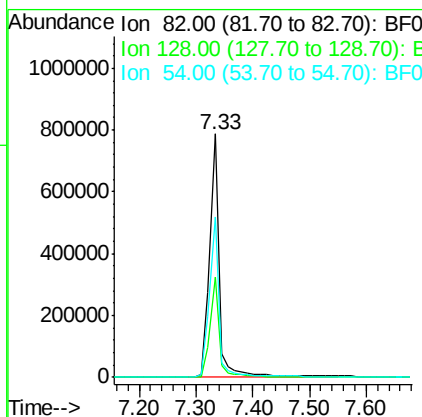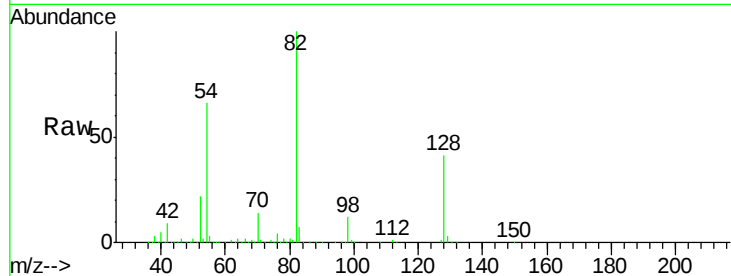

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.80 min Scan# 675
 Delta R.T. -0.05 min
 Lab File: BF086553.D
 Acq: 1 May 2016 6:11

Tgt Ion:164 Resp: 274986
 Ion Ratio Lower Upper
 164 100
 162 103.6 82.8 124.2
 160 46.8 36.9 55.3

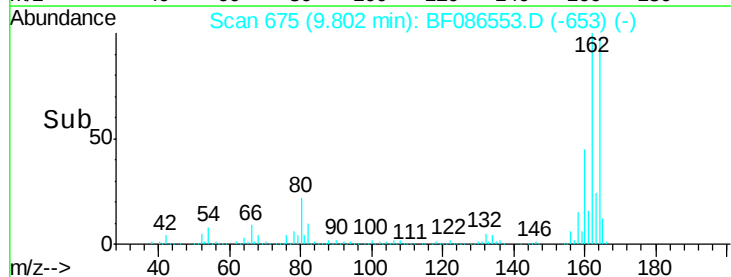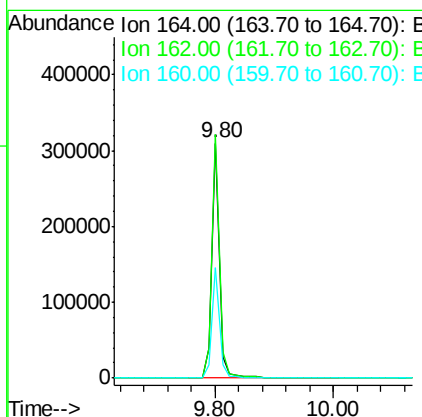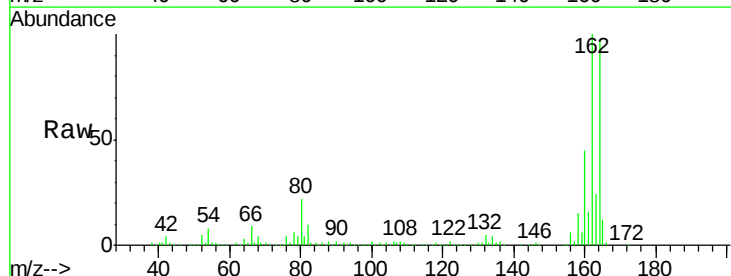


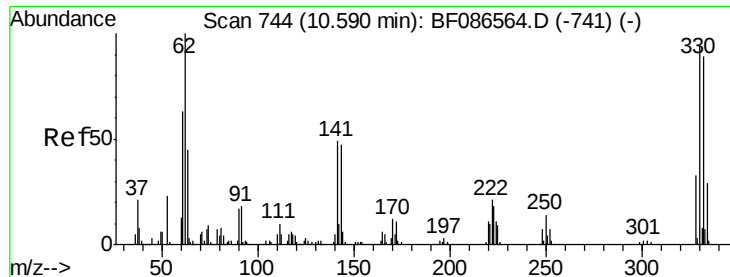




#41
 2,4,6-Tribromophenol
 Concen: 121.36 ng
 RT: 10.59 min Scan# 744
 Delta R.T. -0.05 min
 Lab File: BF086553.D
 Acq: 1 May 2016 6:11

Instrument :
 BNA_F
 ClientSampleId :
 HW-23-4-26-16

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.9	79.0	118.4
141	39.2	31.2	46.8

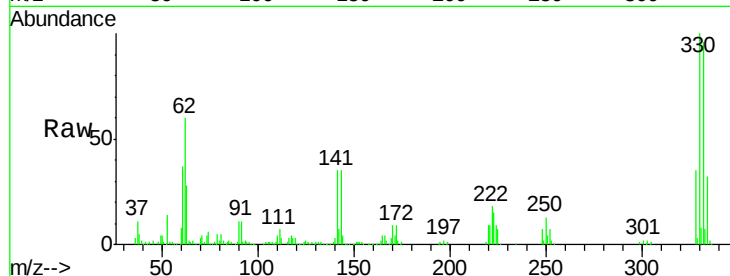


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

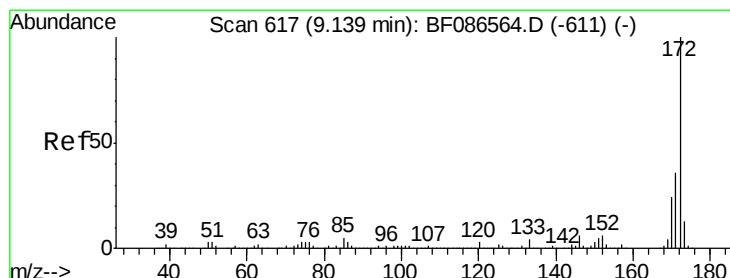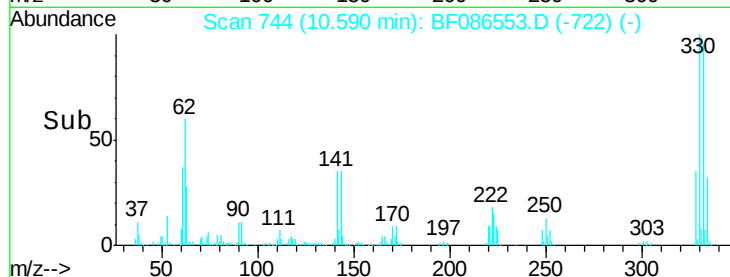
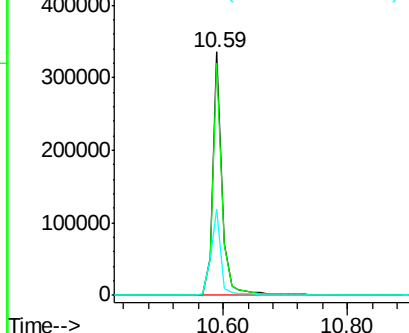



#44
 2-Fluorobiphenyl
 Concen: 85.82 ng
 RT: 9.13 min Scan# 616
 Delta R.T. -0.05 min
 Lab File: BF086553.D
 Acq: 1 May 2016 6:11

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.5	29.0	43.6
170	24.8	19.8	29.8

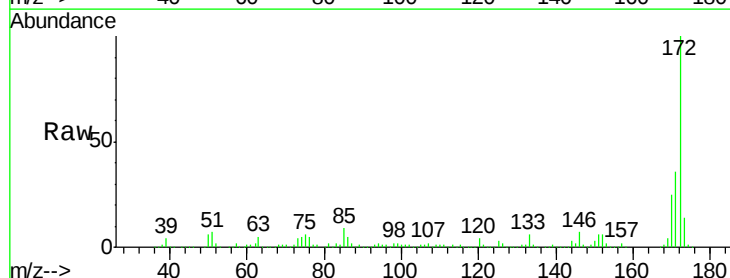

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

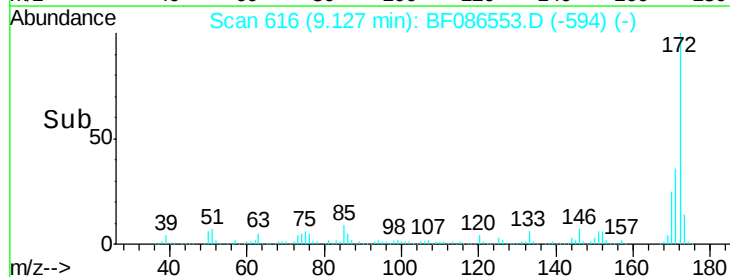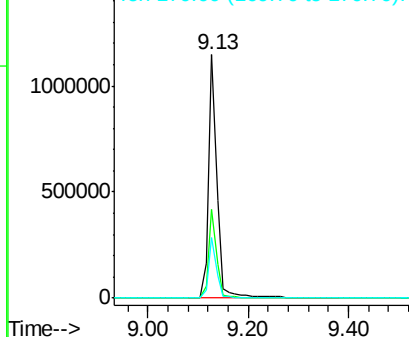

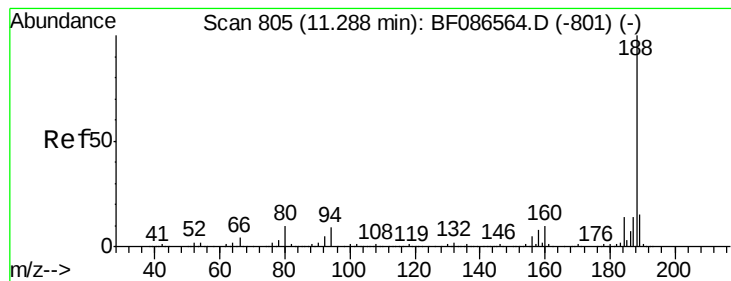

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.28 min Scan# 804

Delta R.T. -0.05 min

Lab File: BF086553.D

Acq: 1 May 2016 6:11

Instrument :

BNA_F

ClientSampleId :

HW-23-4-26-16


Tot Ion:188 Resp: 483682

Ion Ratio Lower Upper

188 100

94 14.4 6.8 10.2#




80 16.5 7.1 10.7#

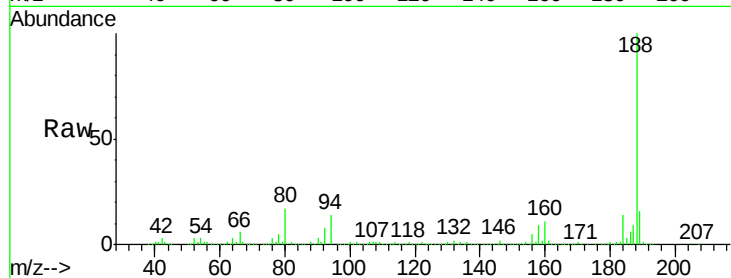

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

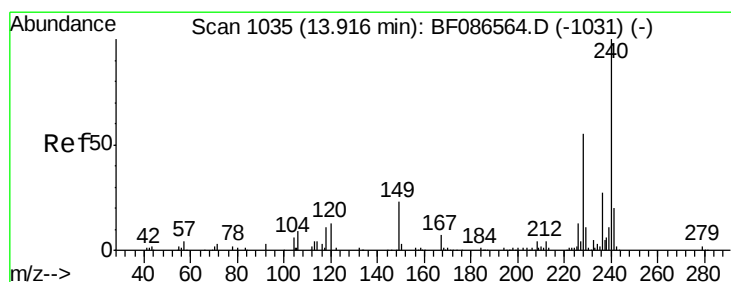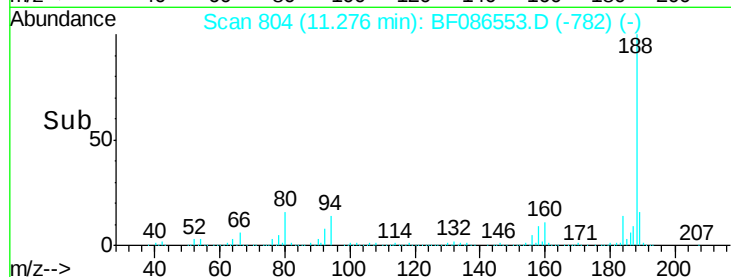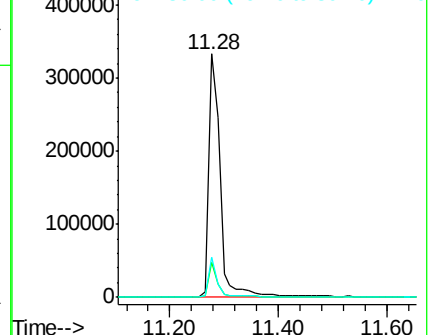

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.91 min Scan# 1034

Delta R.T. -0.06 min

Lab File: BF086553.D

Acq: 1 May 2016 6:11


Tgt Ion:240 Resp: 340257

Ion Ratio Lower Upper

240 100

120 16.3 11.2 16.8



236 26.5 21.2 31.8

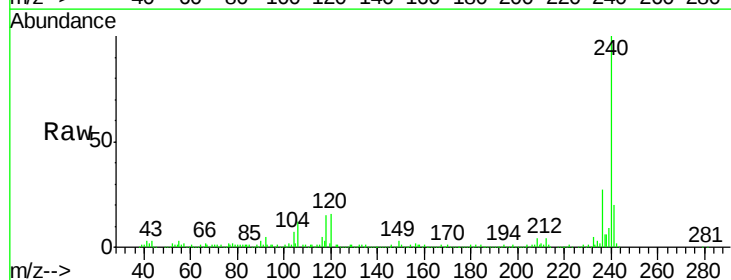


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E



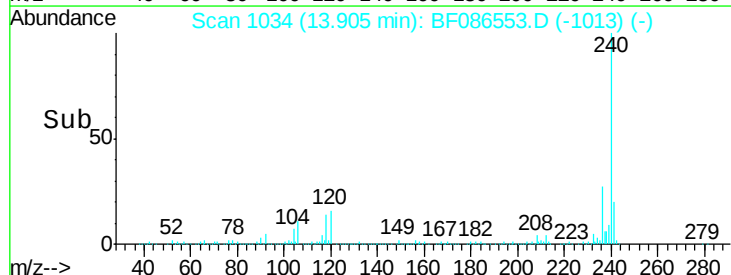
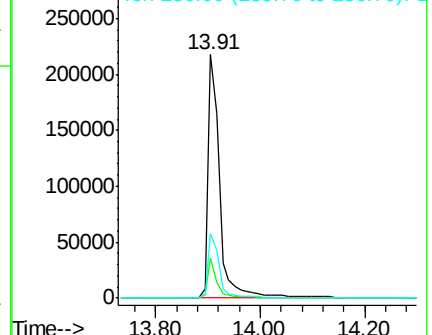


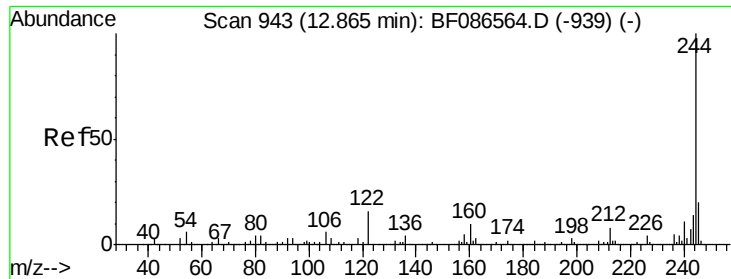

#78
 Terphenyl-d14
 Concen: 84.37 ng
 RT: 12.86 min Scan# 943
 Delta R.T. -0.05 min
 Lab File: BF086553.D
 Acq: 1 May 2016 6:11

Instrument :
 BNA_F
 ClientSampleId :
 HW-23-4-26-16

Tot Ion:244 Resp: 1302968
 Ion Ratio Lower Upper
 244 100
 212 8.1 6.2 9.2
 122 16.0 12.0 18.0

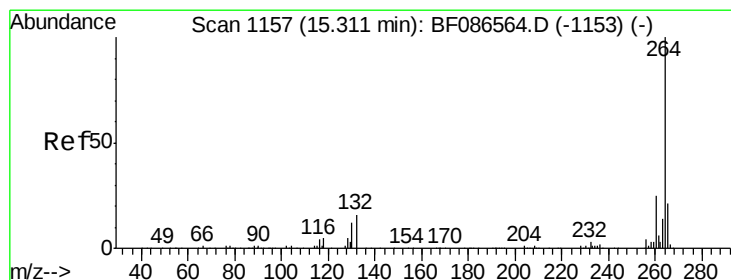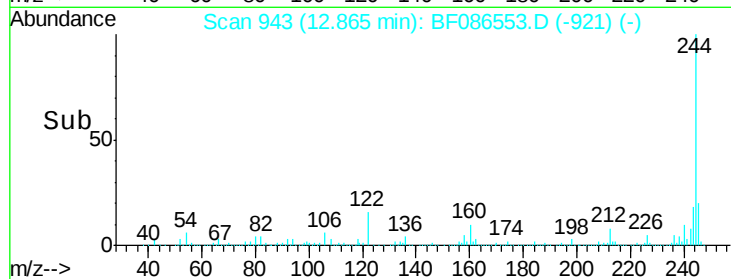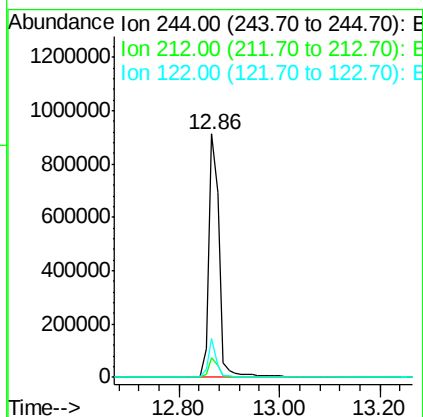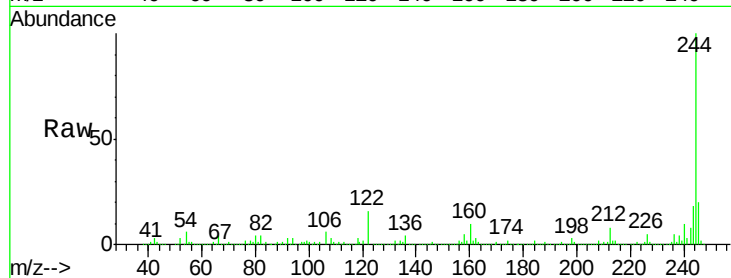

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.30 min Scan# 1156
 Delta R.T. -0.06 min
 Lab File: BF086553.D
 Acq: 1 May 2016 6:11

Tgt Ion:264 Resp: 290388
 Ion Ratio Lower Upper
 264 100
 260 24.5 19.5 29.3
 265 21.0 17.3 25.9

