

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF043016\
 Data File : BF086556.D
 Acq On : 1 May 2016 7:36
 Operator : UM/SJ
 Sample : H2737-09
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 HW-10-4-26-16

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.921	246	248	256	rBV	67134	83009	1.96%	0.290%
2	5.356	283	286	288	rBV	1431739	1629962	38.49%	5.691%
3	6.396	375	377	386	rBV	925946	1098749	25.95%	3.836%
4	6.533	386	389	391	rBV	3479495	3383098	79.89%	11.812%
5	6.762	407	409	419	rBV	847297	910887	21.51%	3.180%
6	6.922	420	423	425	rBV	3295435	3093634	73.05%	10.801%
7	7.333	456	459	461	rBV	2681533	2729820	64.46%	9.531%
8	8.053	519	522	524	rBV	1145745	1162986	27.46%	4.060%
9	8.407	549	553	558	rBV5	21874	77314	1.83%	0.270%
10	8.533	562	564	567	rVB	63681	73988	1.75%	0.258%
11	9.127	613	616	619	rBV	3865282	4234694	100.00%	14.785%
12	9.470	643	646	647	rBV2	73068	91844	2.17%	0.321%
13	9.528	649	651	654	rVV	103807	132311	3.12%	0.462%
14	9.802	672	675	677	rBV	1439636	1366953	32.28%	4.773%
15	9.870	679	681	683	rVV3	37349	54350	1.28%	0.190%
16	10.590	741	744	747	rBV	2436445	2511792	59.31%	8.770%
17	11.288	802	805	807	rBV	744296	1022631	24.15%	3.570%
18	12.876	941	944	946	rBV	2296188	3002181	70.89%	10.482%
19	13.917	1033	1035	1041	rVB	686422	694673	16.40%	2.425%
20	15.311	1155	1157	1173	rVB	630046	1286856	30.39%	4.493%


Sum of corrected areas: 28641732

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF043016\
Data File : BF086556.D
Acq On : 1 May 2016 7:36
Operator : UM/SJ
Sample : H2737-09
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HW-10-4-26-16

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

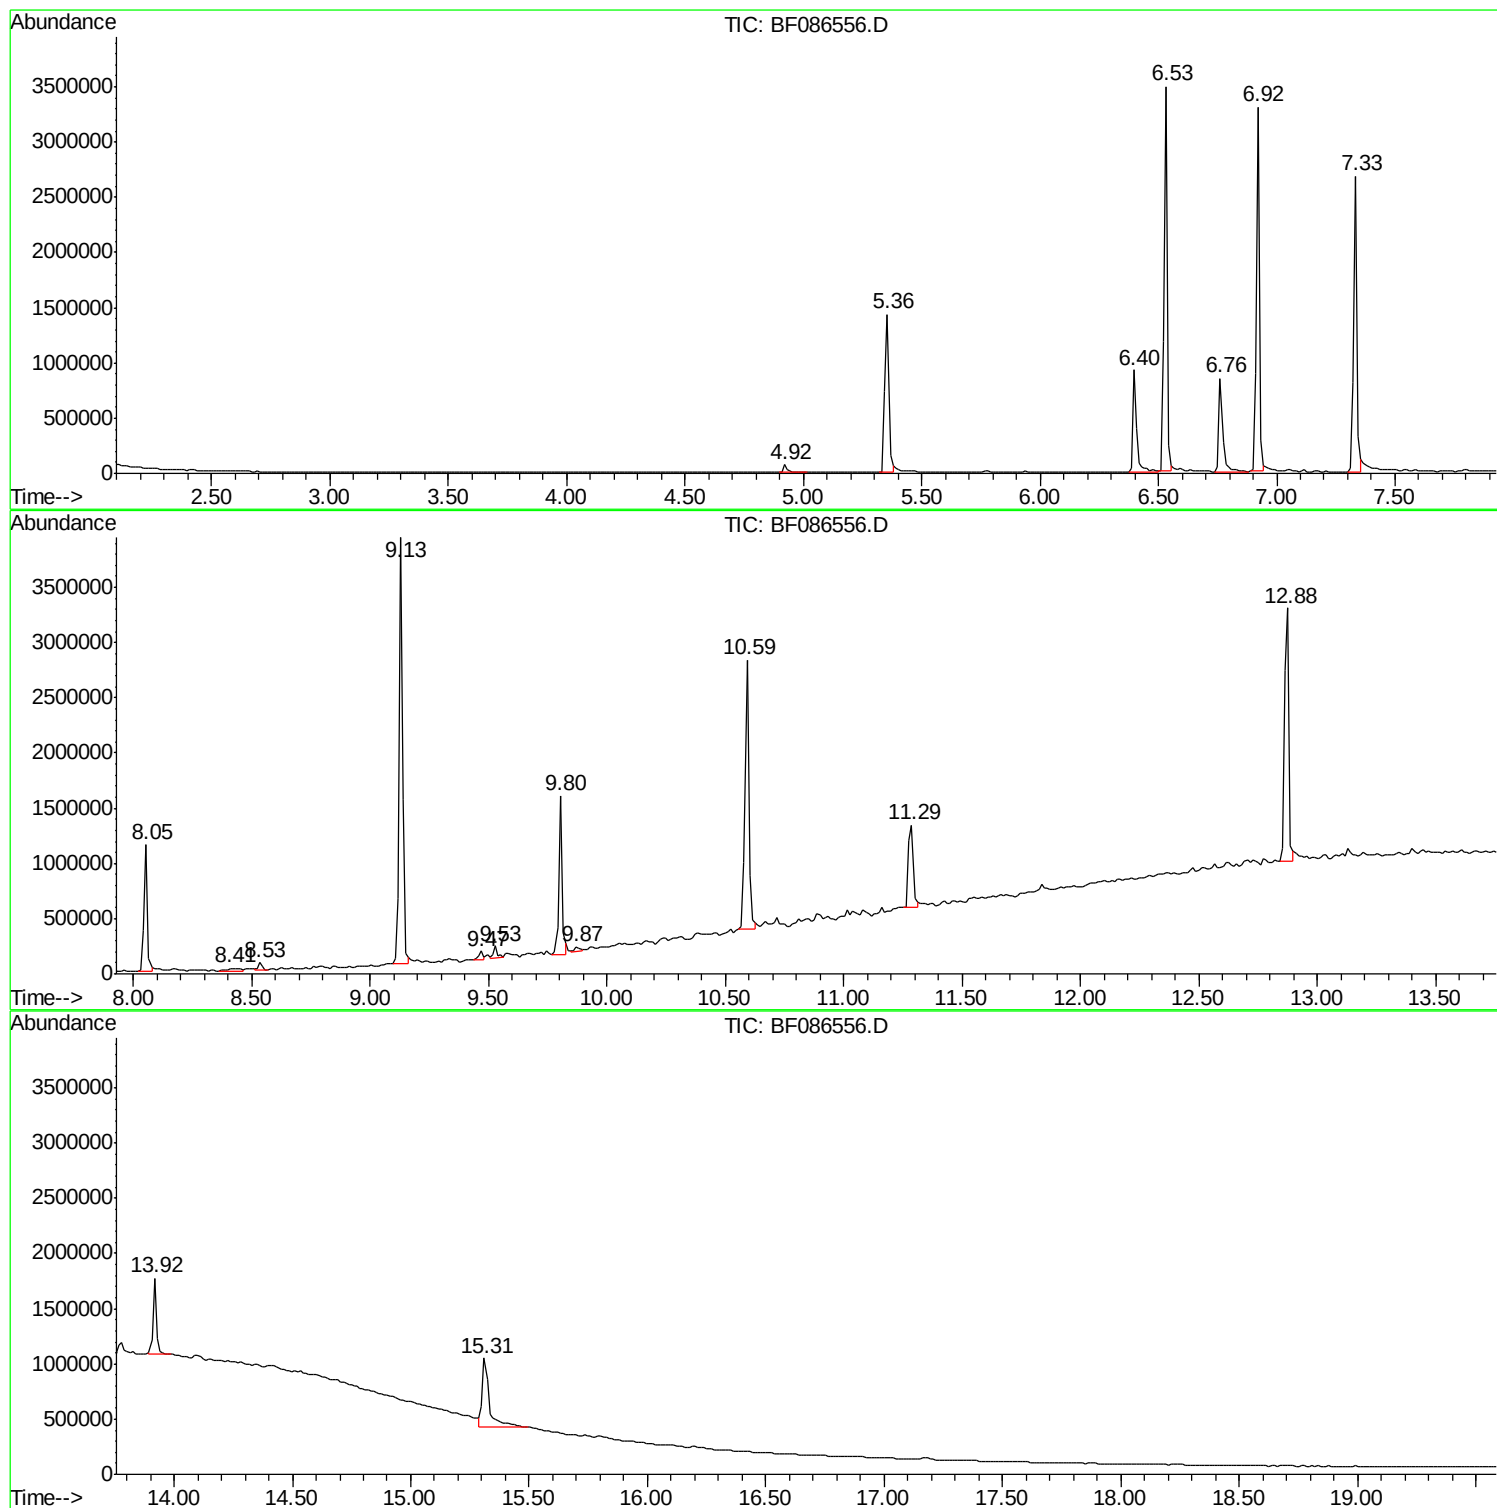

Data Path : Z:\HPCHEM1\BNA F\DATA\BF043016\
Data File : BF086556.D
Acq On : 1 May 2016 7:36
Operator : UM/SJ
Sample : H2737-09
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HW-10-4-26-16










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF042716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.53 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.53	74.28 ng	3383100	1,4-Dichlorobenzene-d4	6.76

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	16
2		(5-METHYL-2-PYRIDYL)ACETONITRILE	132	C8H8N2	1000241-93-9	10
3		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	9
4		Benzene, 1,2,4-trifluoro-	132	C6H3F3	000367-23-7	9
5		Benzene, 1,3,5-trifluoro-	132	C6H3F3	000372-38-3	9

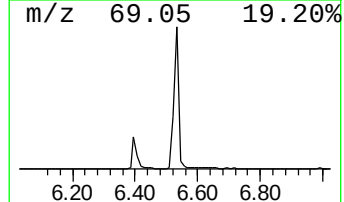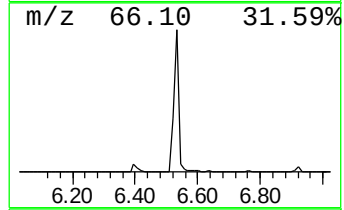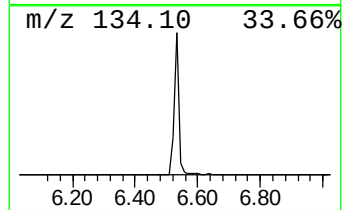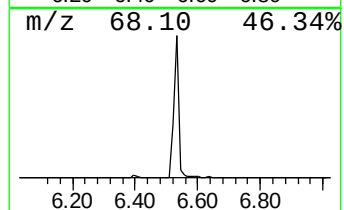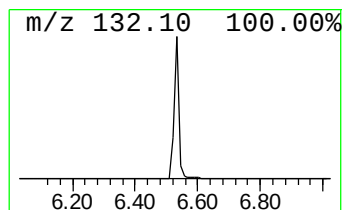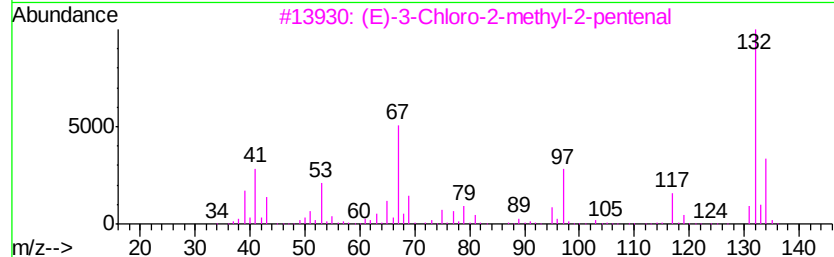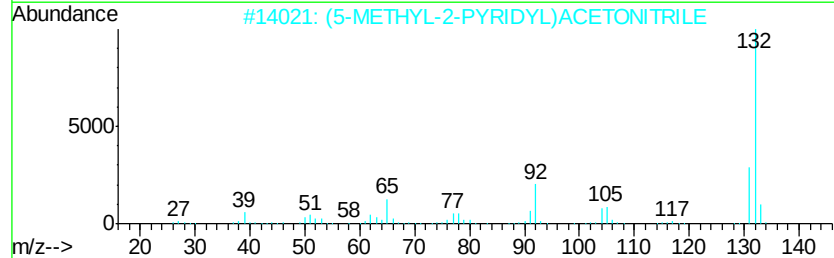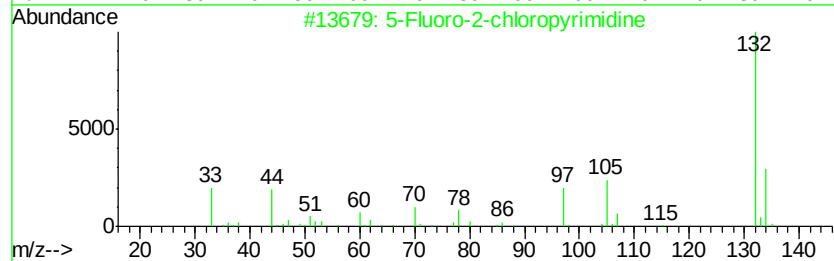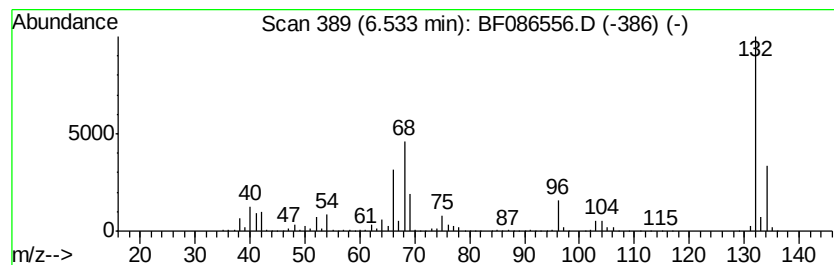

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF043016\
Data File : BF086556.D
Acq On : 1 May 2016 7:36
Operator : UM/SJ
Sample : H2737-09
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HW-10-4-26-16

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.53	6.53	74.3	ng	3383100	1	6.76	910887	20.0