


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF043016\
 Data File : BF086512.D
 Acq On : 30 Apr 2016 9:21
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 27 14:20:52 2016

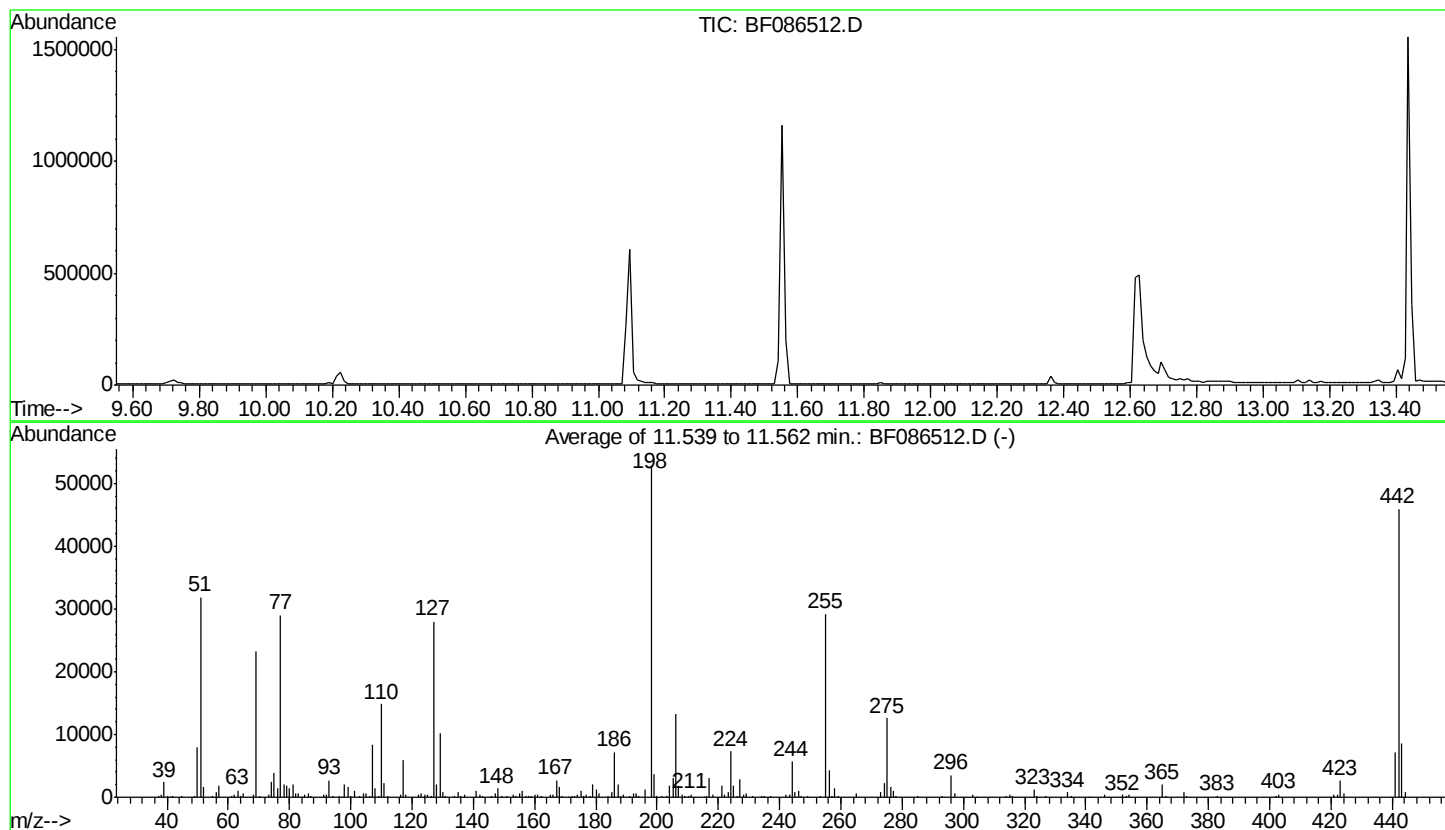

AutoFind: Scans 827, 828, 829; Background Corrected with Scan 824

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	60.4	31889	PASS
68	69	0.00	2	1.5	345	PASS
69	198	0.00	100	44.1	23291	PASS
70	69	0.00	2	0.6	132	PASS
127	198	10	80	53.1	28040	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	52821	PASS
199	198	5	9	6.9	3667	PASS
275	198	10	60	23.8	12566	PASS
365	198	1	100	3.7	1959	PASS
441	442	0.01	24	15.5	7110	PASS
442	198	50	100	87.0	45938	PASS
443	442	15	24	18.6	8547	PASS