


Data Path : Z:\HPCHEM1\BNA F\DATA\BF043016\
Data File : BF086537.D
Acq On : 30 Apr 2016 21:37
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042716.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Apr 27 14:20:52 2016

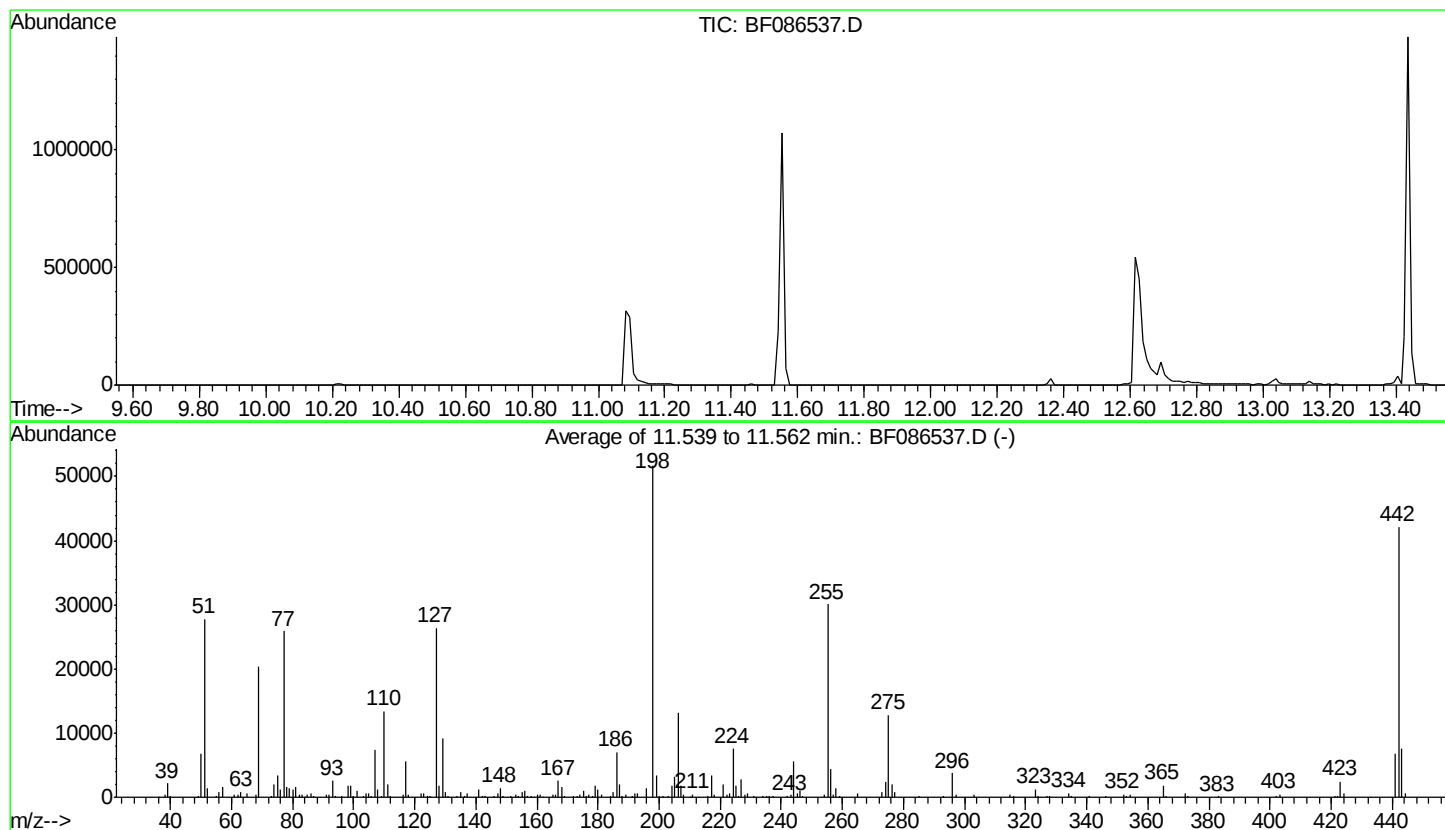

AutoFind: Scans 827, 828, 829; Background Corrected with Scan 824

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.9	27838	PASS
68	69	0.00	2	1.7	347	PASS
69	198	0.00	100	39.3	20295	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.0	26360	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	51686	PASS
199	198	5	9	6.5	3363	PASS
275	198	10	60	24.9	12845	PASS
365	198	1	100	3.6	1850	PASS
441	442	0.01	24	16.0	6731	PASS
442	198	50	100	81.6	42154	PASS
443	442	15	24	18.0	7602	PASS