

Data Path : Z:\HPCHEM1\BNA F\DATA\BF043017\
 Data File : BF094717.D
 Acq On : 30 Apr 2017 16:26
 Operator : SJ/MA
 Sample : I2860-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: May 01 01:20:46 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF041717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 17 14:59:23 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	5.77	152	116085	20.00	ng	0.00
21) Naphthalene-d8	7.25	136	469551	20.00	ng	0.00
38) Acenaphthene-d10	9.39	164	228116	20.00	ng	0.00
63) Phenanthrene-d10	11.21	188	412059	20.00	ng	0.00
75) Chrysene-d12	14.47	240	311727	20.00	ng	0.00
86) Perylene-d12	16.09	264	217337	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	4.32	112	273200	39.05	ng	0.01
7) Phenol-d6	5.38	99	215730	26.15	ng	0.00
23) Nitrobenzene-d5	6.41	82	647937	85.21	ng	0.00
41) 2,4,6-Tribromophenol	10.37	330	167812	94.05	ng	0.00
44) 2-Fluorobiphenyl	8.58	172	1274855	82.23	ng	0.00
78) Terphenyl-d14	13.19	244	1145827	98.25	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	6.41	70	85535	15.65	ng	# 75
49) Dimethylphthalate	9.08	163	124178	7.30	ng	99
56) 2,4-Dinitrotoluene	9.39	165	28377	6.06	ng	# 33

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF043017\
Data File : BF094717.D
Acq On : 30 Apr 2017 16:26
Operator : SJ/MA
Sample : I2860-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: May 01 01:20:46 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF041717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 17 14:59:23 2017
Response via : Initial Calibration

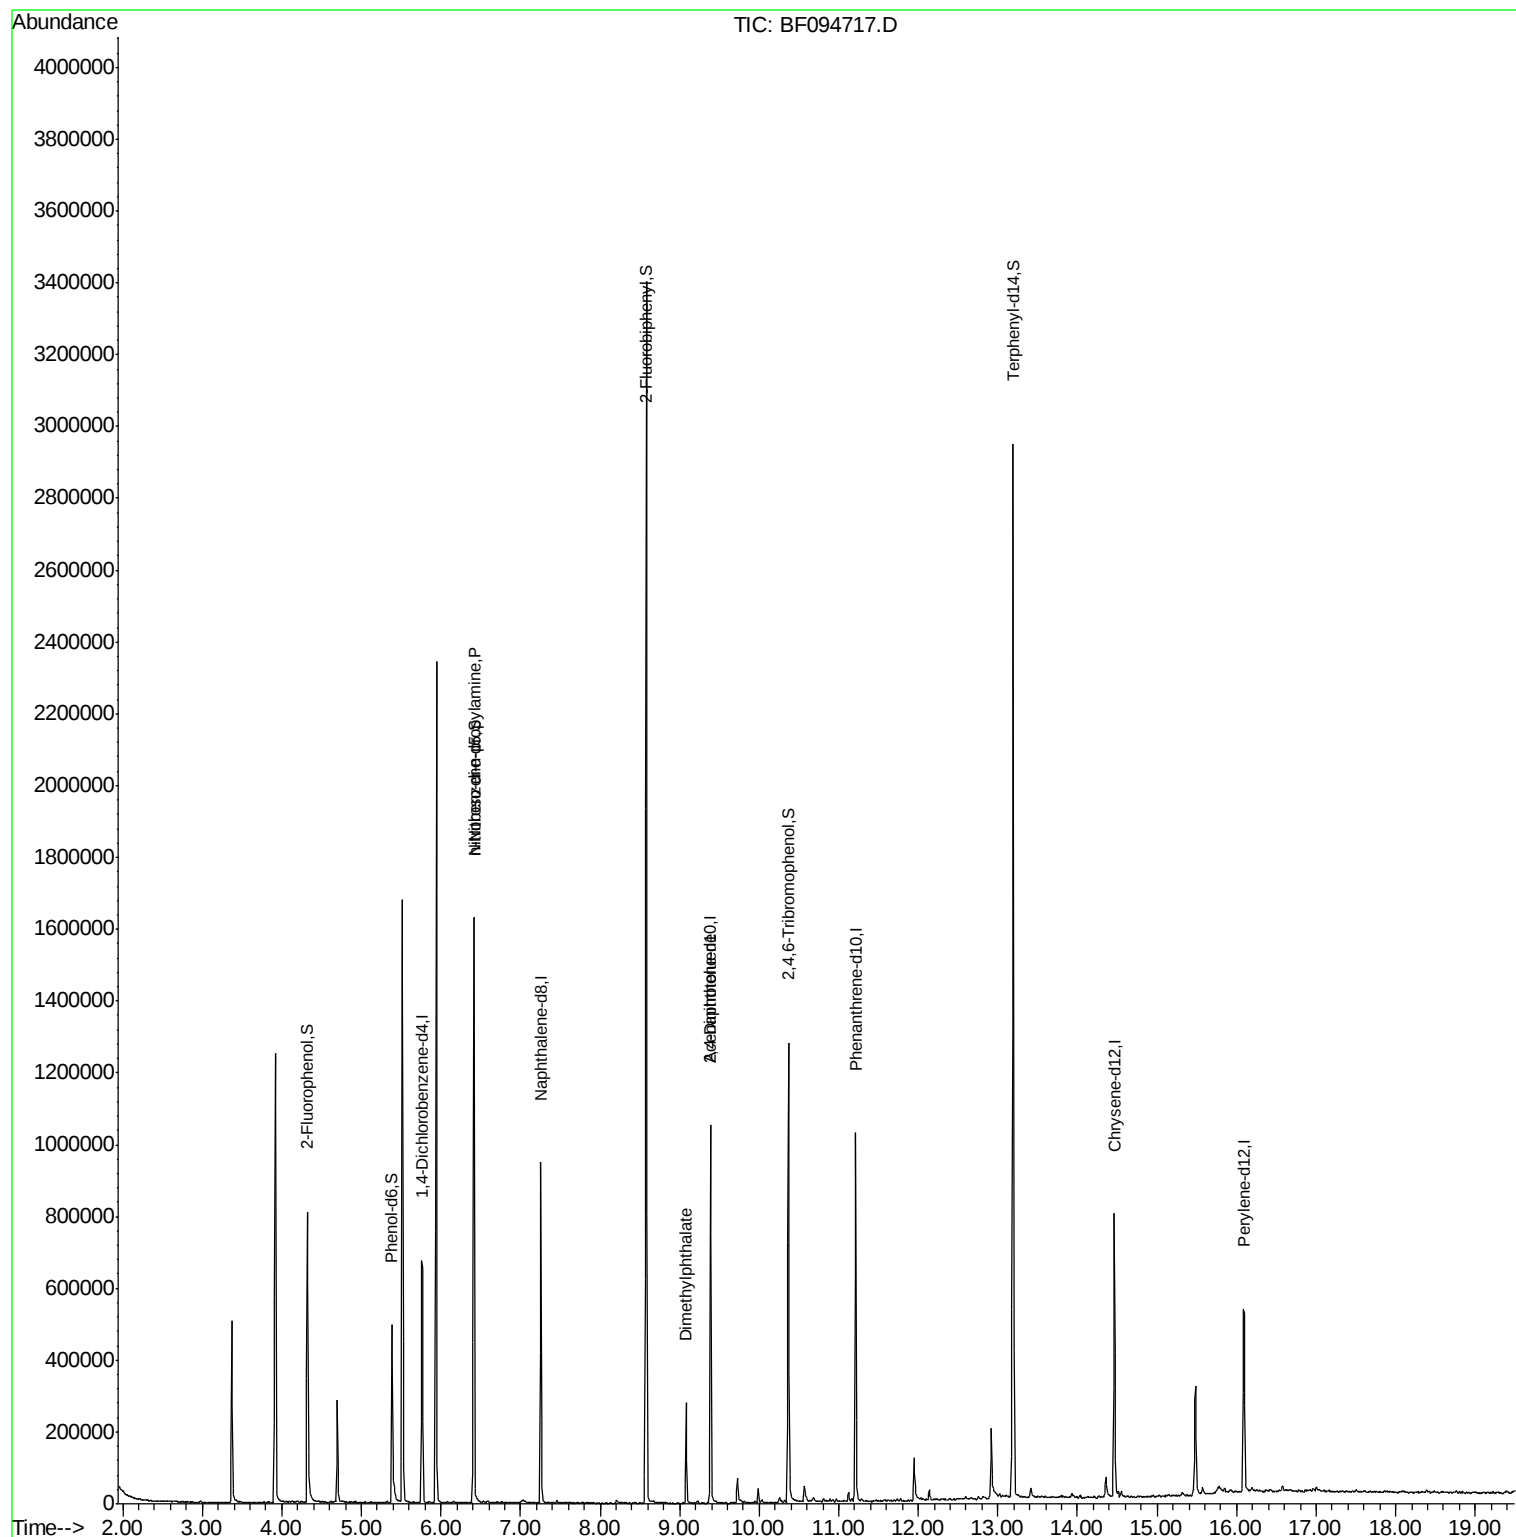




#1



1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 5.77 min Scan# 651
Delta R.T. 0.00 min
Lab File: BF094717.D
Acq: 30 Apr 2017 16:26

Instrument :
BNA_F
ClientSampleId :

Tot Ion:152 Resp: 116085
Ion Ratio Lower Upper
152 100
150 157.3 126.2 189.2
115 59.0 52.2 78.2

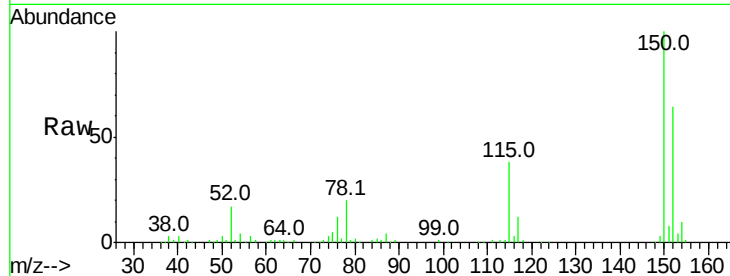


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

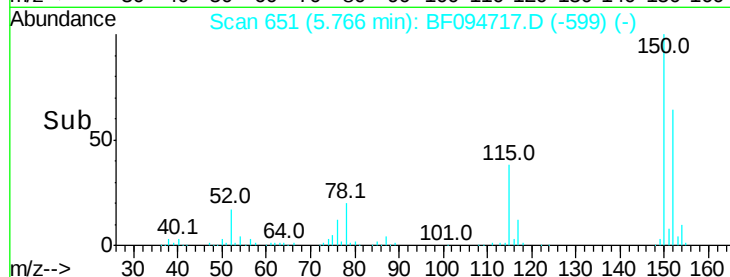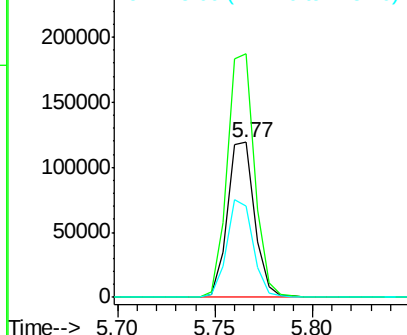



#5


2-Fluorophenol
Concen: 39.05 ng
RT: 4.32 min Scan# 405
Delta R.T. 0.01 min
Lab File: BF094717.D
Acq: 30 Apr 2017 16:26

Tgt Ion:112 Resp: 273200
Ion Ratio Lower Upper
112 100
64 54.9 46.0 69.0
63 27.7 23.4 35.0

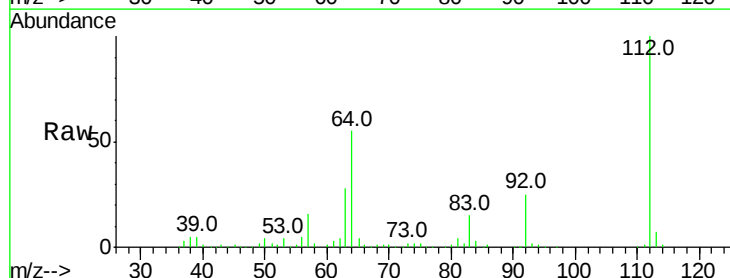

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

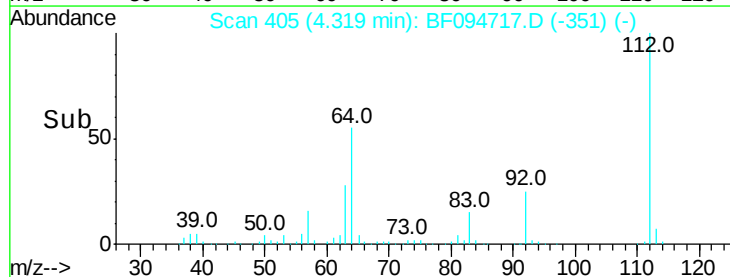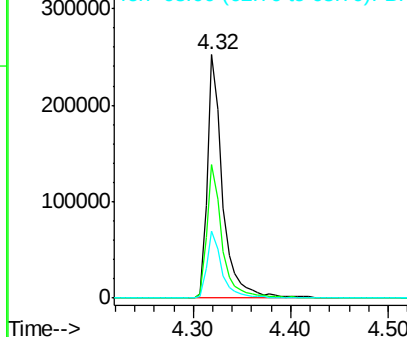

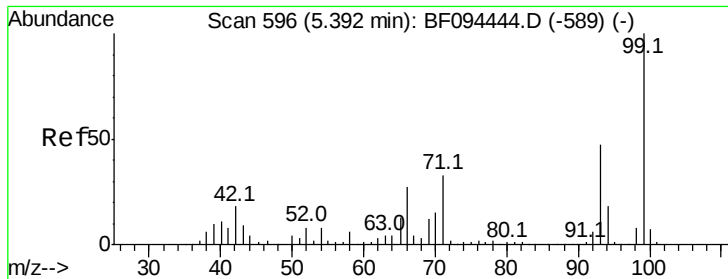

#7

Phenol-d6

Concen: 26.15 ng

RT: 5.38 min Scan# 586

Delta R.T. -0.01 min

Lab File: BF094717.D

Acq: 30 Apr 2017 16:26

Instrument :

BNA_F

ClientSampled :


Tot Ion: 99 Resp: 215730

Ion Ratio Lower Upper




99 100

42 16.0 13.5 20.3

71 32.3 24.5 36.7

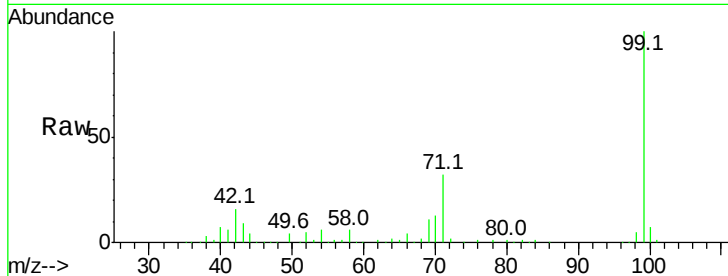

Abundance Ion 99.00 (98.70 to 99.70): BF0
Ion 42.00 (41.70 to 42.70): BF0
Ion 71.00 (70.70 to 71.70): BF0

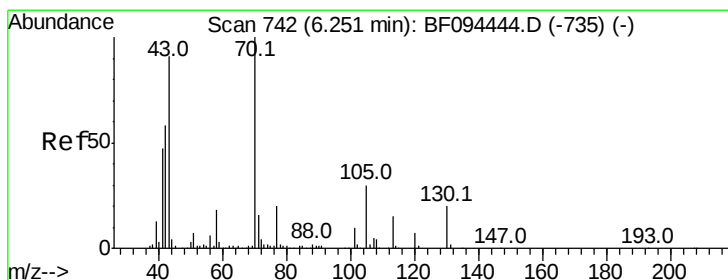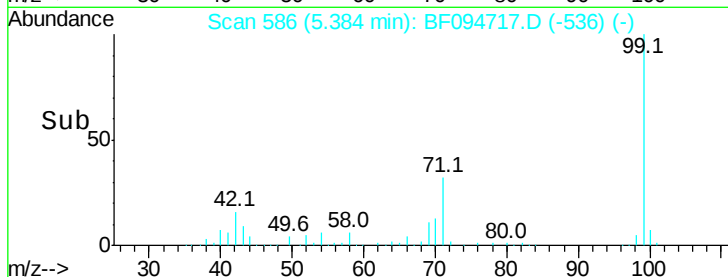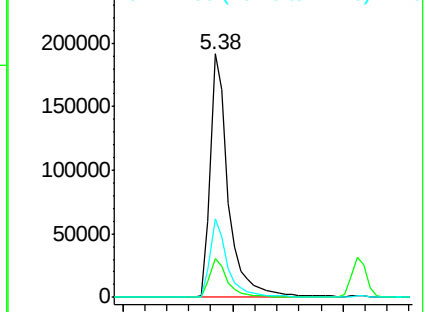

#19

n-Nitroso-di-n-propylamine

Concen: 15.65 ng

RT: 6.41 min Scan# 761

Delta R.T. 0.16 min

Lab File: BF094717.D

Acq: 30 Apr 2017 16:26

Tgt Ion: 70 Resp: 85535


Ion Ratio Lower Upper

70 100



42 43.5 47.2 70.8#


101 0.0 7.2 10.8#

130 2.1 15.9 23.9#

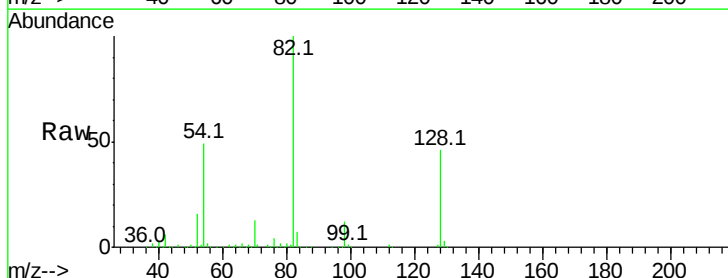

Abundance Ion 70.00 (69.70 to 70.70): BF0
Ion 42.00 (41.70 to 42.70): BF0
Ion 101.00 (100.70 to 101.70): E
Ion 130.00 (129.70 to 130.70): E

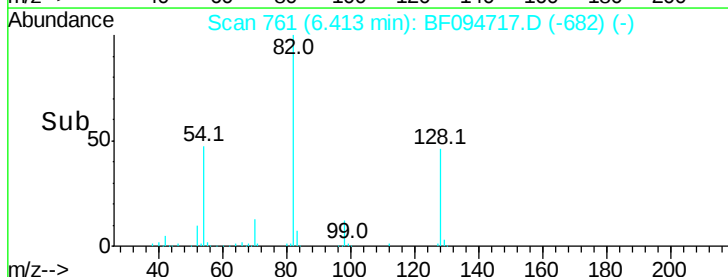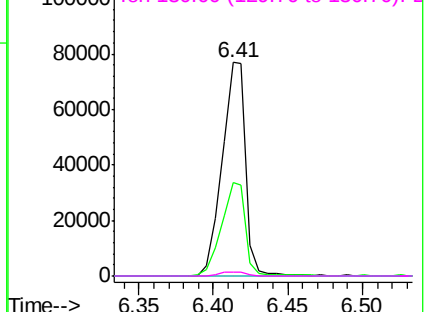

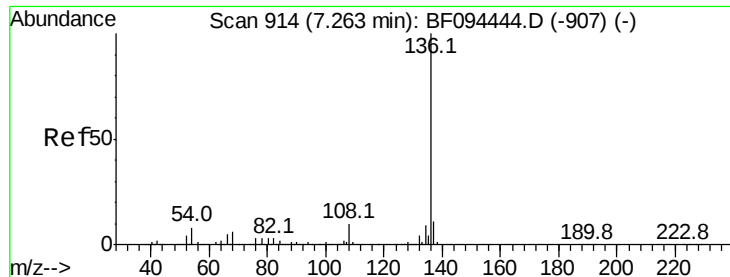

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.25 min Scan# 904

Delta R.T. -0.01 min

Lab File: BF094717.D

Acq: 30 Apr 2017 16:26

Instrument :

BNA_F

ClientSampleId :

Tot Ion:136 Resp: 469551


Ion Ratio Lower Upper

136 100

137 11.2 8.5 12.7

54 7.3 4.9 7.3#

68 6.0 4.1 6.1



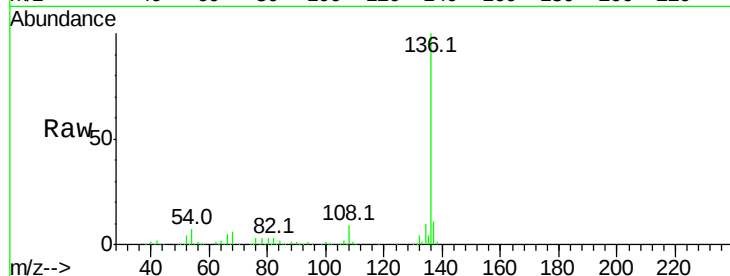


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

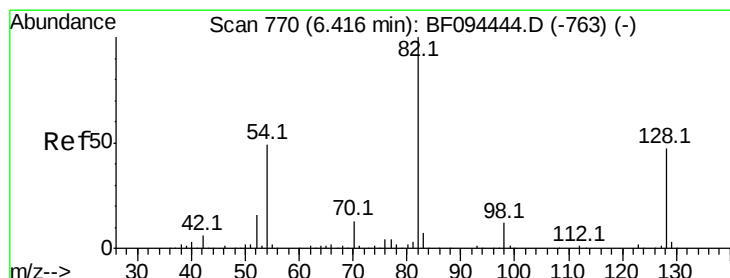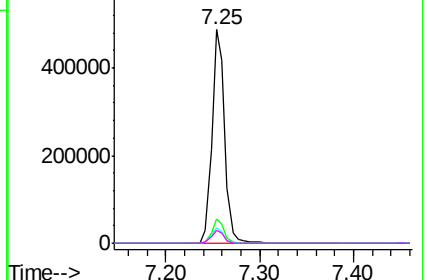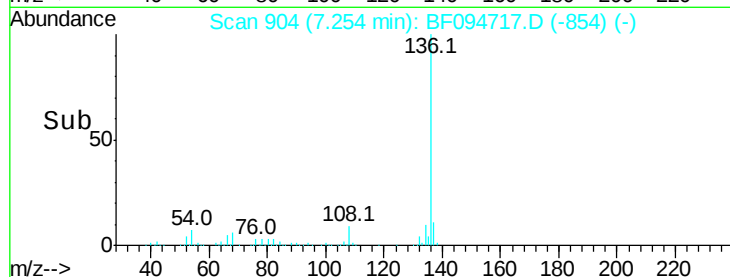

#23

Nitrobenzene-d5

Concen: 85.21 ng

RT: 6.41 min Scan# 761

Delta R.T. -0.00 min

Lab File: BF094717.D

Acq: 30 Apr 2017 16:26


Tgt Ion: 82 Resp: 647937

Ion Ratio Lower Upper

82 100

128 45.7 34.0 51.0



54 48.9 42.2 63.2

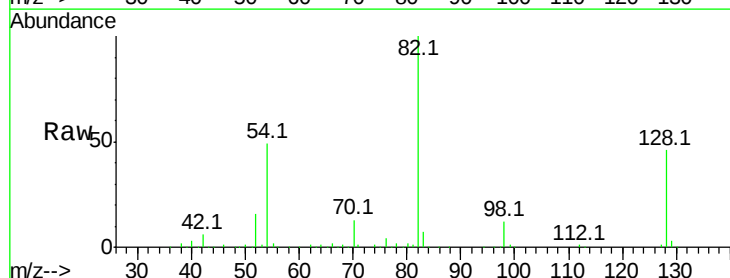

Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF0

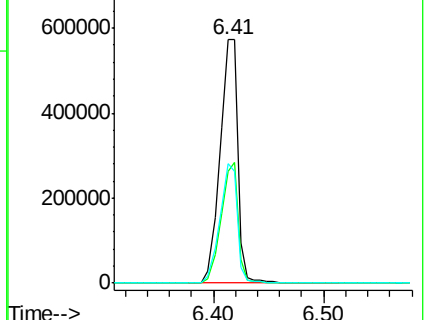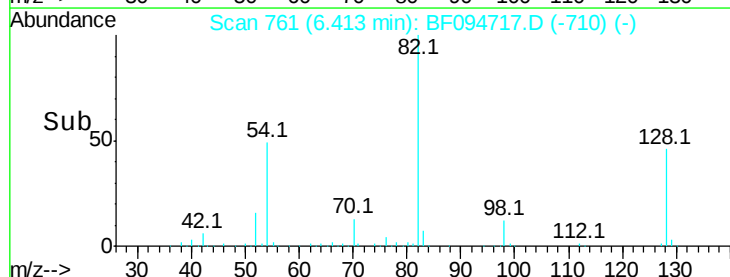



#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.39 min Scan# 1267

Delta R.T. -0.01 min

Lab File: BF094717.D

Acq: 30 Apr 2017 16:26

Instrument :

BNA_F

ClientSampleId :


Tot Ion:164 Resp: 228116

Ion Ratio Lower Upper

164 100

162 100.2 82.6 123.8




160 45.2 36.2 54.2

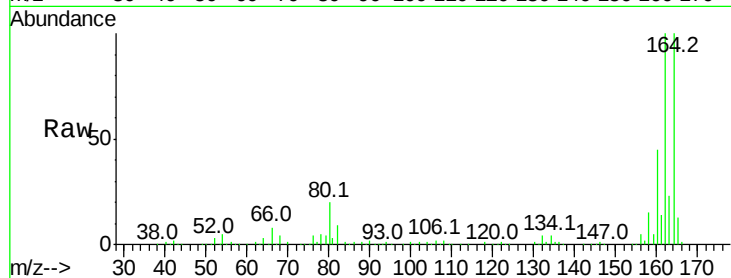

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

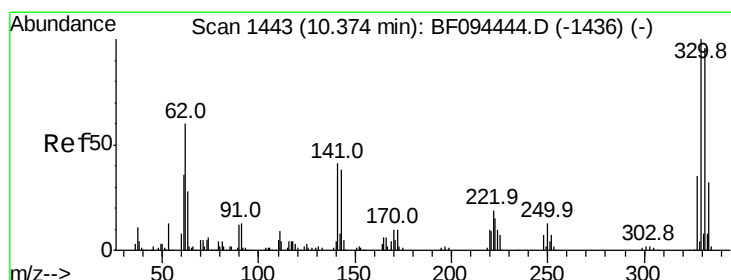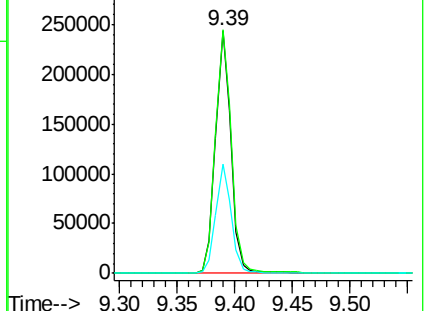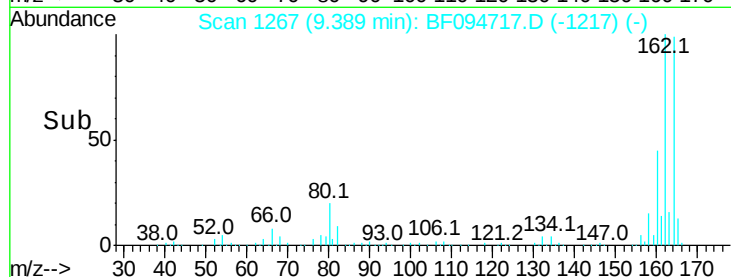

#41

2,4,6-Tribromophenol

Concen: 94.05 ng

RT: 10.37 min Scan# 1434

Delta R.T. -0.00 min

Lab File: BF094717.D

Acq: 30 Apr 2017 16:26


Tgt Ion:330 Resp: 167812

Ion Ratio Lower Upper

330 100

332 97.5 76.6 115.0



141 38.7 31.4 47.2

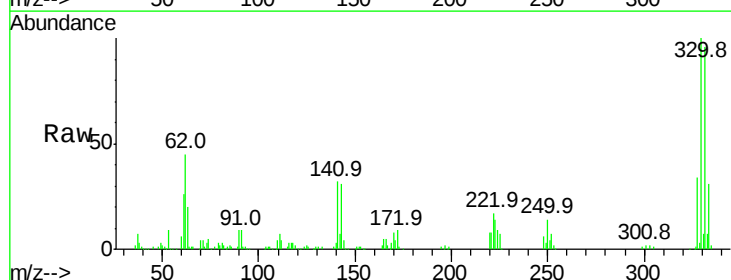


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

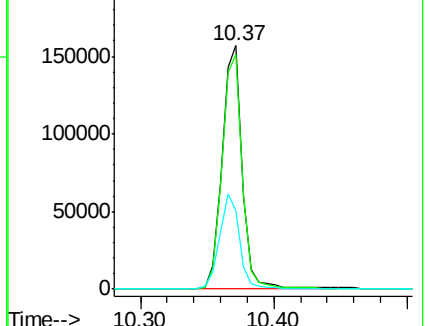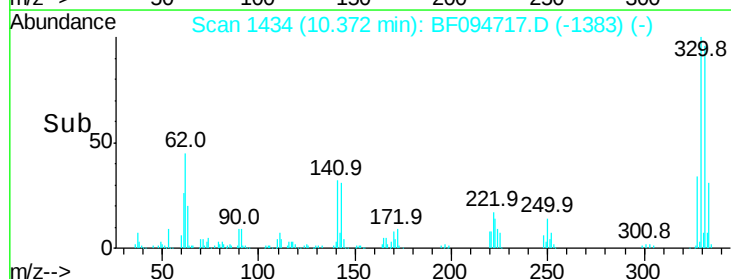


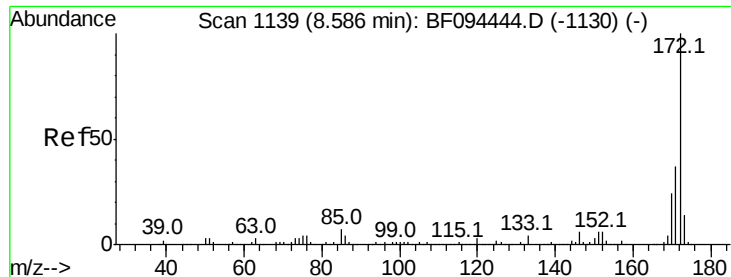




#44
2-Fluorobiphenyl
Concen: 82.23 ng
RT: 8.58 min Scan# 1130
Delta R.T. -0.00 min
Lab File: BF094717.D
Acq: 30 Apr 2017 16:26

Instrument :
BNA_F
ClientSampleId :

Tot Ion:172 Resp: 1274855
Ion Ratio Lower Upper
172 100
171 36.3 29.6 44.4
170 24.0 19.8 29.8

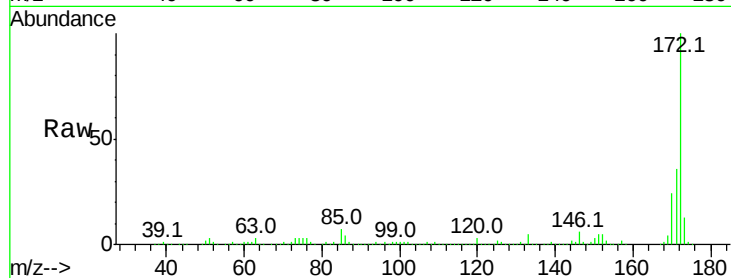


Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

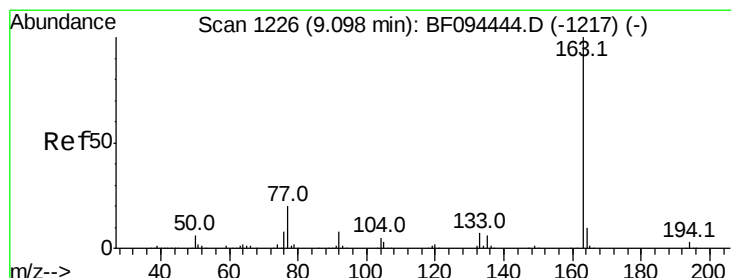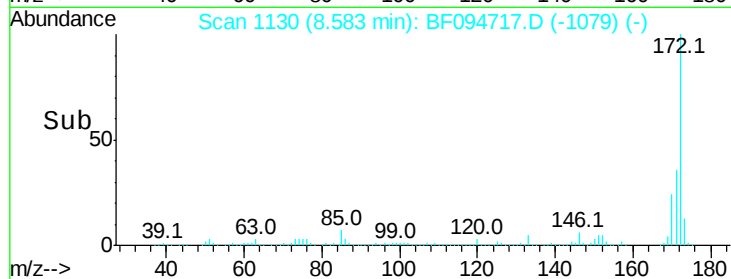
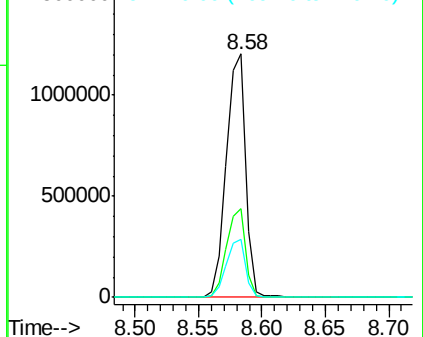


#49
Dimethylphthalate
Concen: 7.30 ng
RT: 9.08 min Scan# 1215
Delta R.T. -0.01 min
Lab File: BF094717.D
Acq: 30 Apr 2017 16:26

Tgt Ion:163 Resp: 124178
Ion Ratio Lower Upper
163 100
194 3.8 2.6 4.0
164 10.0 8.4 12.6

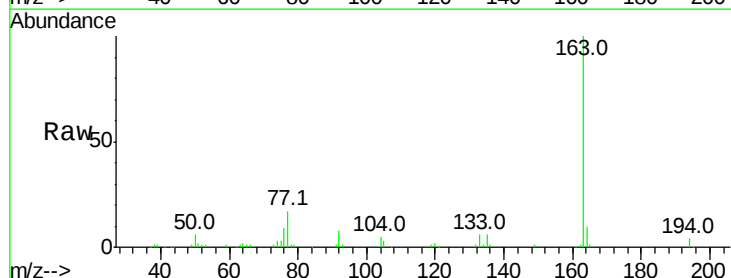

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

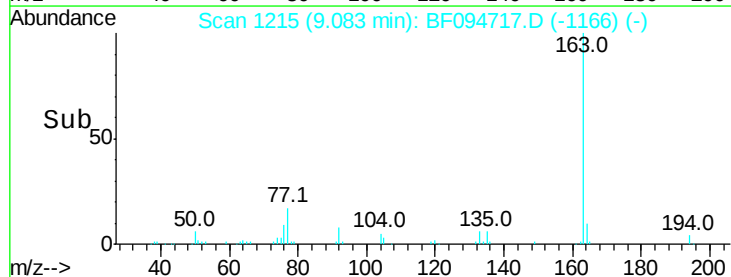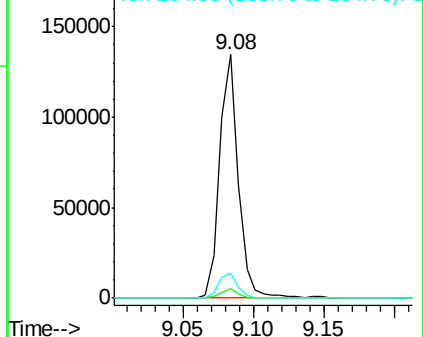




#56
 2,4-Dinitrotoluene
 Concen: 6.06 ng
 RT: 9.39 min Scan# 1267
 Delta R.T. -0.27 min
 Lab File: BF094717.D
 Acq: 30 Apr 2017 16:26

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
165	100		
63	1.7	25.4	38.0#
89	1.7	46.4	69.6#
182	0.0	1.8	2.6#



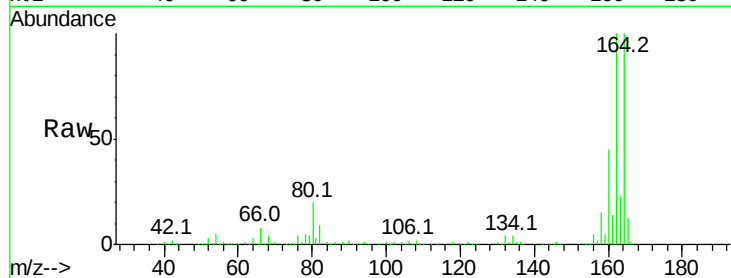


Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF0


Ion 89.00 (88.70 to 89.70): BF0

Ion 182.00 (181.70 to 182.70): E

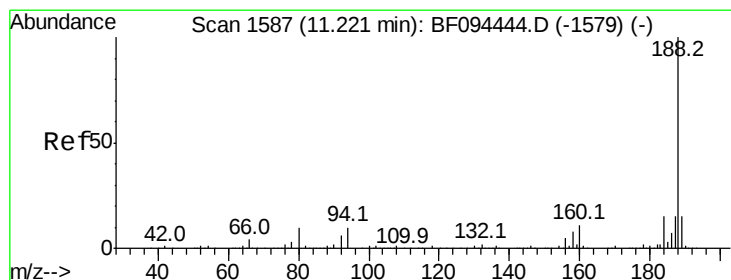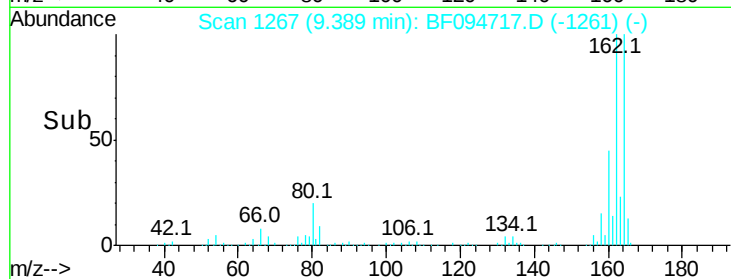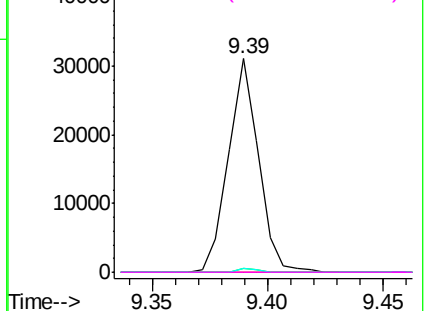

#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 11.21 min Scan# 1577
 Delta R.T. -0.01 min
 Lab File: BF094717.D
 Acq: 30 Apr 2017 16:26



Tgt Ion	Ratio	Lower	Upper
188	100		
94	10.2	9.4	14.2
80	10.8	10.2	15.2

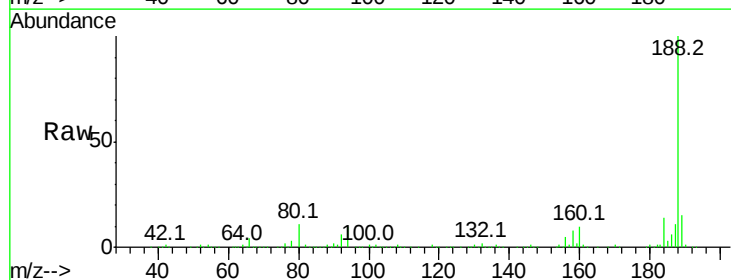


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

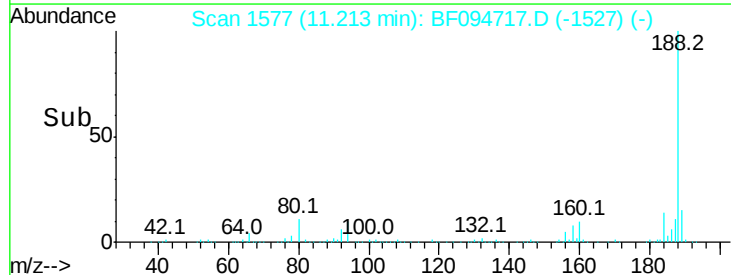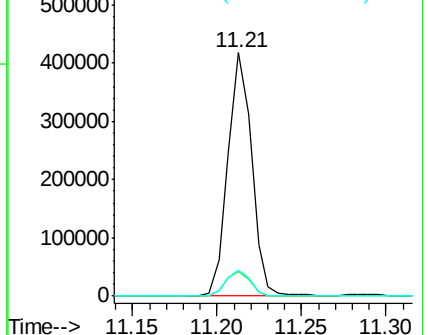

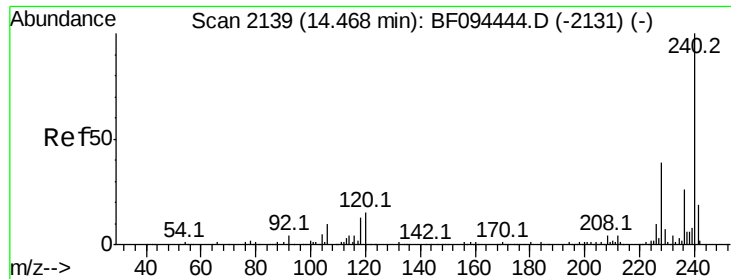

#75

Chrysene-d12

Concen: 20.00 ng

RT: 14.47 min Scan# 2130

Delta R.T. -0.00 min

Lab File: BF094717.D

Acq: 30 Apr 2017 16:26

Instrument :

BNA_F

ClientSampleId :


Tot Ion:240 Resp: 311727

Ion Ratio Lower Upper

240 100

120 14.1 5.8 8.8#




236 26.1 20.5 30.7

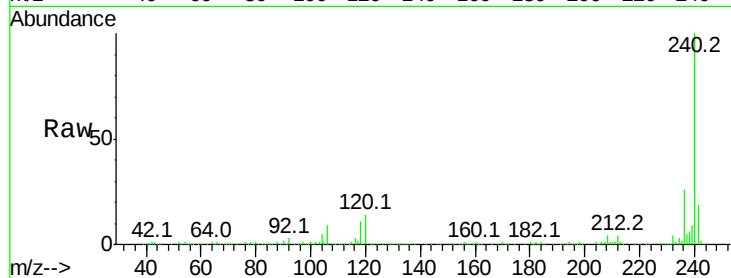

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

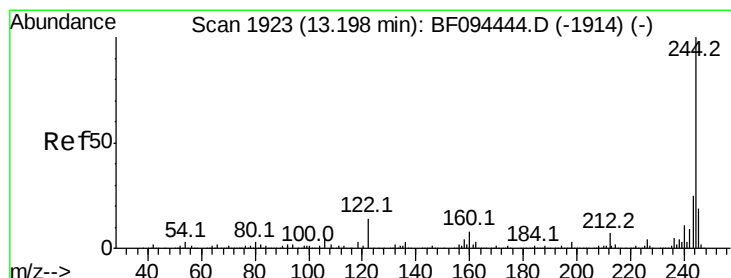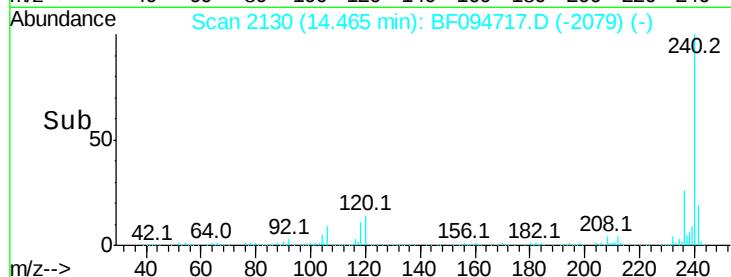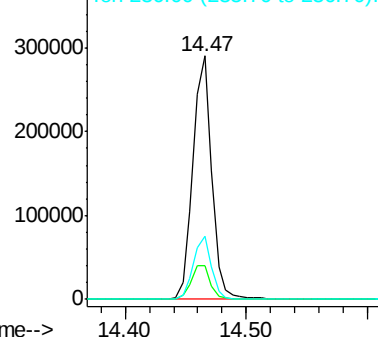

#78

Terphenyl-d14

Concen: 98.25 ng

RT: 13.19 min Scan# 1914

Delta R.T. -0.00 min

Lab File: BF094717.D

Acq: 30 Apr 2017 16:26


Tgt Ion:244 Resp: 1145827

Ion Ratio Lower Upper

244 100

212 7.2 6.0 9.0



122 14.0 10.3 15.5

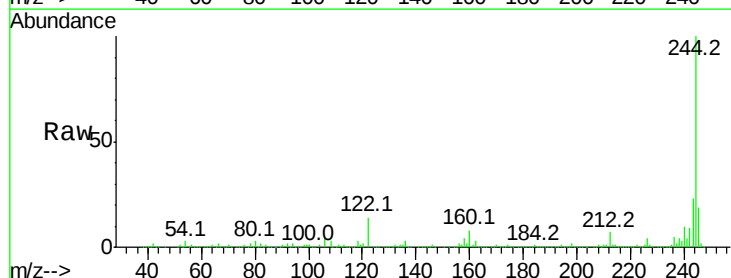


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

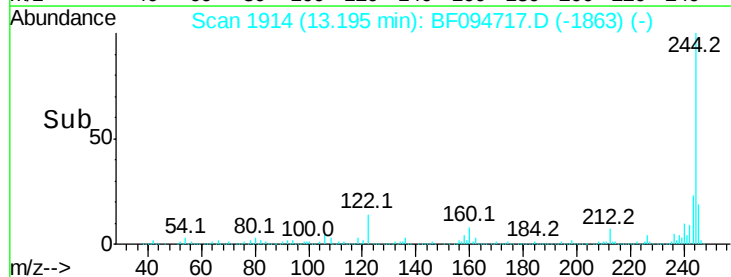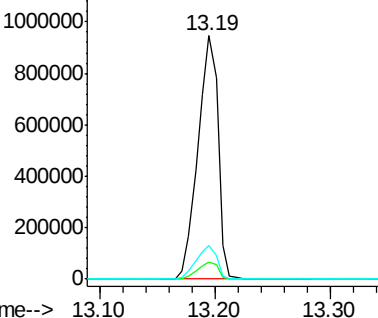


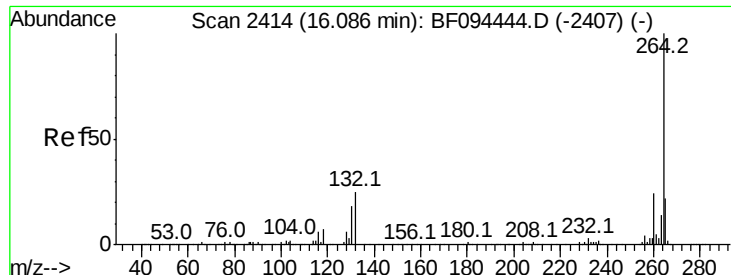

#86
Pervlene-d12
Concen: 20.00 ng
RT: 16.09 min Scan# 2407
Delta R.T. 0.01 min
Lab File: BF094717.D
Acq: 30 Apr 2017 16:26

Instrument :
BNA_F
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.3	19.5	29.3
265	21.2	17.2	25.8

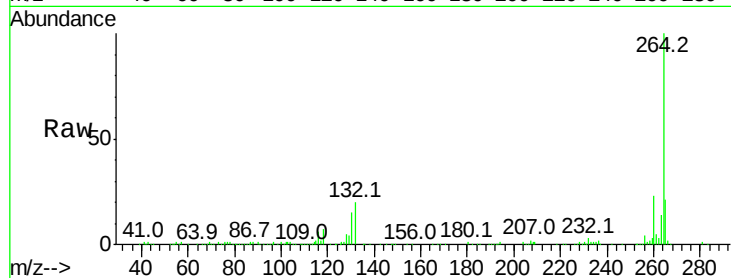

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

