
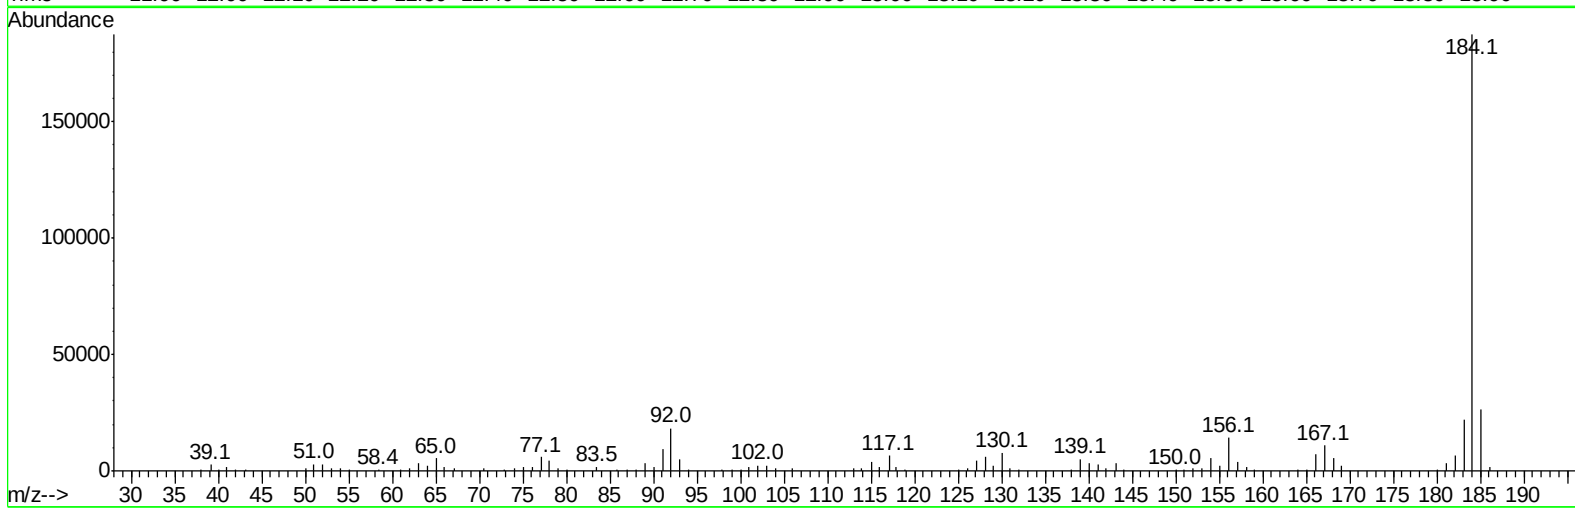


Data Path : Z:\HPCHEM1\BNA F\DATA\BF043017\
Data File : BF094733.D
Acq On : 1 May 2017 00:36
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 01 07:37:56 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF041717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 17 14:59:23 2017
Response via : Initial Calibration

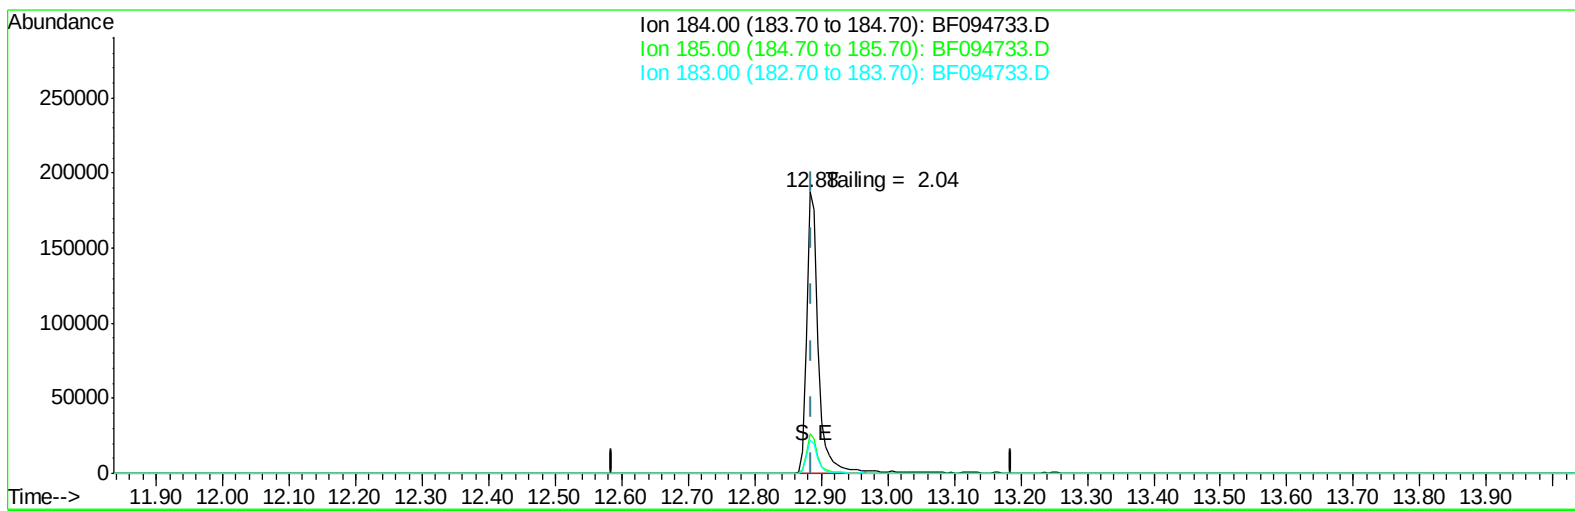

TIC: BF094733.D

(76) Benzidine



12.883min (-0.003) 0.00ng

response 233921

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.19#
183.00	12.20	11.67
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF043017\
Data File : BF094733.D
Acq On : 1 May 2017 00:36
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 01 07:37:56 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF041717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 17 14:59:23 2017
Response via : Initial Calibration

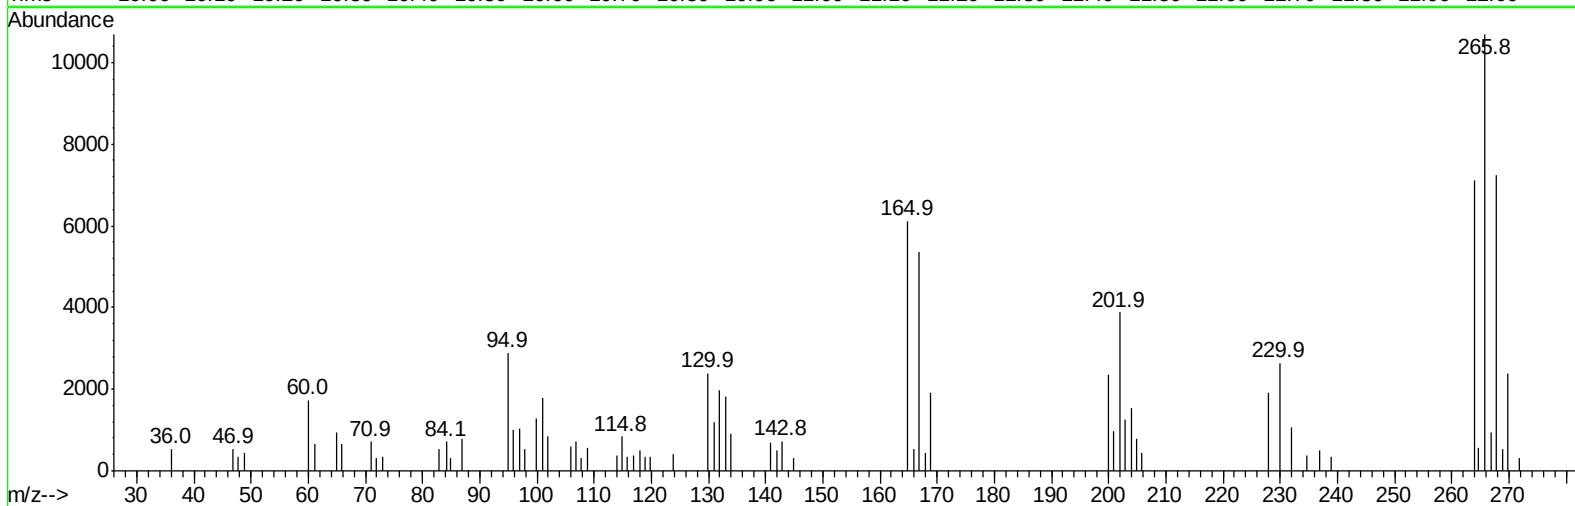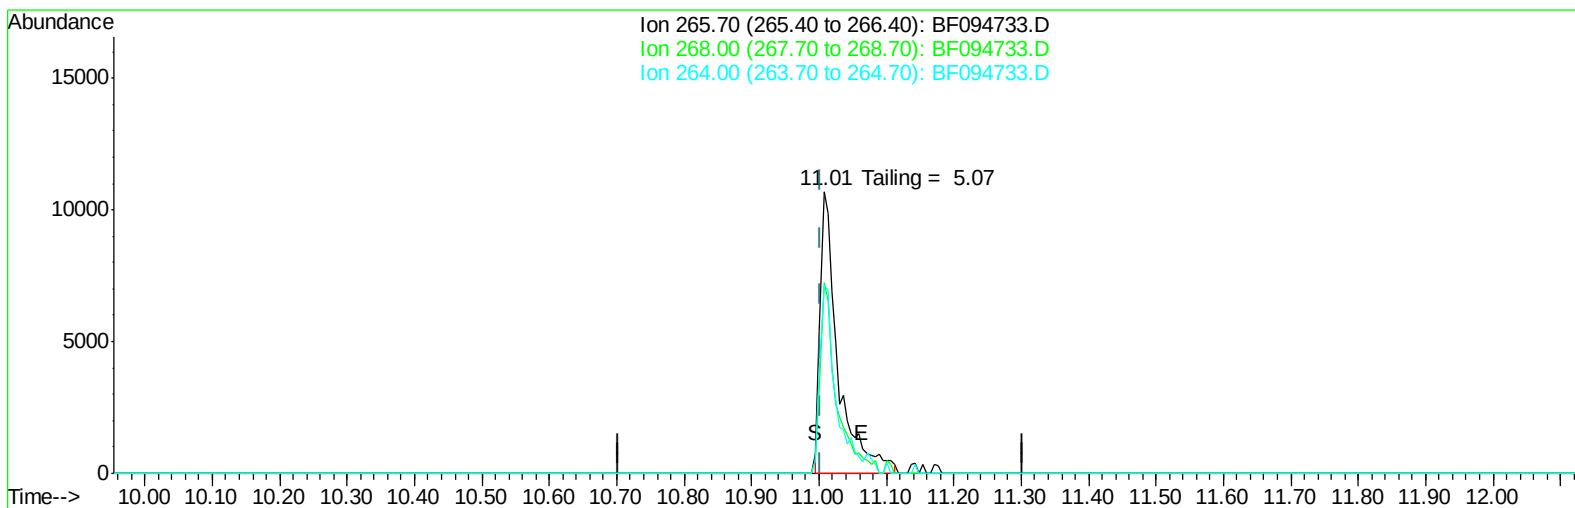

TIC: BF094733.D

(69) Pentachlorophenol (C)

11.007min (+0.003) 0.00ng

response 19771

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	67.81
264.00	64.60	72.10
0.00	0.00	0.00