


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF043017\
 Data File : BF094706.D
 Acq On : 30 Apr 2017 11:22
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF041717.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 17 14:59:23 2017

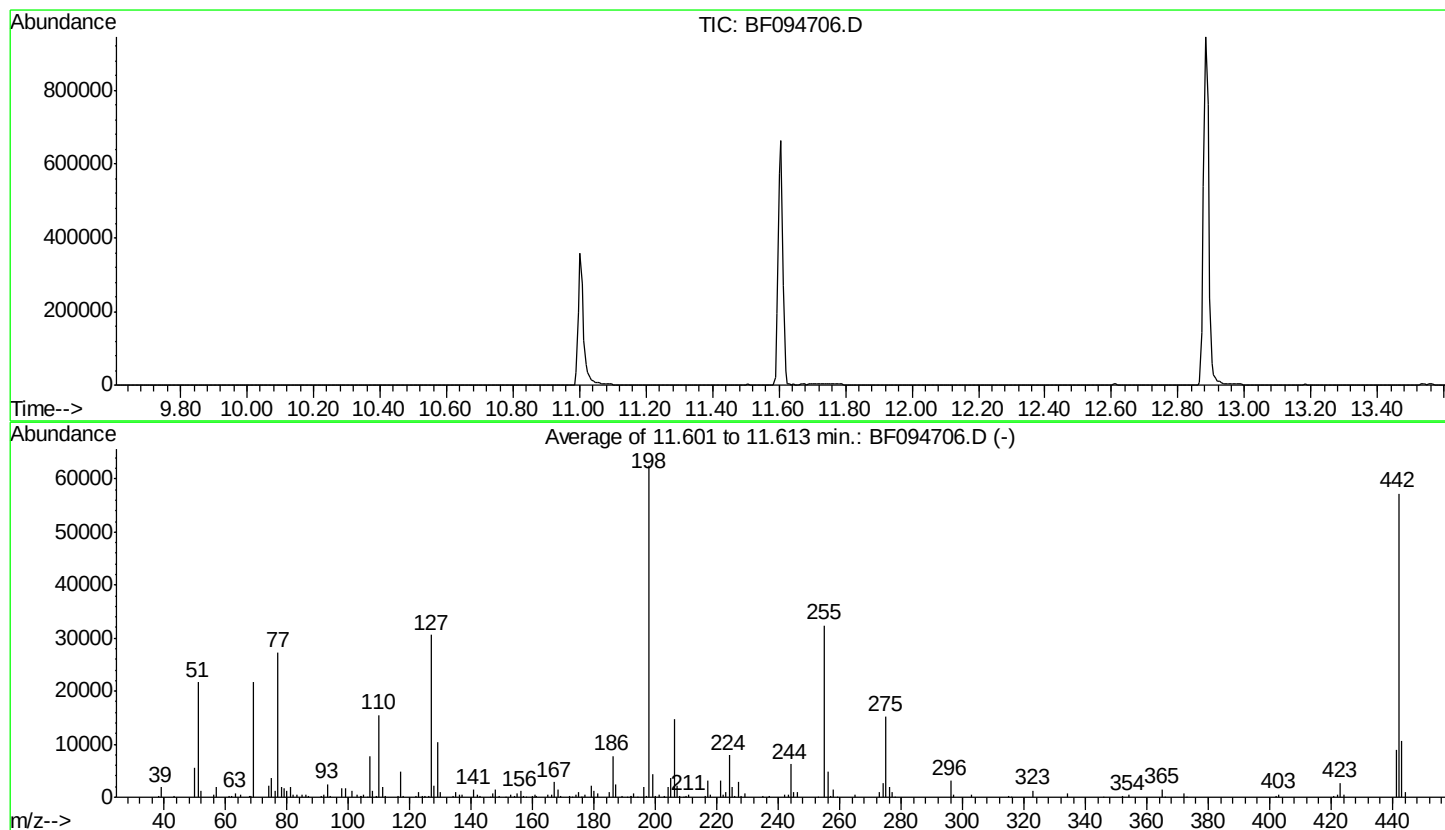

AutoFind: Scans 1643, 1644, 1645; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.7	21699	PASS
68	69	0.00	2	1.5	333	PASS
69	198	0.00	100	34.7	21671	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.9	30561	PASS
197	198	0.00	2	0.5	297	PASS
198	198	100	100	100.0	62512	PASS
199	198	5	9	7.1	4414	PASS
275	198	10	60	24.2	15150	PASS
365	198	1	100	2.3	1467	PASS
441	442	0.01	24	15.8	9035	PASS
442	198	50	100	91.6	57288	PASS
443	442	15	24	18.8	10747	PASS