
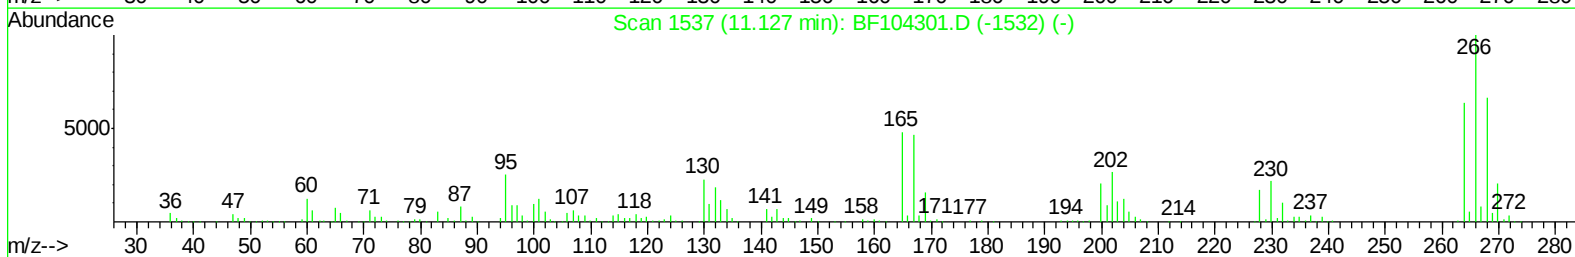
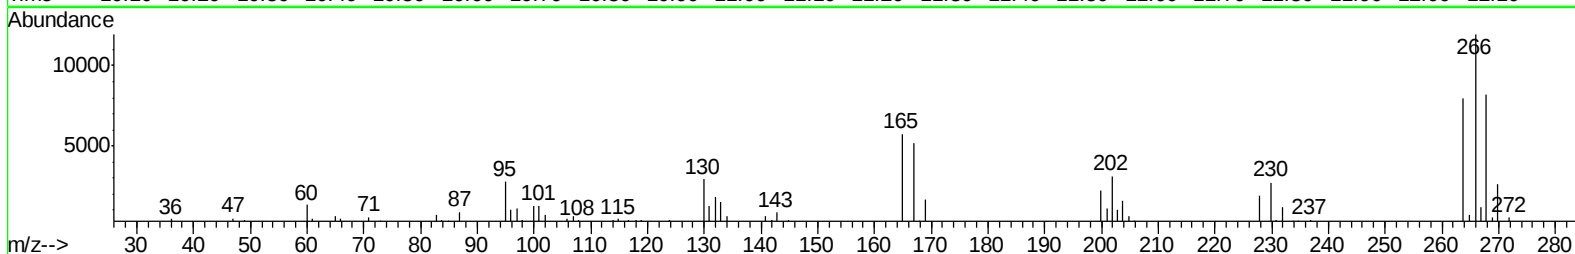


Data Path : Z:\HPCHEM1\BNA F\Data\BF043018\
Data File : BF104953.D
Acq On : 1 May 2018 1:13
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 01 09:05:20 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 30 15:20:08 2018
Response via : Initial Calibration

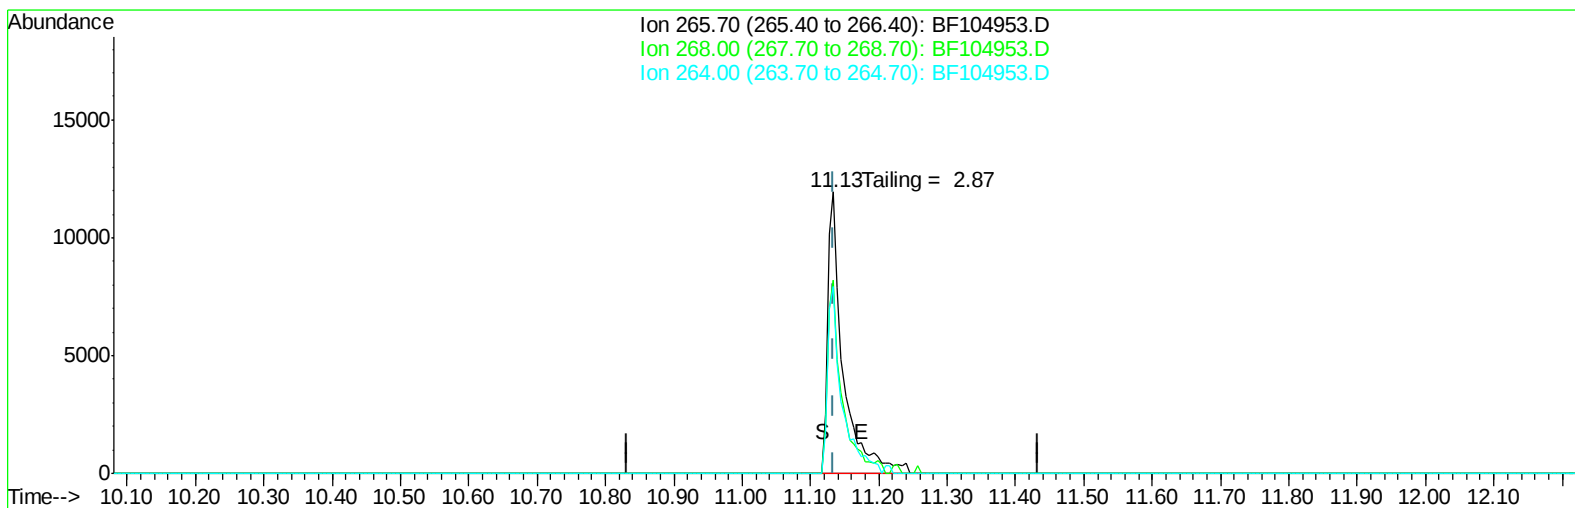

TIC: BF104953.D

(69) Pentachlorophenol (C)




11.133min (+0.000) 19232.82ng

response 18513

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	68.46
264.00	61.90	66.42
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF043018\
 Data File : BF104953.D
 Acq On : 1 May 2018 1:13
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 01 09:05:20 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 30 15:20:08 2018
 Response via : Initial Calibration

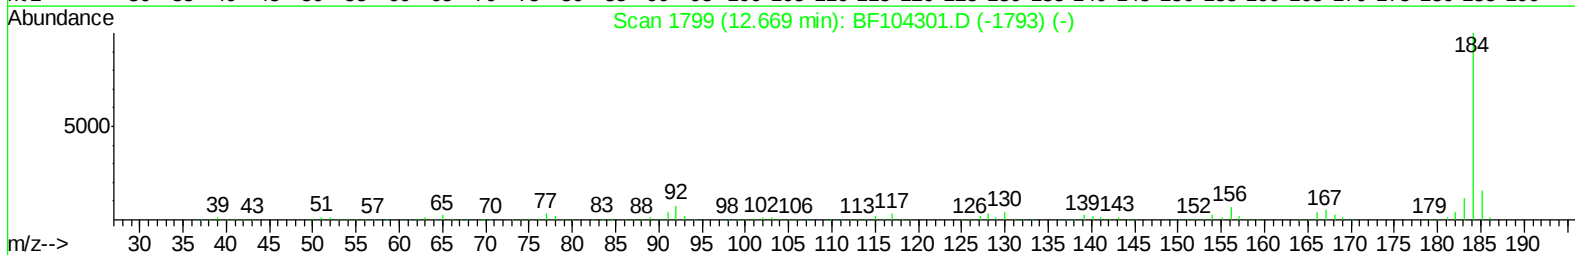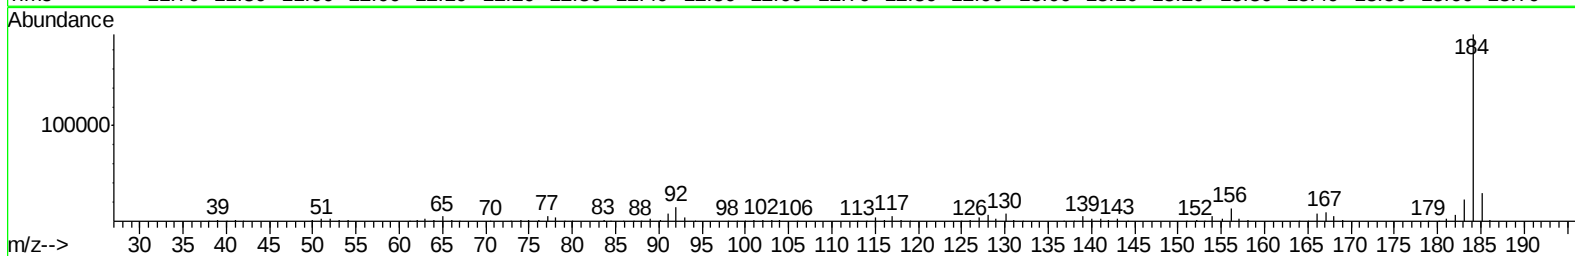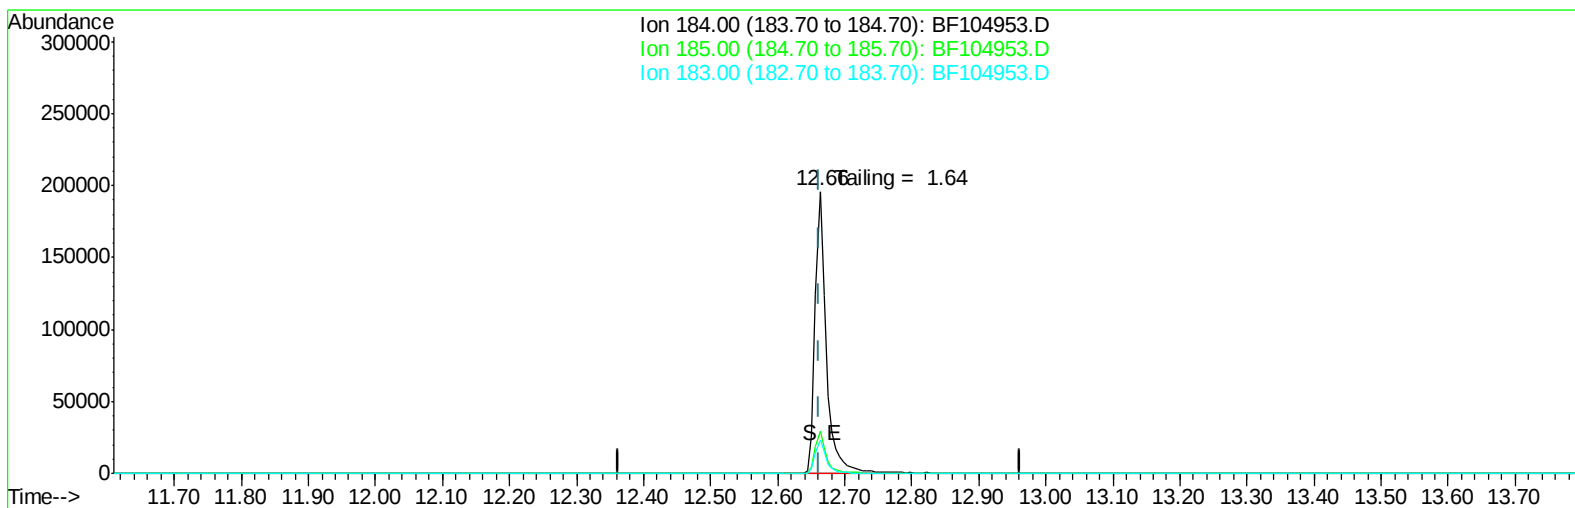

TIC: BF104953.D

(76) Benzidine

12.663min (+0.000) 0.00ng

response 218674

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.04
183.00	11.60	11.74
0.00	0.00	0.00