


Data Path : Z:\HPCHEM1\BNA F\Data\BF043018\
 Data File : BF104953.D
 Acq On : 1 May 2018 1:13
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 30 15:20:08 2018

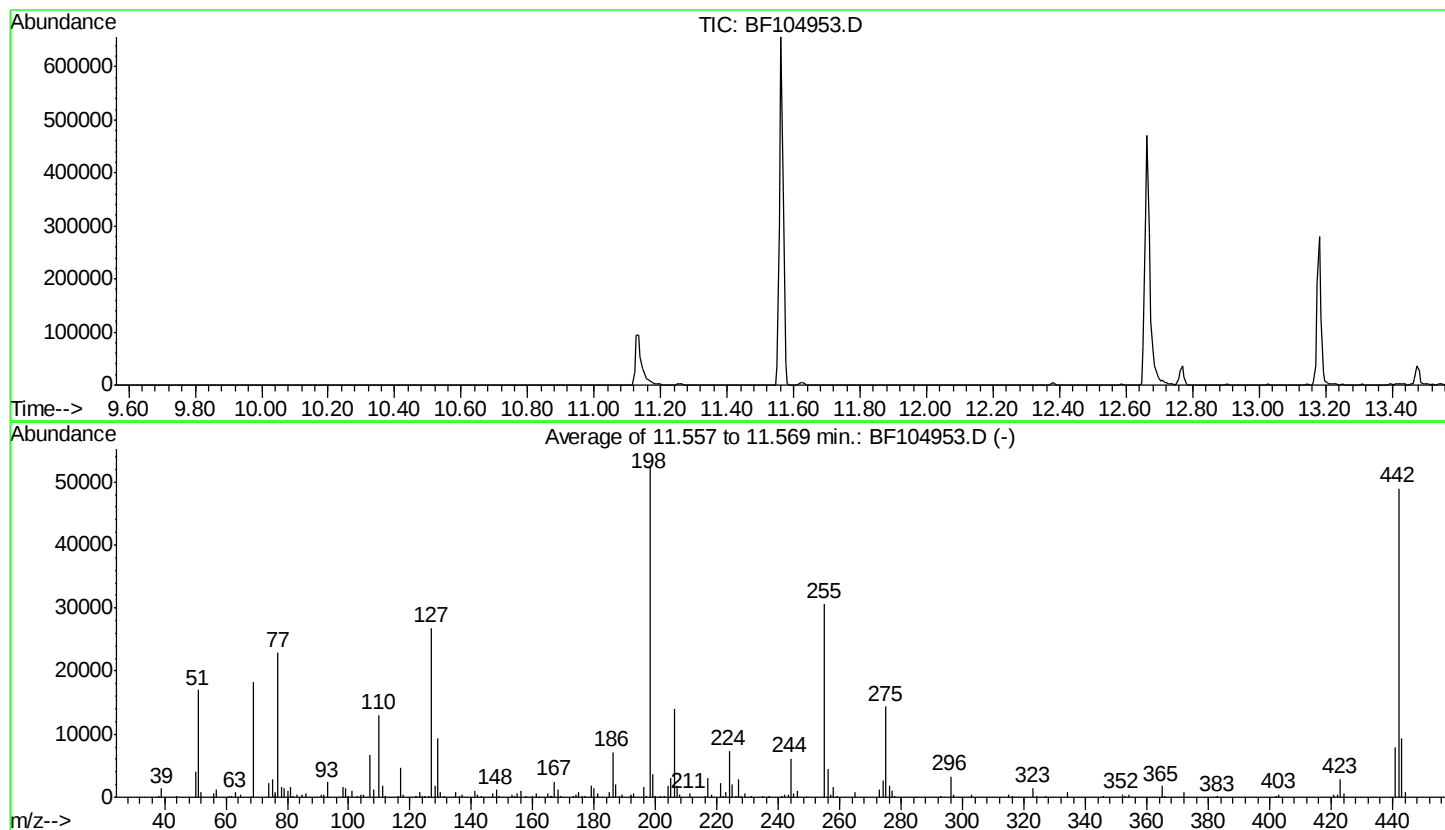

AutoFind: Scans 1610, 1611, 1612; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.3	16973	PASS
68	69	0.00	2	0.6	107	PASS
69	198	0.00	100	34.6	18184	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.1	26874	PASS
197	198	0.00	2	0.3	146	PASS
198	198	100	100	100.0	52578	PASS
199	198	5	9	6.8	3568	PASS
275	198	10	60	27.3	14350	PASS
365	198	1	100	3.3	1757	PASS
441	443	0.01	100	84.3	7875	PASS
442	198	50	100	93.2	48989	PASS
443	442	15	24	19.1	9346	PASS