


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF043019\
 Data File : BF114036.D
 Acq On : 30 Apr 2019 12:28
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 23 03:32:35 2019

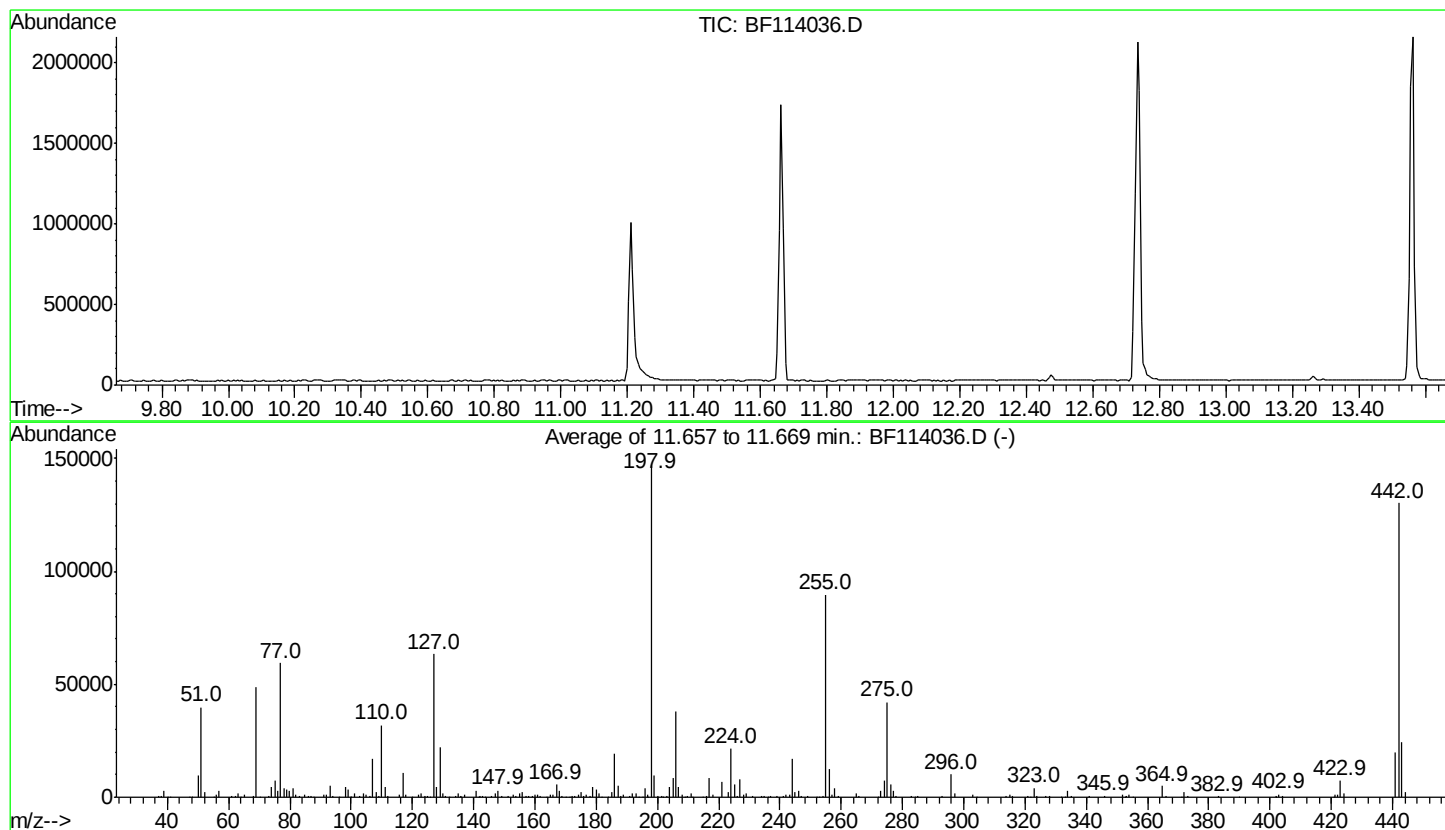

AutoFind: Scans 1627, 1628, 1629; Background Corrected with Scan 1622

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.1	39744	PASS
68	69	0.00	2	1.6	781	PASS
69	198	0.00	100	33.0	48466	PASS
70	69	0.00	2	0.5	247	PASS
127	198	10	80	43.2	63357	PASS
197	198	0.00	2	0.6	921	PASS
198	198	100	100	100.0	146752	PASS
199	198	5	9	6.7	9761	PASS
275	198	10	60	28.7	42152	PASS
365	198	1	100	3.3	4842	PASS
441	198	0.01	100	13.7	20102	PASS
442	198	50	100	88.7	130229	PASS
443	442	15	24	18.7	24339	PASS