
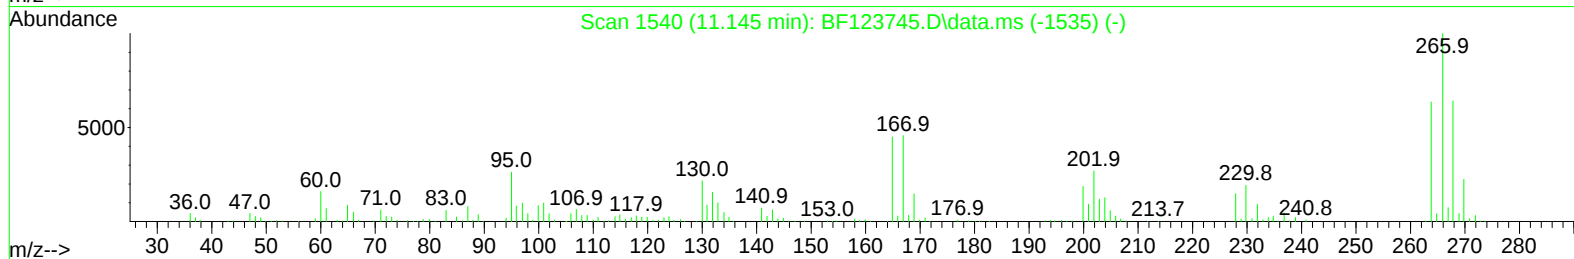
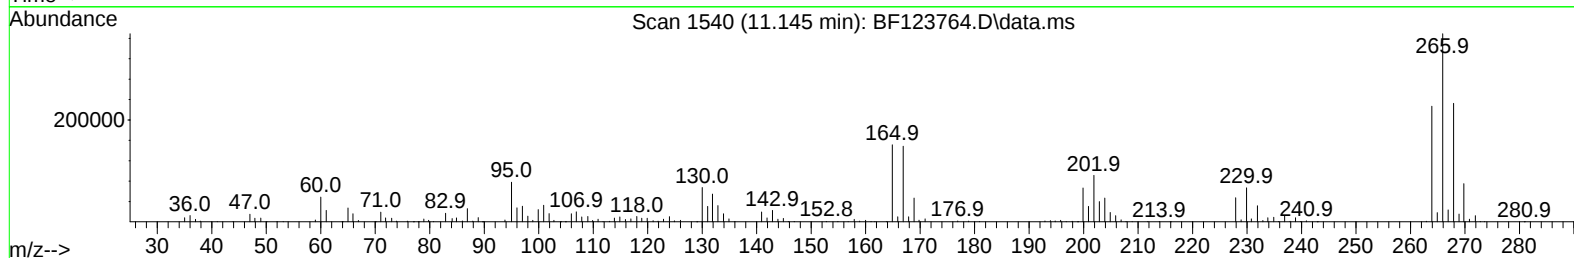


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF043021\
Data File : BF123764.D
Acq On : 30 Apr 2021 8:12
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 30 12:23:05 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 27 16:30:39 2021
Response via : Initial Calibration

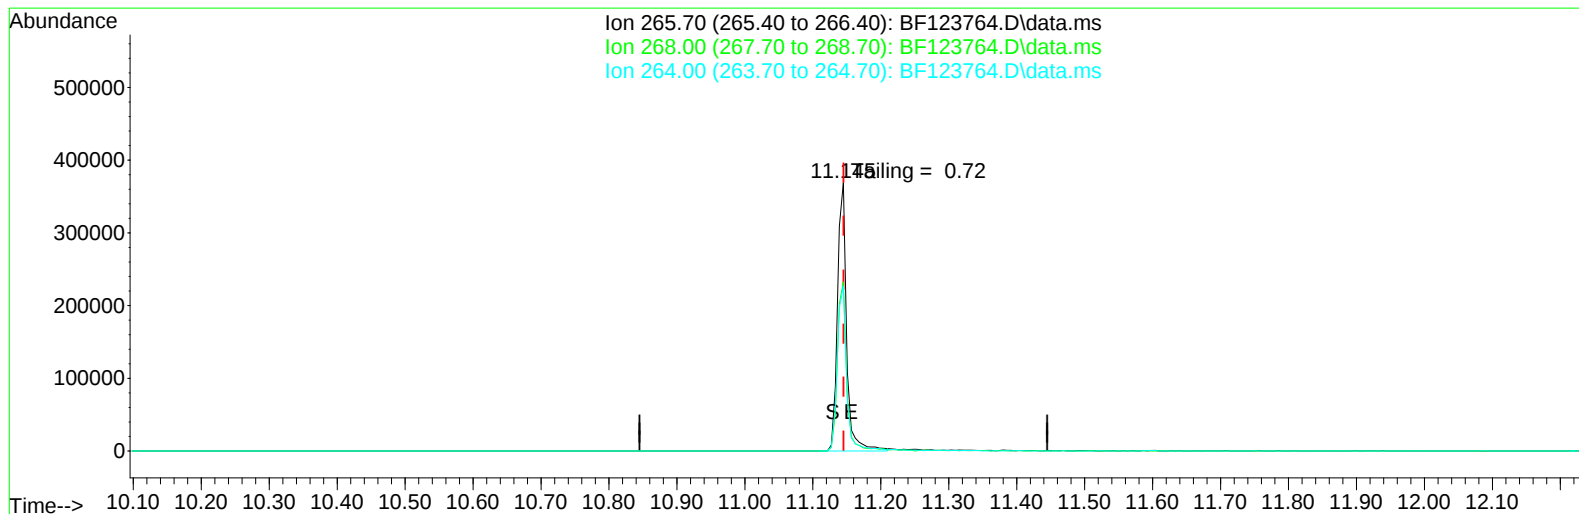

TIC: BF123764.D\data.ms

(70) Pentachlorophenol (C)




11.145min (-0.000) 360380.36 ng

response 347845

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	62.98
264.00	65.70	61.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF043021\
Data File : BF123764.D
Acq On : 30 Apr 2021 8:12
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 30 12:23:05 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 27 16:30:39 2021
Response via : Initial Calibration

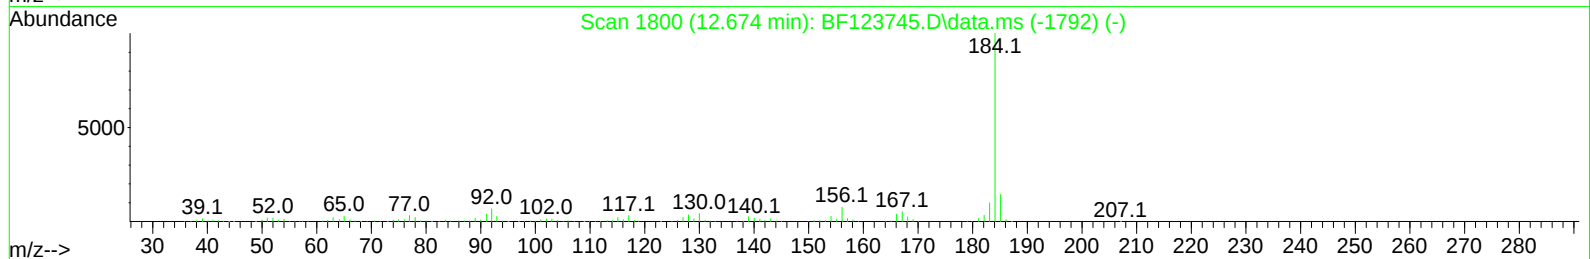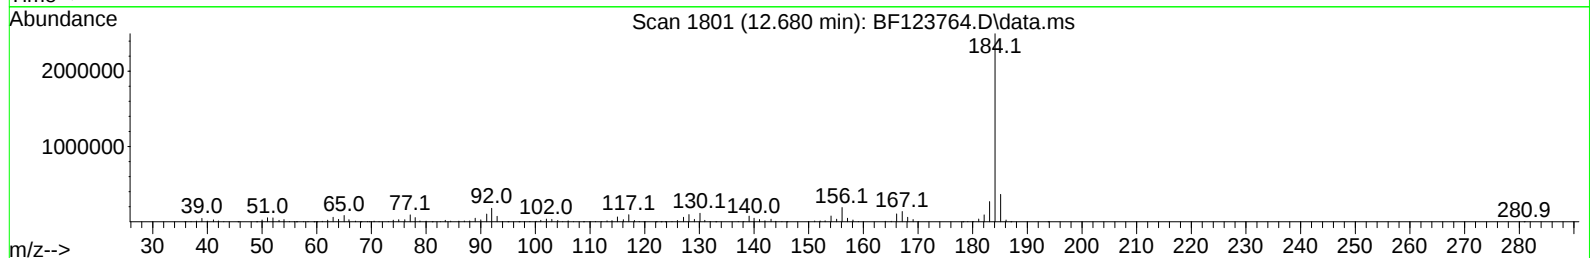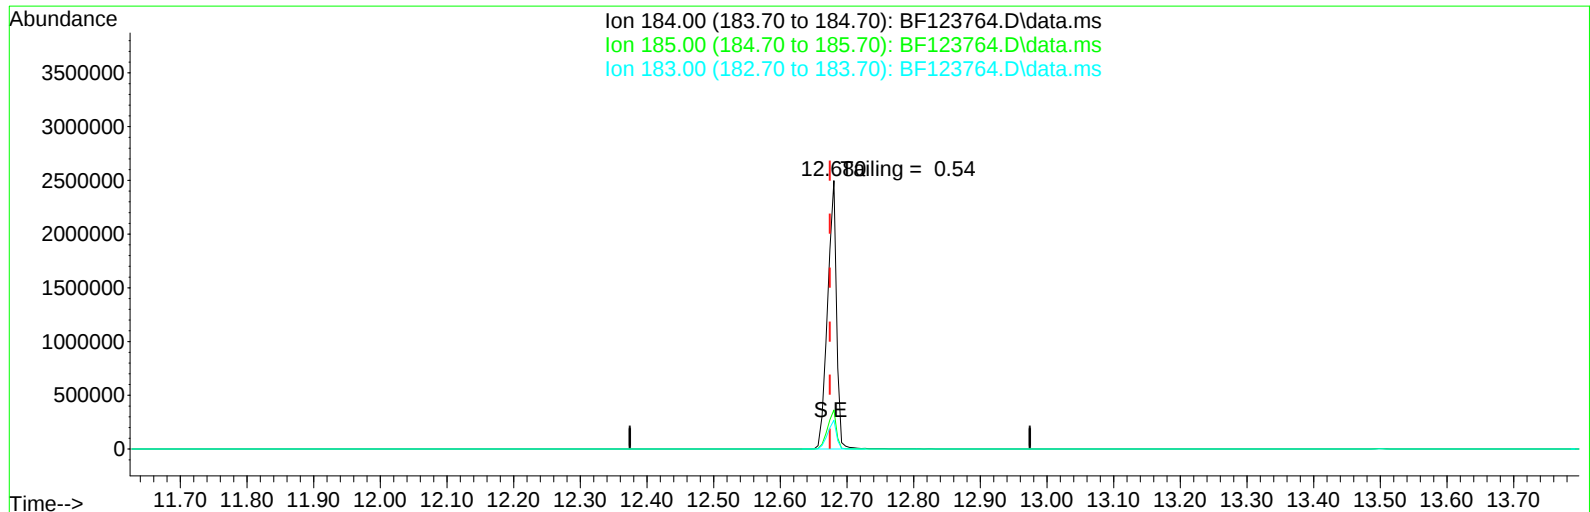

TIC: BF123764.D\data.ms

(77) Benzidine**12.680min (+ 0.006) 78681.71 ng****response 2328919**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.59
183.00	9.80	10.78
0.00	0.00	0.00