

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF043021\
 Data File : BF123769.D
 Acq On : 30 Apr 2021 14:16
 Operator : JU/CG
 Sample : PB136095BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB136095BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF123769.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.434	565	569	572	rBV	8849626	8737173	90.30%	14.097%
2	6.445	735	741	744	rBV	8196395	8705369	89.97%	14.045%
3	6.804	799	802	806	rBV	2099339	1711536	17.69%	2.761%
4	7.369	893	898	901	rBV	5270910	5893401	60.91%	9.508%
5	8.092	1016	1021	1024	rBV	2425672	2227266	23.02%	3.593%
6	9.169	1199	1204	1207	rBV	8928804	8973604	92.74%	14.478%
7	9.845	1314	1319	1323	rBV	2663547	2359463	24.38%	3.807%
8	10.639	1448	1454	1457	rBV	6418084	5803695	59.98%	9.364%
9	11.333	1568	1572	1575	rBV	3013460	2473795	25.57%	3.991%
10	12.751	1809	1813	1816	rBV	114461	101215	1.05%	0.163%
11	12.927	1838	1843	1846	rBV	9336183	9676014	100.00%	15.611%
12	13.457	1929	1933	1937	rBV	134914	111091	1.15%	0.179%
13	13.980	2017	2022	2025	rBV	2396862	2298277	23.75%	3.708%
14	15.092	2208	2211	2217	rVB	111720	125555	1.30%	0.203%
15	15.433	2264	2269	2273	rBV	1650236	2076428	21.46%	3.350%
16	15.474	2273	2276	2285	rVB	169513	217476	2.25%	0.351%
17	15.904	2344	2349	2355	rBV	133626	195296	2.02%	0.315%
18	16.404	2428	2434	2441	rBV2	103612	180338	1.86%	0.291%
19	16.992	2527	2534	2543	rBV4	54903	113559	1.17%	0.183%




Sum of corrected areas: 61980551

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF043021\
Data File : BF123769.D
Acq On : 30 Apr 2021 14:16
Operator : JU/CG
Sample : PB136095BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB136095BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

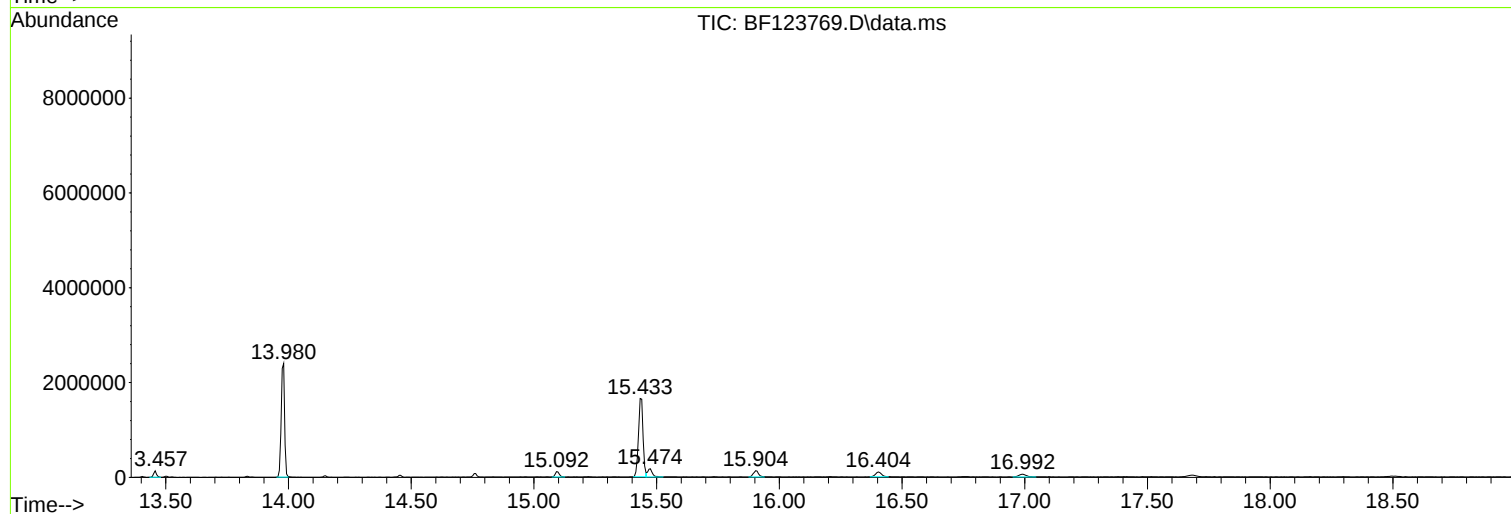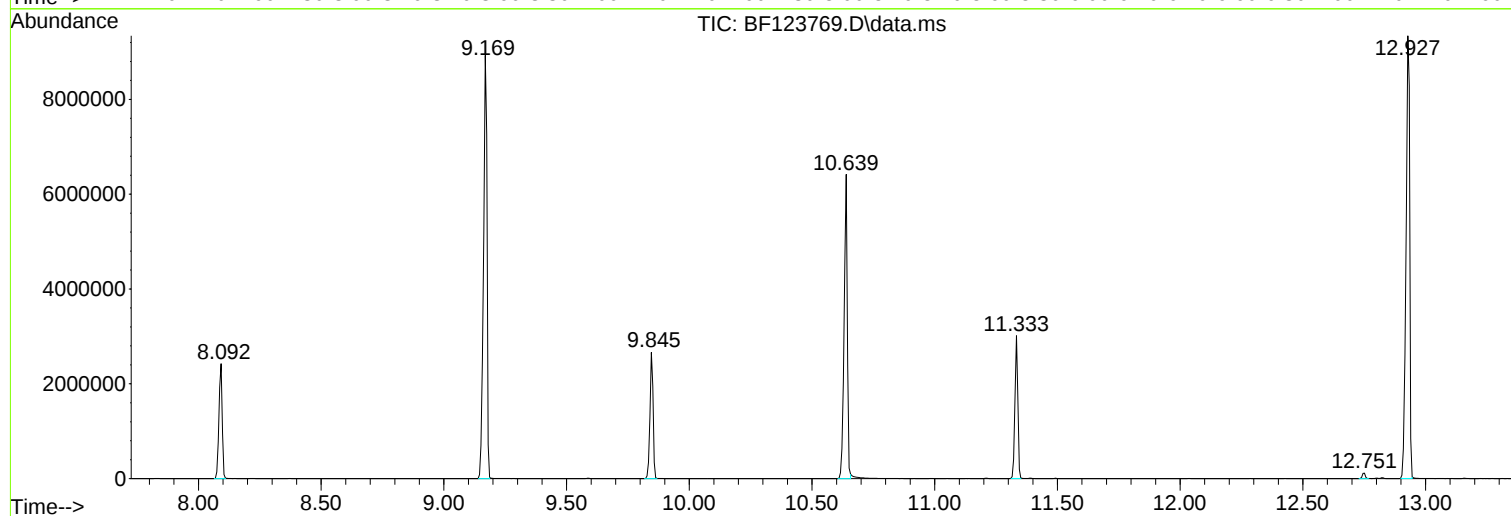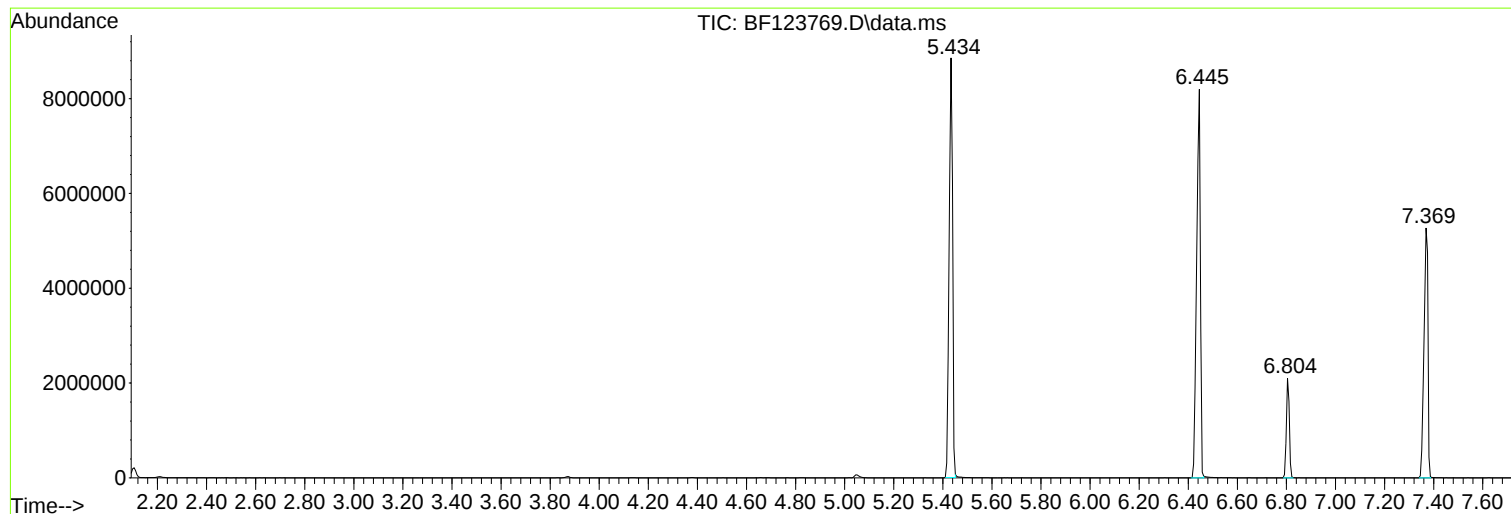

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF043021\
Data File : BF123769.D
Acq On : 30 Apr 2021 14:16
Operator : JU/CG
Sample : PB136095BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB136095BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF043021\
Data File : BF123769.D
Acq On : 30 Apr 2021 14:16
Operator : JU/CG
Sample : PB136095BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB136095BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------