
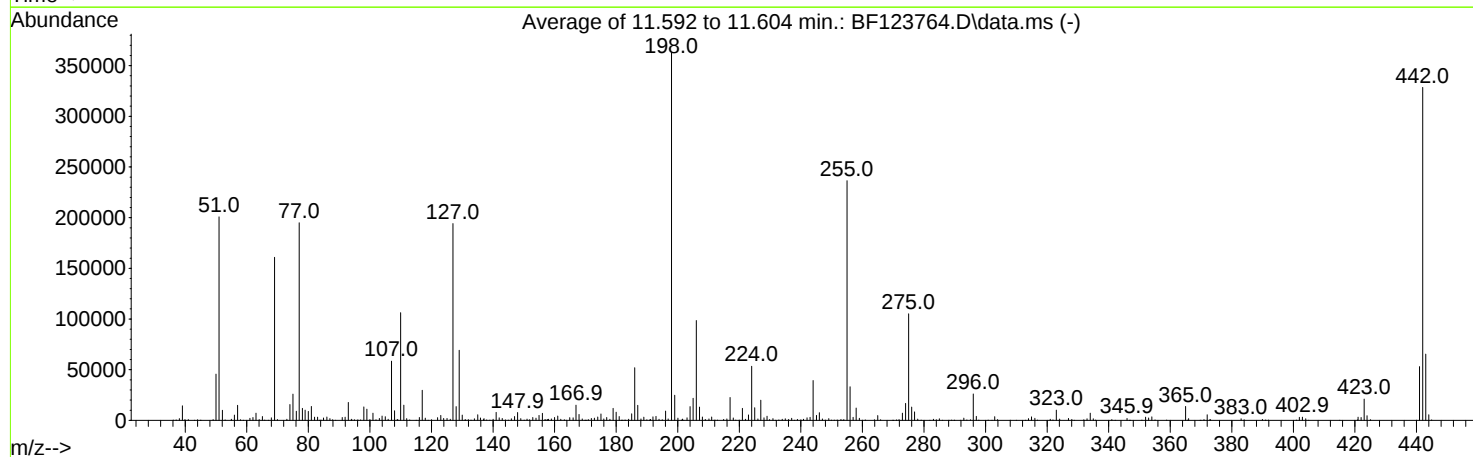


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF043021\
 Data File : BF123764.D
 Acq On : 30 Apr 2021 8:12
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 27 16:30:39 2021

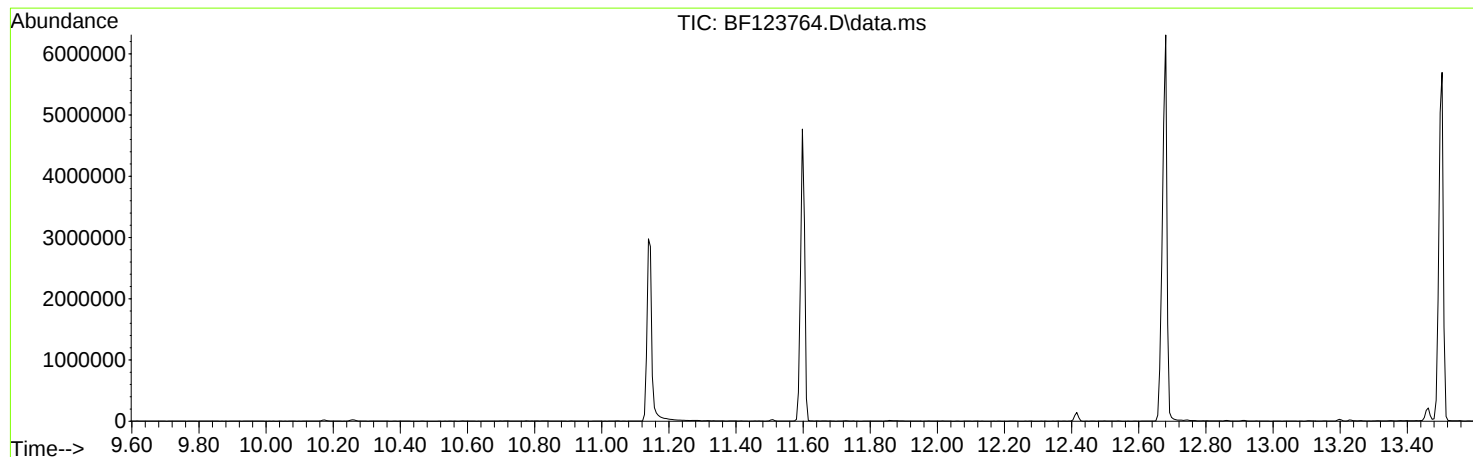

AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1611

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.3	200885	PASS
68	69	0.00	2	1.6	2577	PASS
69	198	0.00	100	44.3	160811	PASS
70	69	0.00	2	0.5	790	PASS
127	198	10	80	53.5	194240	PASS
197	198	0.00	2	0.4	1465	PASS
198	198	100	100	100.0	362965	PASS
199	198	5	9	6.8	24776	PASS
275	198	10	60	29.0	105227	PASS
365	198	1	100	3.8	13677	PASS
441	198	0.01	100	14.6	53125	PASS
442	442	50	100	100.0	328475	PASS
443	442	15	24	19.9	65347	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/30/2021	BNA_F	<u>BF123764.D</u>
Compound Name	Response	Retention Time
DDT	970132	13.5
DDD	6018	13.19
DDE	1766	12.86
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7784	977916	0.80

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF043021\
Data File : BF123764.D
Acq On : 30 Apr 2021 8:12
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 30 12:23:05 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 27 16:30:39 2021
Response via : Initial Calibration

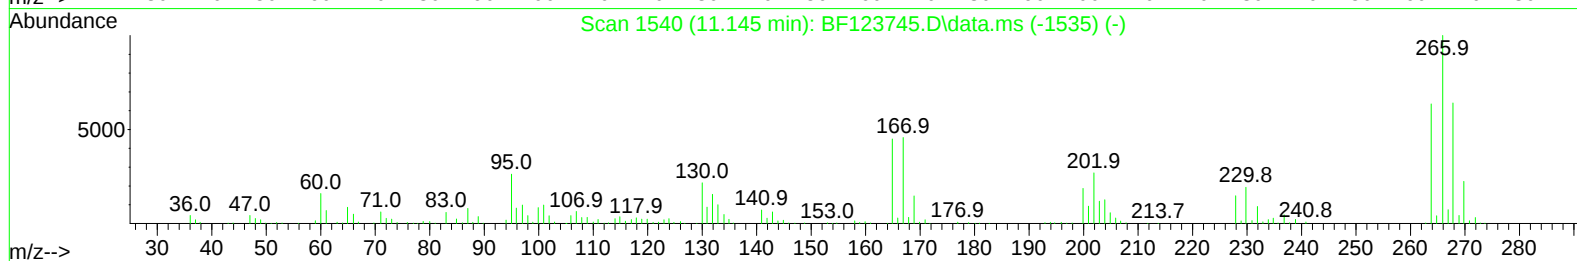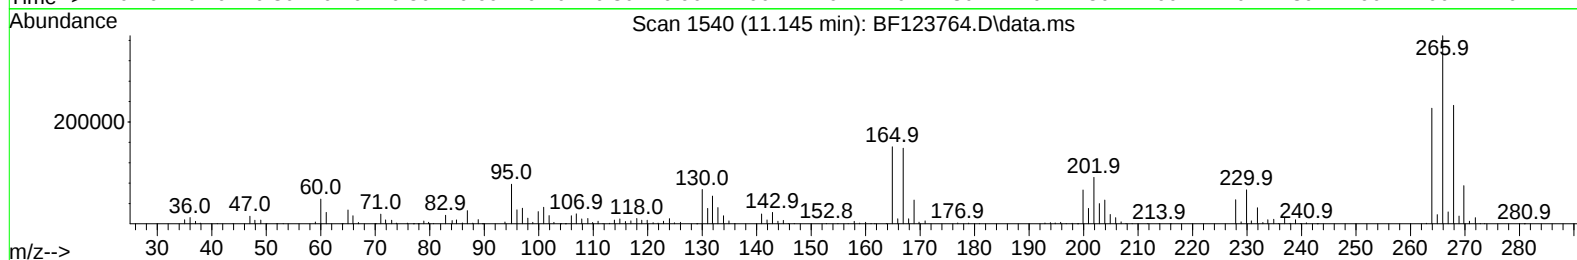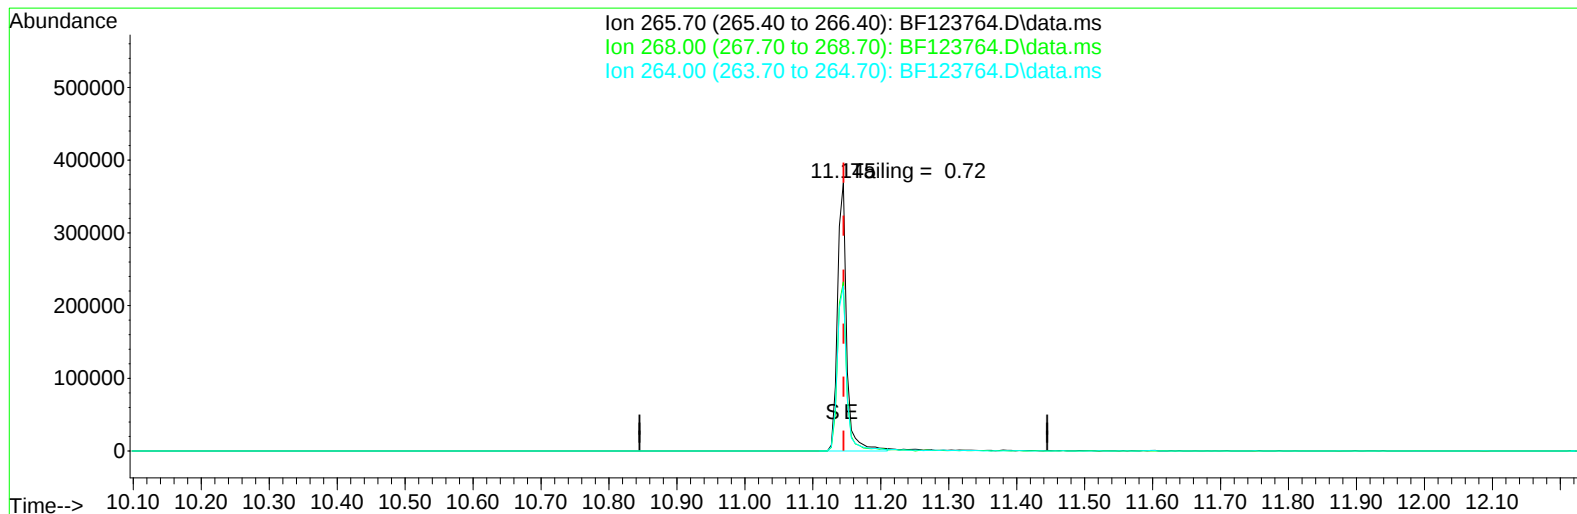

TIC: BF123764.D\data.ms

(70) Pentachlorophenol (C)

11.145min (-0.000) 360380.36 ng




response 347845

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	62.98
264.00	65.70	61.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF043021\
Data File : BF123764.D
Acq On : 30 Apr 2021 8:12
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 30 12:23:05 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 27 16:30:39 2021
Response via : Initial Calibration

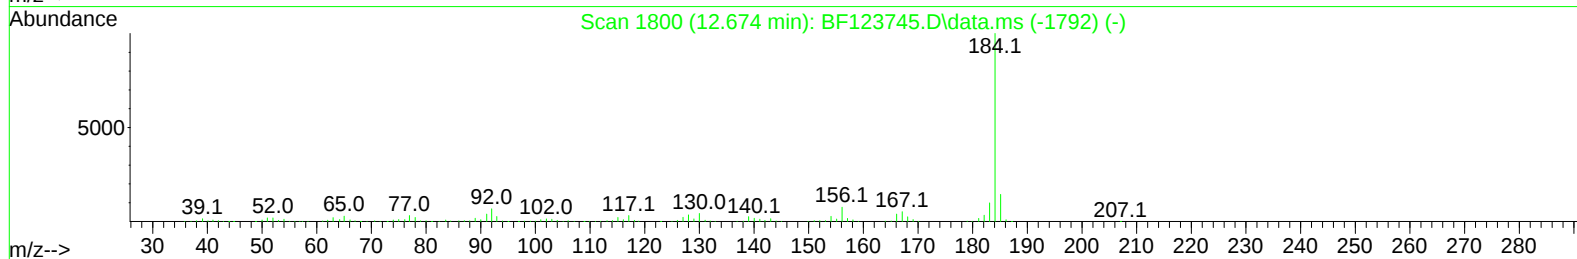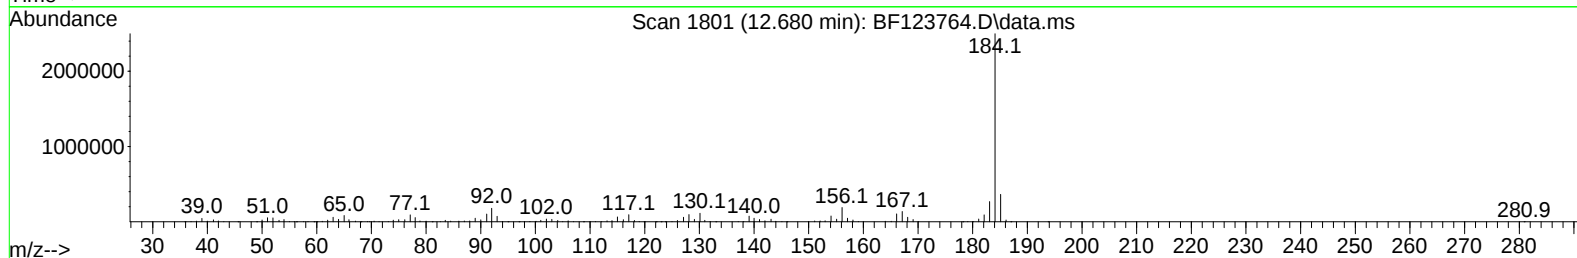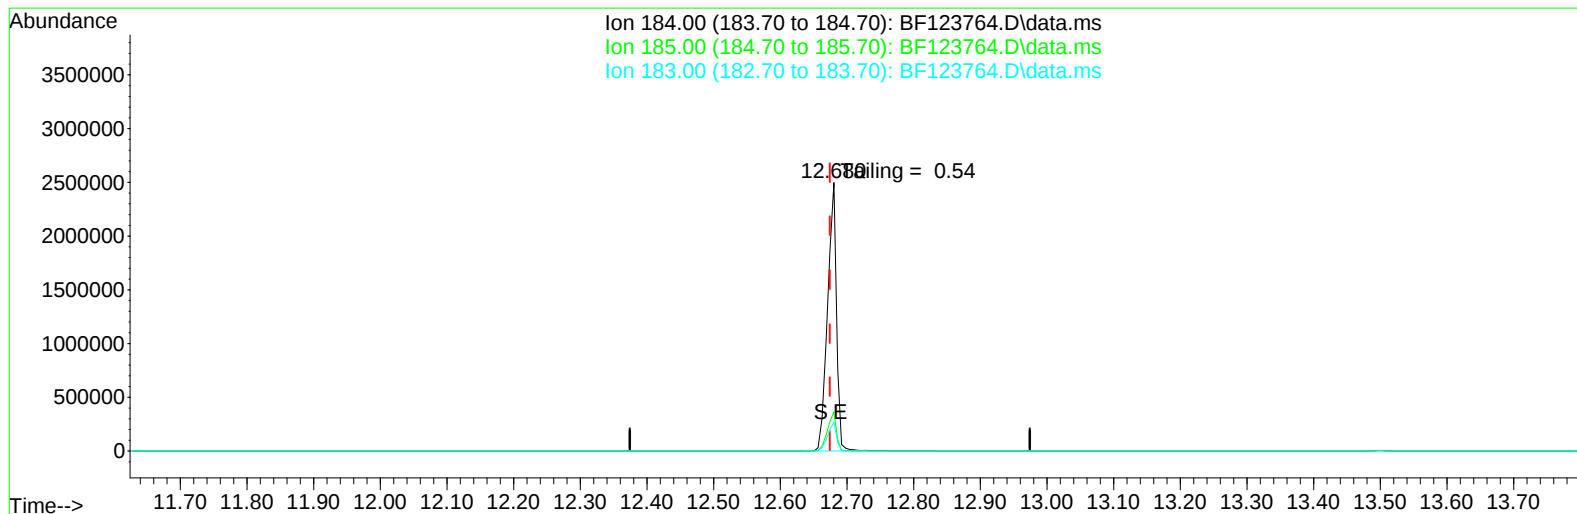

TIC: BF123764.D\data.ms

(77) Benzidine

12.680min (+ 0.006) 78681.71 ng

response 2328919

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.59
183.00	9.80	10.78
0.00	0.00	0.00