
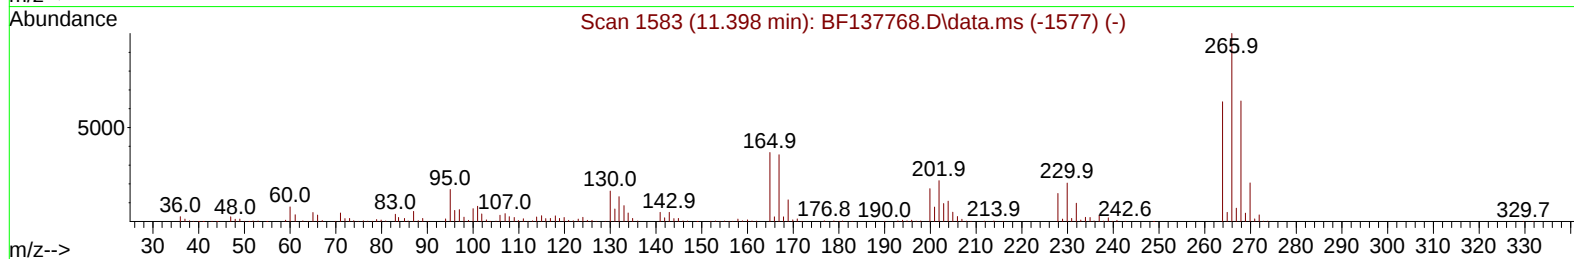
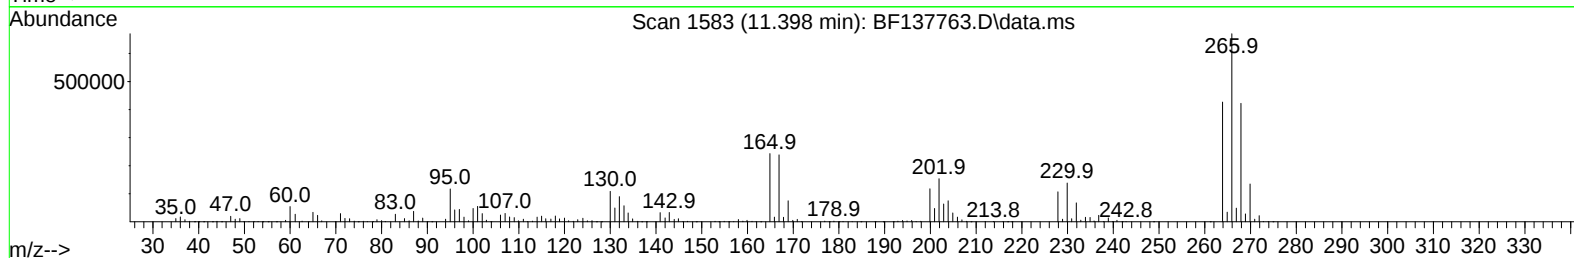


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF043024\
Data File : BF137763.D
Acq On : 30 Apr 2024 10:37
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 02 19:57:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 03:25:08 2024
Response via : Initial Calibration

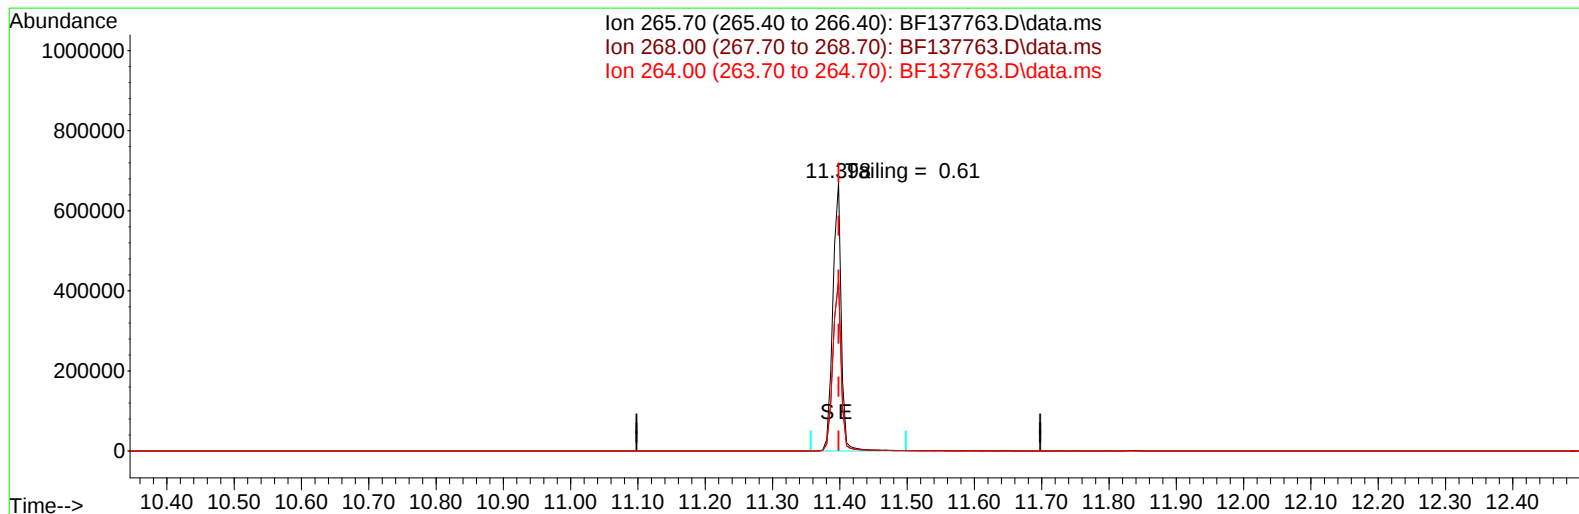

TIC: BF137763.D\data.ms

(70) Pentachlorophenol (C)




11.398min (+ 0.000) 455467.36 ng

response 585142

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.10	62.95
264.00	63.70	63.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF043024\
Data File : BF137763.D
Acq On : 30 Apr 2024 10:37
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 02 19:57:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 03:25:08 2024
Response via : Initial Calibration

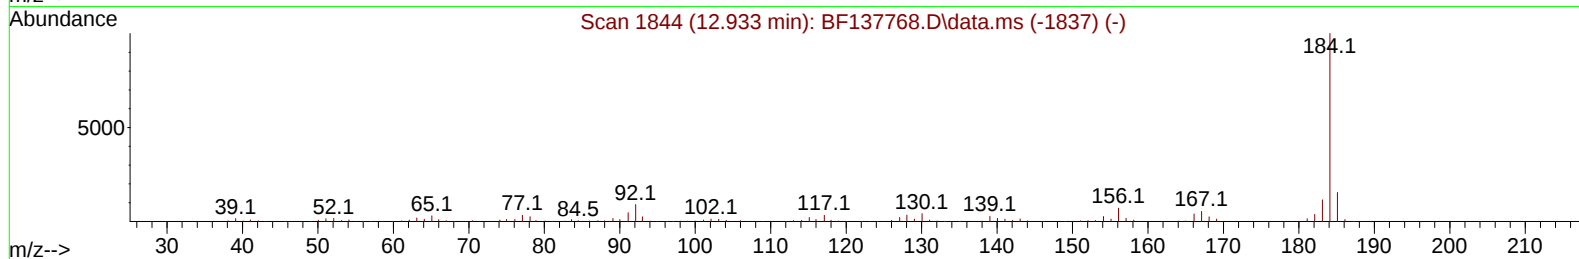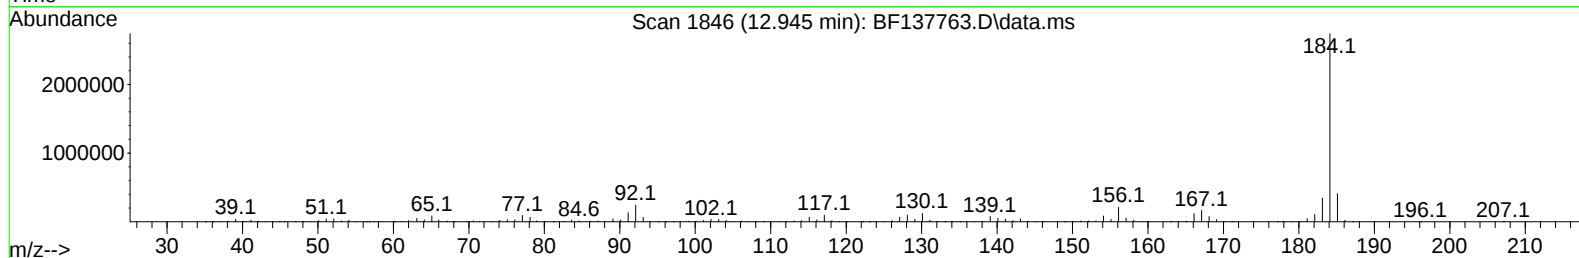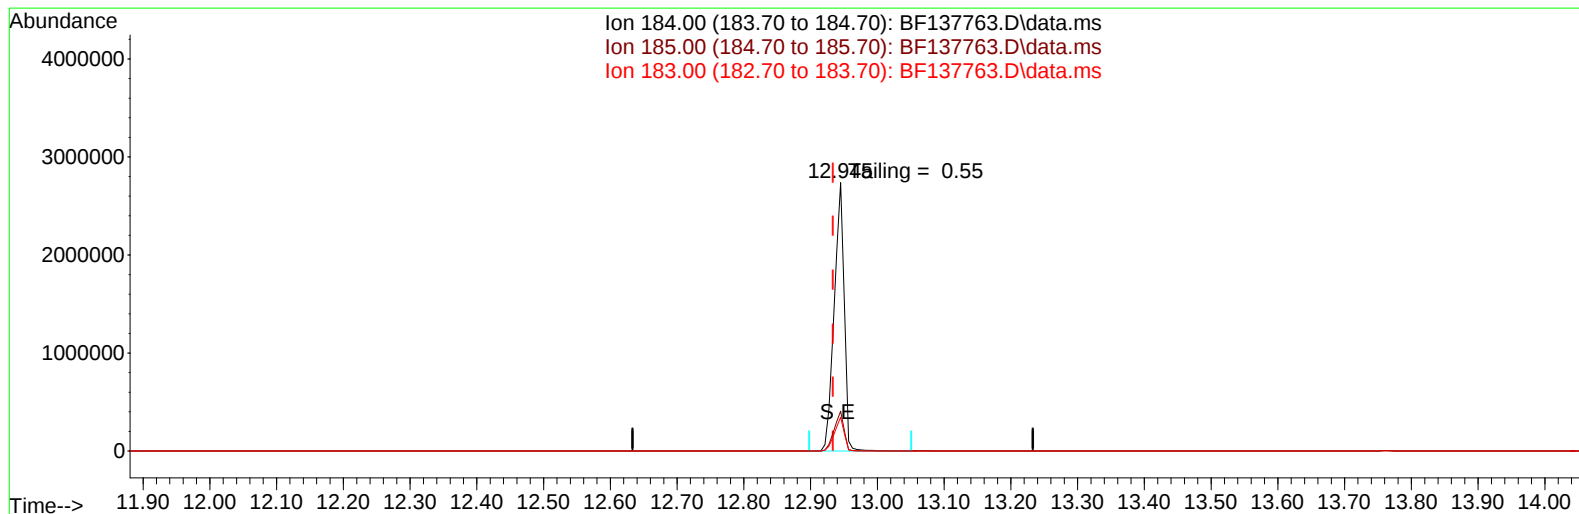

TIC: BF137763.D\data.ms

(77) Benzidine**12.945min (+ 0.012) 515509.87 ng****response 2873337**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.40	14.87
183.00	11.50	12.60
0.00	0.00	0.00