

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF043024\
 Data File : BF137781.D
 Acq On : 30 Apr 2024 20:35
 Operator : CG\JU
 Sample : P2310-03 5X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SU-03-042924

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF137781.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.381	46	50	59	rVB	52639	73748	4.89%	0.581%
2	4.216	359	362	367	rVB	17551	21155	1.40%	0.167%
3	5.669	605	609	613	rBV	718927	584917	38.76%	4.607%
4	6.657	774	777	781	rBV	691250	578978	38.36%	4.560%
5	7.057	841	845	848	rBV	1556606	1177037	77.99%	9.271%
6	7.610	936	939	943	rBV	450903	357417	23.68%	2.815%
7	8.339	1059	1063	1067	rBV	1800796	1509164	100.00%	11.887%
8	9.410	1242	1245	1249	rBV	873489	746233	49.45%	5.878%
9	9.480	1255	1257	1261	rBV	24978	23227	1.54%	0.183%
10	10.016	1345	1348	1351	rVB	37520	29121	1.93%	0.229%
11	10.104	1359	1363	1366	rBV	1899552	1484441	98.36%	11.692%
12	10.186	1373	1377	1383	rVB5	15753	24521	1.62%	0.193%
13	10.516	1430	1433	1436	rVB	50239	38171	2.53%	0.301%
14	10.739	1466	1471	1473	rBV	22878	28167	1.87%	0.222%
15	10.892	1493	1497	1500	rBV	341173	305179	20.22%	2.404%
16	10.992	1511	1514	1522	rVB	52434	80994	5.37%	0.638%
17	11.439	1588	1590	1593	rBV	46882	37182	2.46%	0.293%
18	11.469	1593	1595	1598	rVV2	24612	23405	1.55%	0.184%
19	11.598	1613	1617	1620	rBV	1549230	1243566	82.40%	9.795%
20	11.622	1620	1621	1626	rVV	113525	67264	4.46%	0.530%
21	11.674	1627	1630	1633	rVV	25297	21825	1.45%	0.172%
22	11.869	1661	1663	1666	rBV	37996	27796	1.84%	0.219%
23	12.098	1699	1702	1705	rBV2	60324	58964	3.91%	0.464%
24	12.127	1705	1707	1711	rVB	26839	24660	1.63%	0.194%
25	12.216	1719	1722	1724	rBV2	31490	30106	1.99%	0.237%
26	12.280	1730	1733	1735	rBV	33990	27842	1.84%	0.219%
27	12.668	1794	1799	1804	rBV4	43291	70846	4.69%	0.558%
28	12.816	1821	1824	1829	rBV	284392	228662	15.15%	1.801%
29	13.045	1857	1863	1869	rBV	227893	296595	19.65%	2.336%
30	13.180	1883	1886	1889	rBV	690385	549187	36.39%	4.326%
31	13.374	1917	1919	1921	rVB	36465	24796	1.64%	0.195%
32	13.398	1921	1923	1925	rBV	31201	26391	1.75%	0.208%
33	13.439	1928	1930	1933	rVB	31858	24786	1.64%	0.195%
34	13.745	1979	1982	1985	rBV	46911	49501	3.28%	0.390%
35	14.251	2063	2068	2071	rBV	1454108	1436095	95.16%	11.311%
36	14.274	2071	2072	2075	rVB	110403	63155	4.18%	0.497%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF043024\
Data File : BF137781.D
Acq On : 30 Apr 2024 20:35
Operator : CG\JU
Sample : P2310-03 5X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SU-03-042924

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	14.392	2089	2092	2094	rBV	71677	75125	4.98%	0.592%
38	15.827	2331	2336	2346	rVB	880464	1225892	81.23%	9.656%




Sum of corrected areas: 12696111

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF043024\
Data File : BF137781.D
Acq On : 30 Apr 2024 20:35
Operator : CG\JU
Sample : P2310-03 5X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SU-03-042924

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

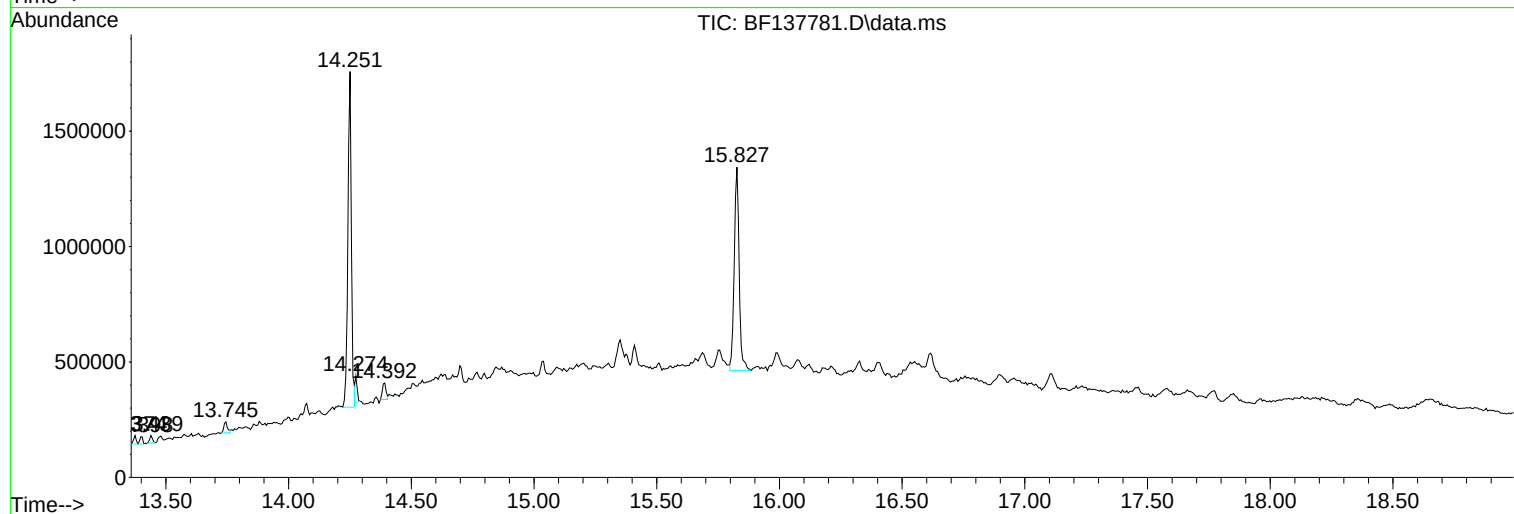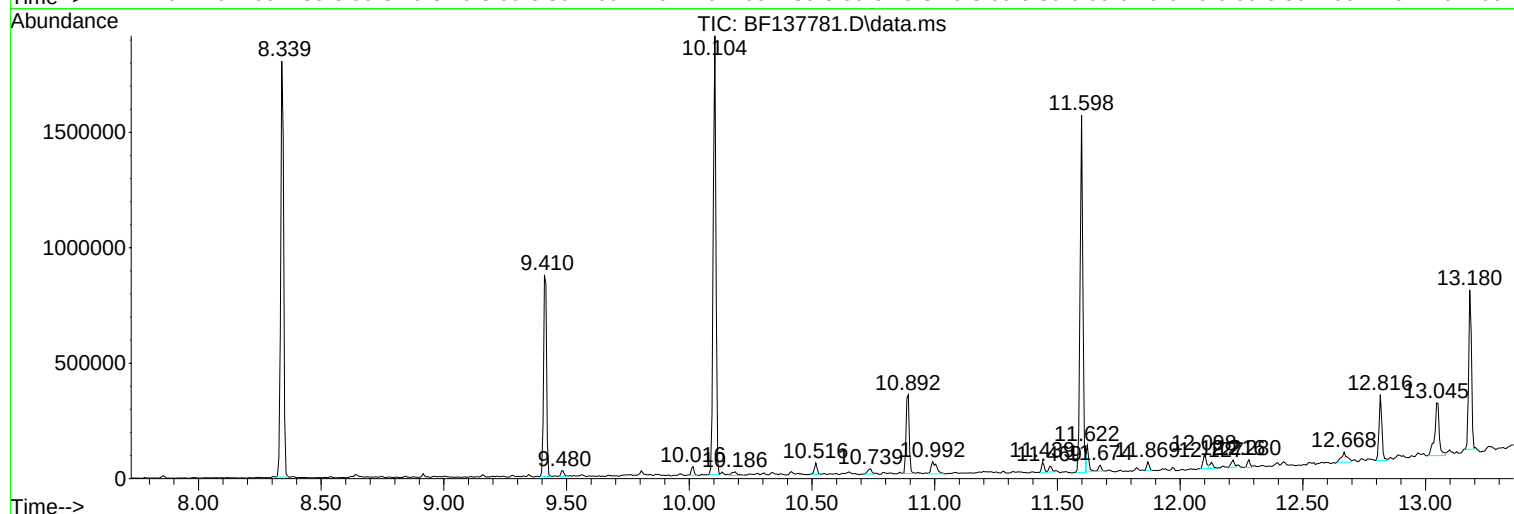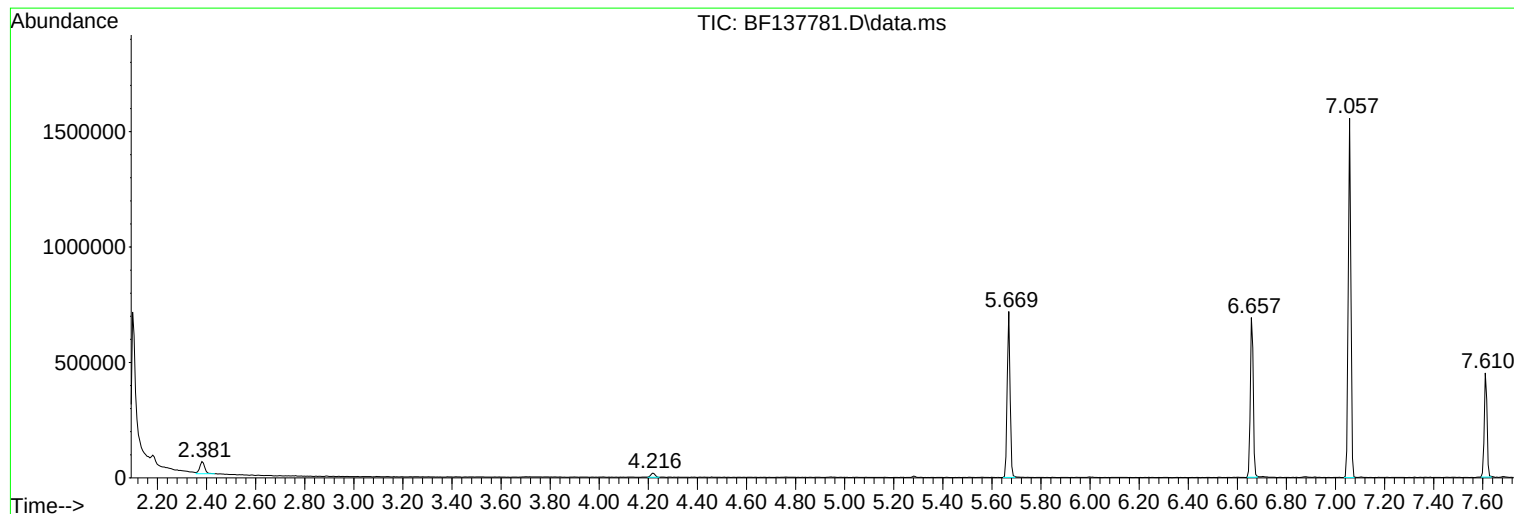

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF043024\
Data File : BF137781.D
Acq On : 30 Apr 2024 20:35
Operator : CG\JU
Sample : P2310-03 5X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SU-03-042924

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF043024\
Data File : BF137781.D
Acq On : 30 Apr 2024 20:35
Operator : CG\JU
Sample : P2310-03 5X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SU-03-042924

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------